


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025072.D
Acq On : 26 Feb 2020 08:41
Operator : CG/JU
Sample : L1541-16
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Feb 26 11:32:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD84

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:29 PM

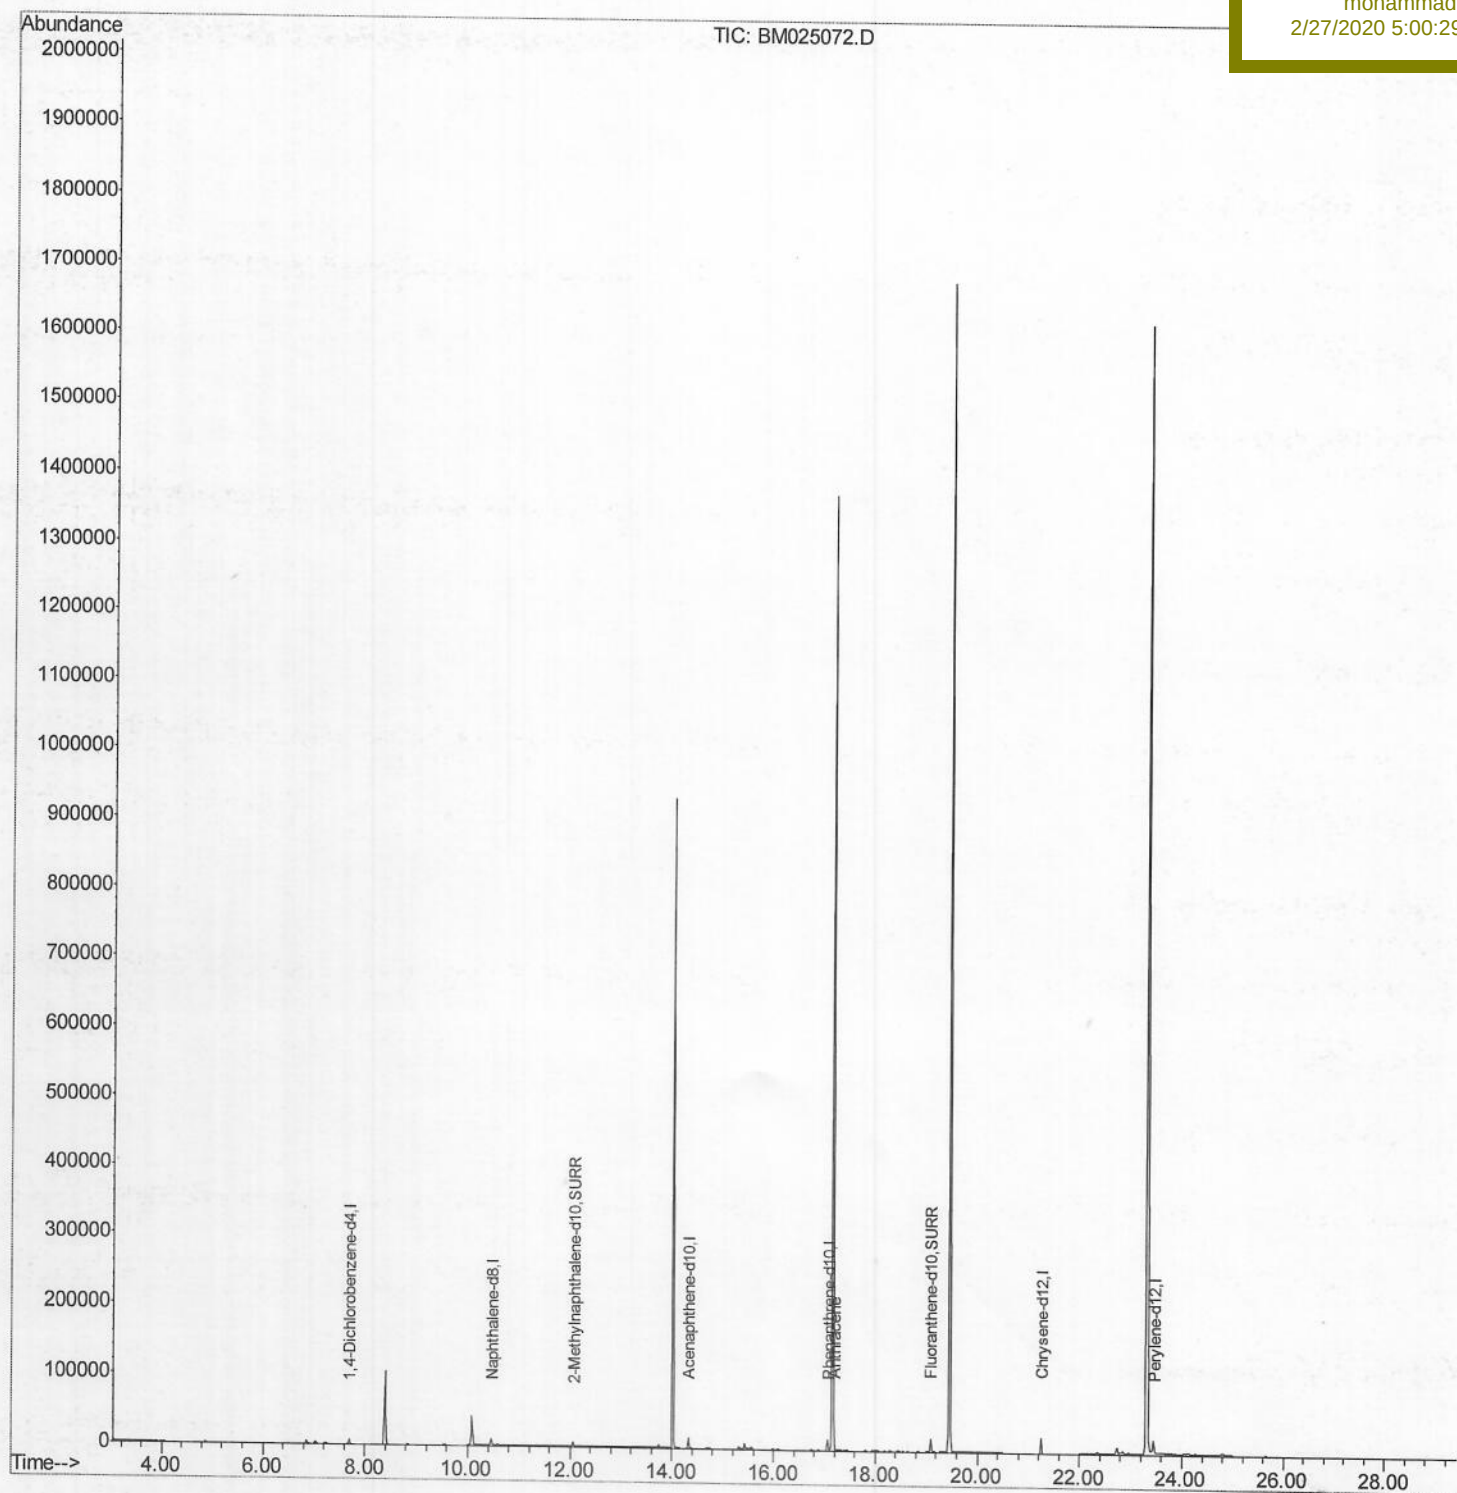

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025072.D

Acq On : 26 Feb 2020 08:41

Operator : CG/JU

Sample : L1541-16

Misc :

ALS Vial : 36 Sample Multiplier: 1

Quant Time: Feb 26 11:31:09 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBD84

Manual Integrations

APPROVED

mohammad

2/27/2020 5:00:29 PM

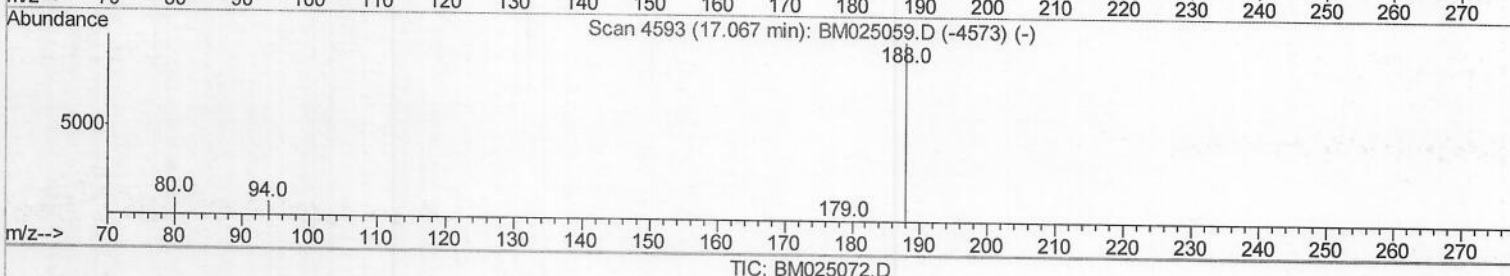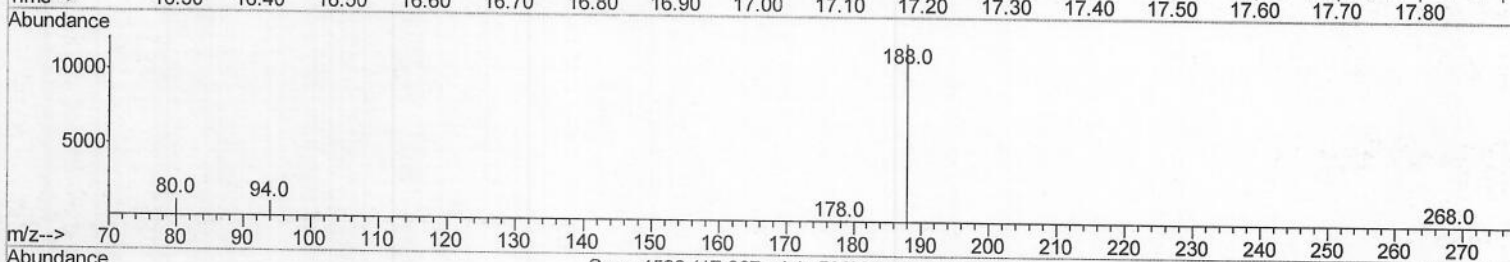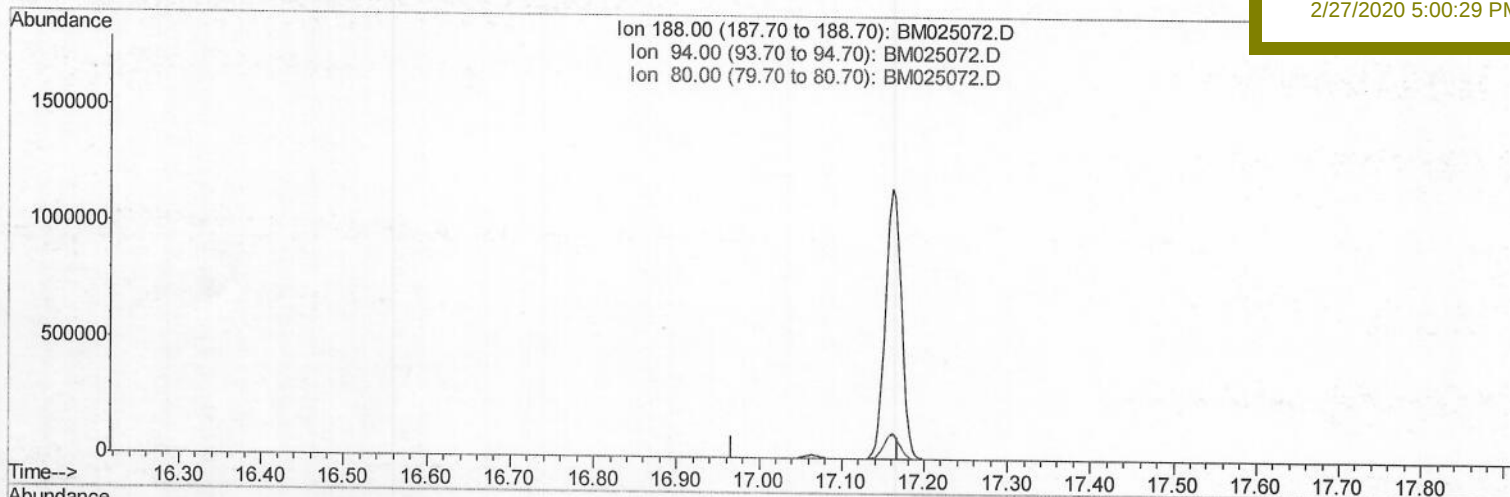

TIC: BM025072.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025072.D

Acq On : 26 Feb 2020 08:41

Operator : CG/JU

Sample : L1541-16

Misc :

ALS Vial : 36 Sample Multiplier: 1

Quant Time: Feb 26 11:31:09 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020




Response via : Initial Calibration

Instrument :

BNA_M

ClientSampled :

DBD84

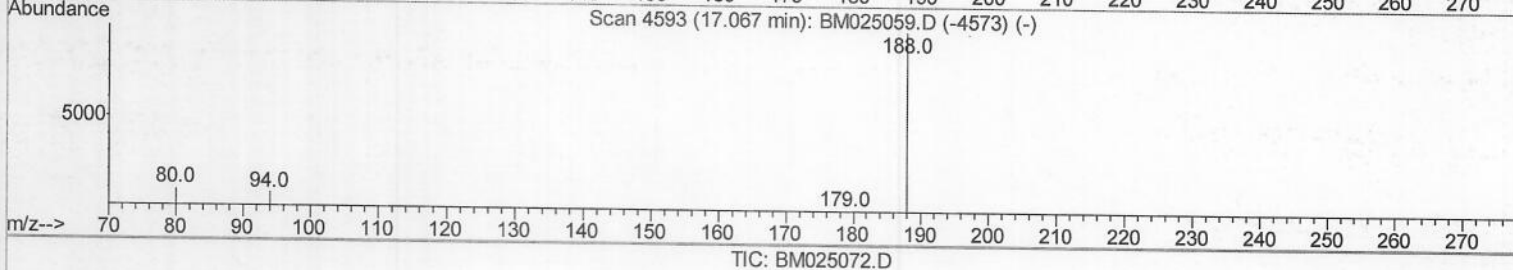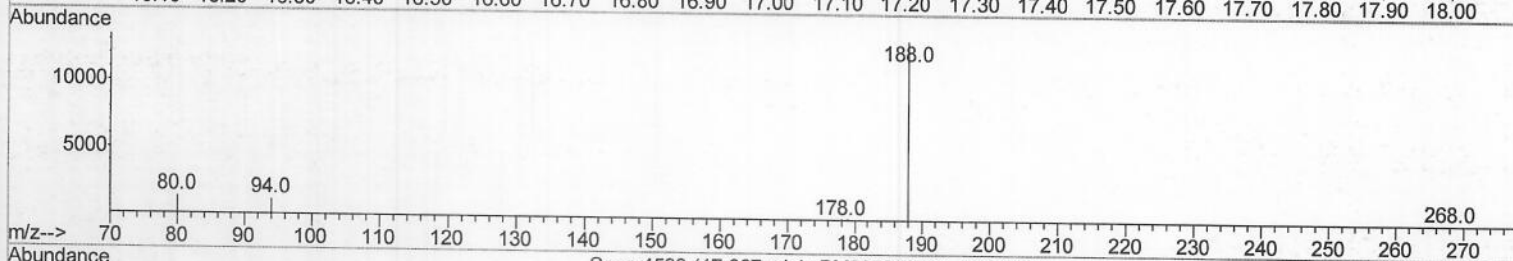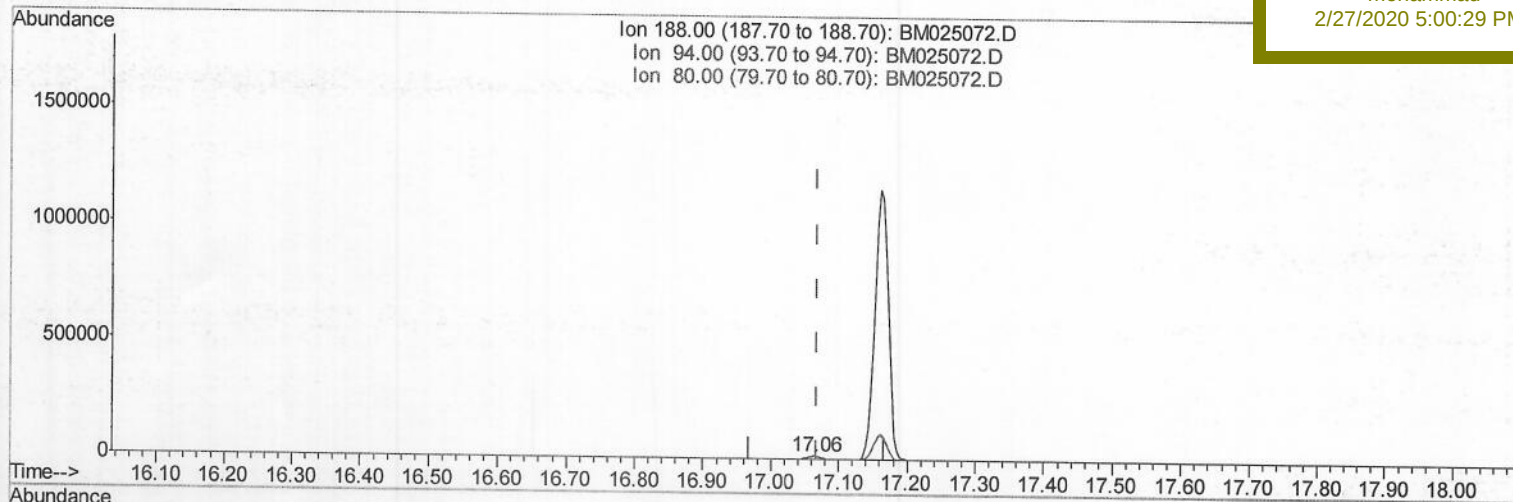Manual Integrations
APPROVEDmohammad
2/27/2020 5:00:29 PM

(10) Phenanthrene-d10 (I)

17.064min (-0.004) 0.40ng/ul m> JV 02/27/20

response 18361

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.64#
80.00	22.60	10.21#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
 Data File : BM025072.D
 Acq On : 26 Feb 2020 08:41
 Operator : CG/JU
 Sample : L1541-16
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD84

Quant Time: Feb 26 11:32:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 2/27/2020 5:00:29 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	3011	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	12044	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.32	164	7947	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	18361m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	19442	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	22521	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	6880	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	20912	0.33	ng/ul	0.00
Target Compounds						
13) Anthracene	17.20	178	1276	0.020	ng/ul#	85

(#) = qualifier out of range (m) = manual integration (+) = signals summed