

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025075.D
Acq On : 26 Feb 2020 10:30
Operator : CG/JU
Sample : L1541-19
Misc :
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Feb 26 11:36:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :


DBD90

Manual Integrations

APPROVED

mohammad

2/27/2020 5:00:23 PM

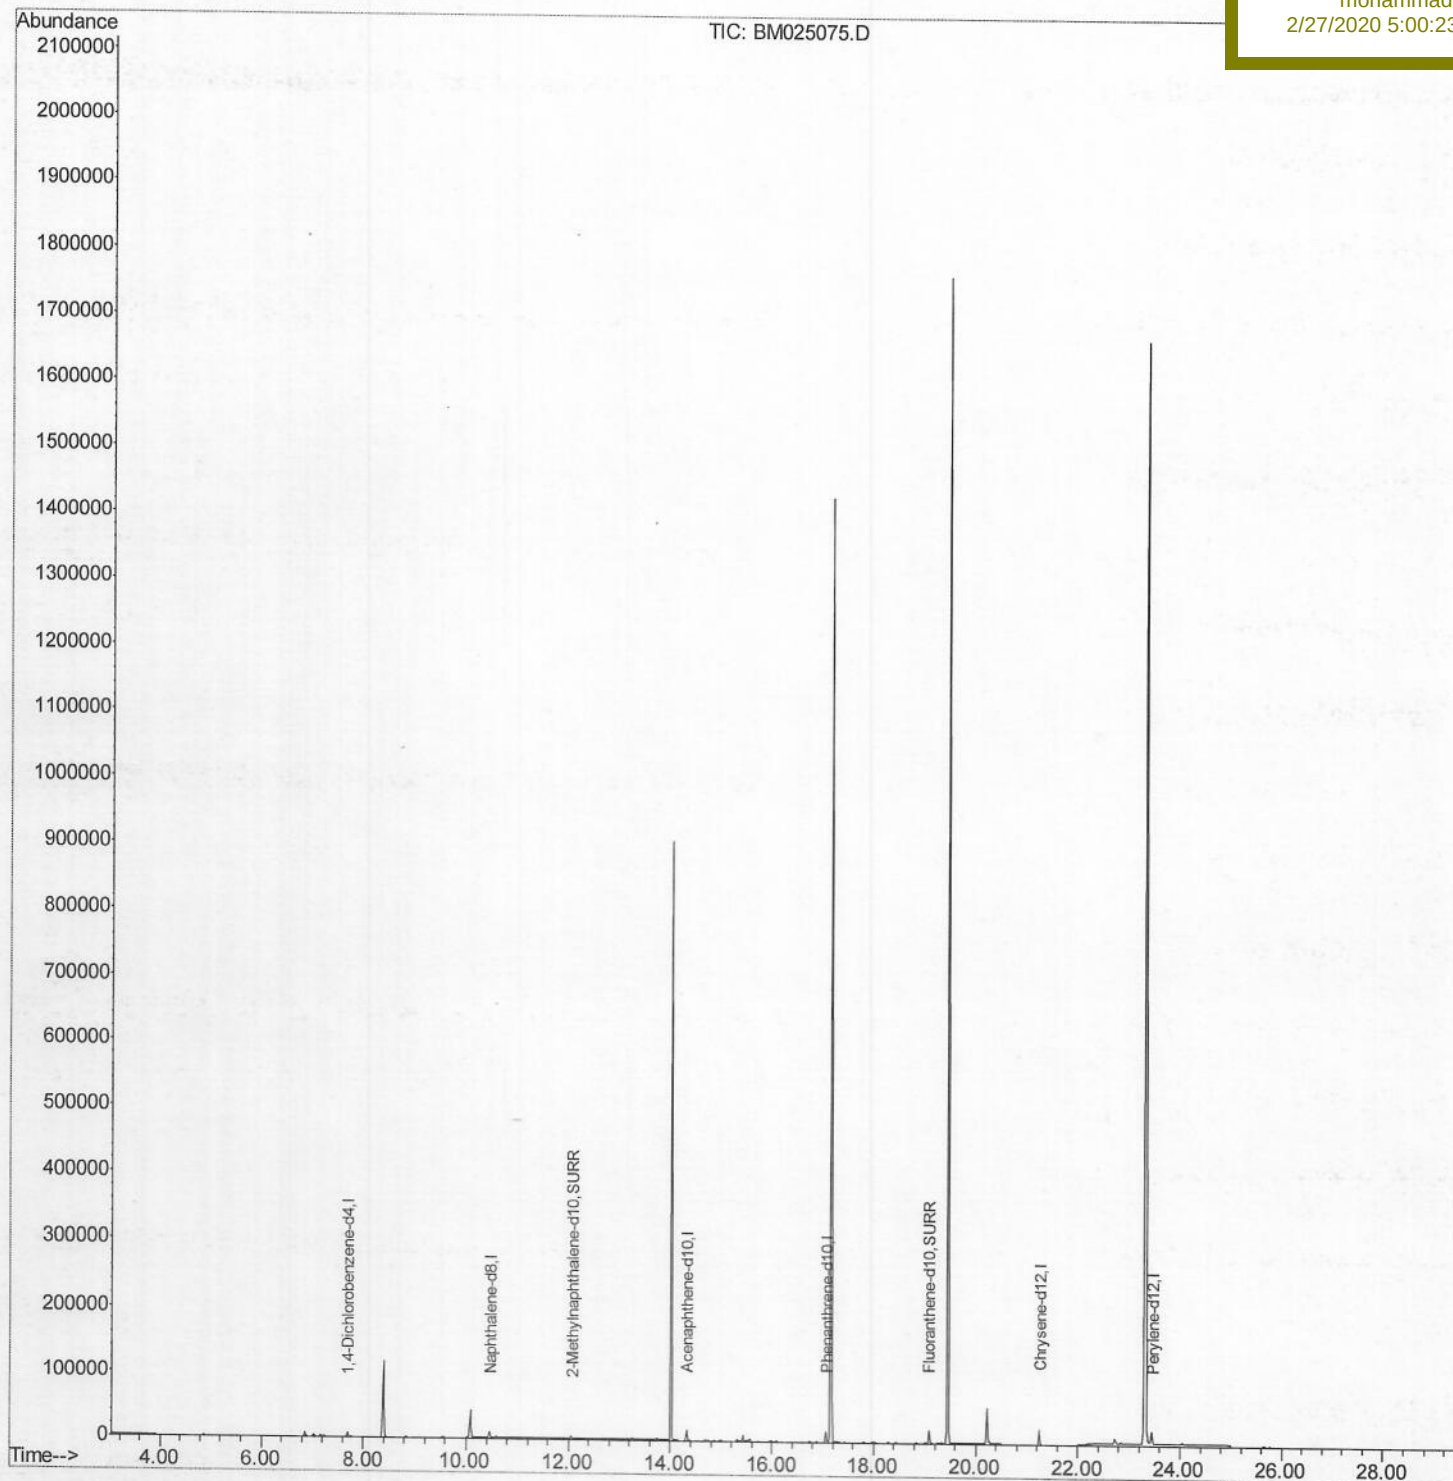

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
 Data File : BM025075.D
 Acq On : 26 Feb 2020 10:30
 Operator : CG/JU
 Sample : L1541-19
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Quant Time: Feb 26 11:35:27 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 DBD90

Manual Integrations
 APPROVED

mohammad
 2/27/2020 5:00:23 PM

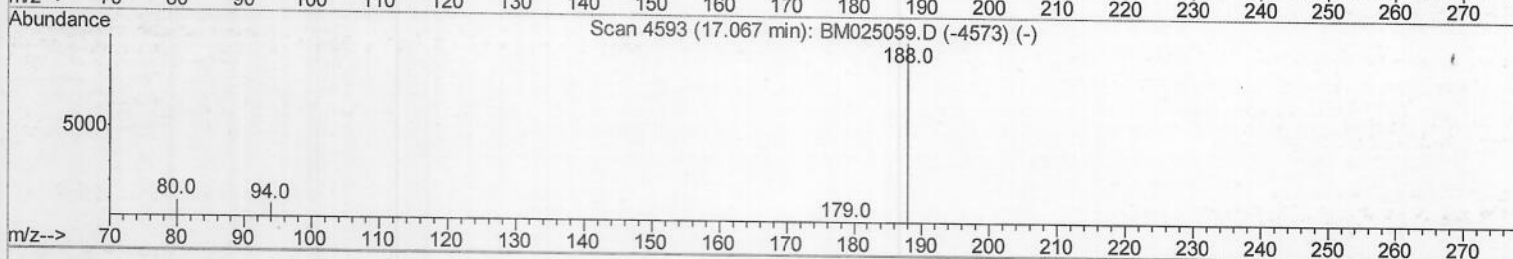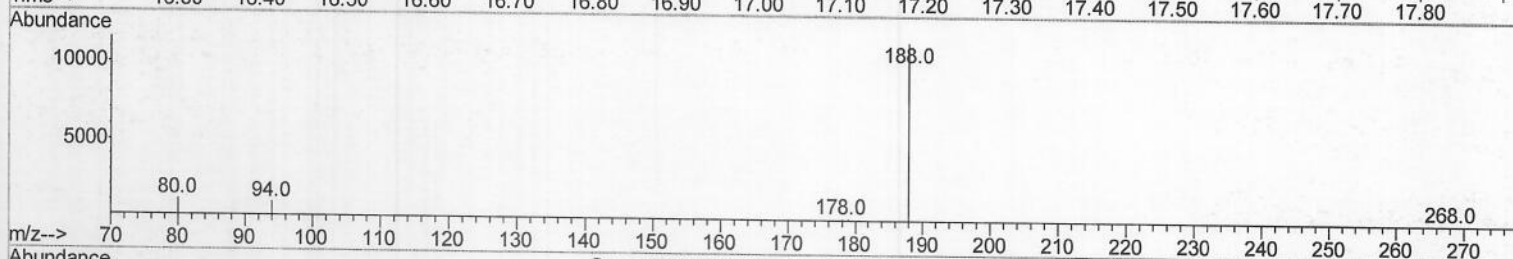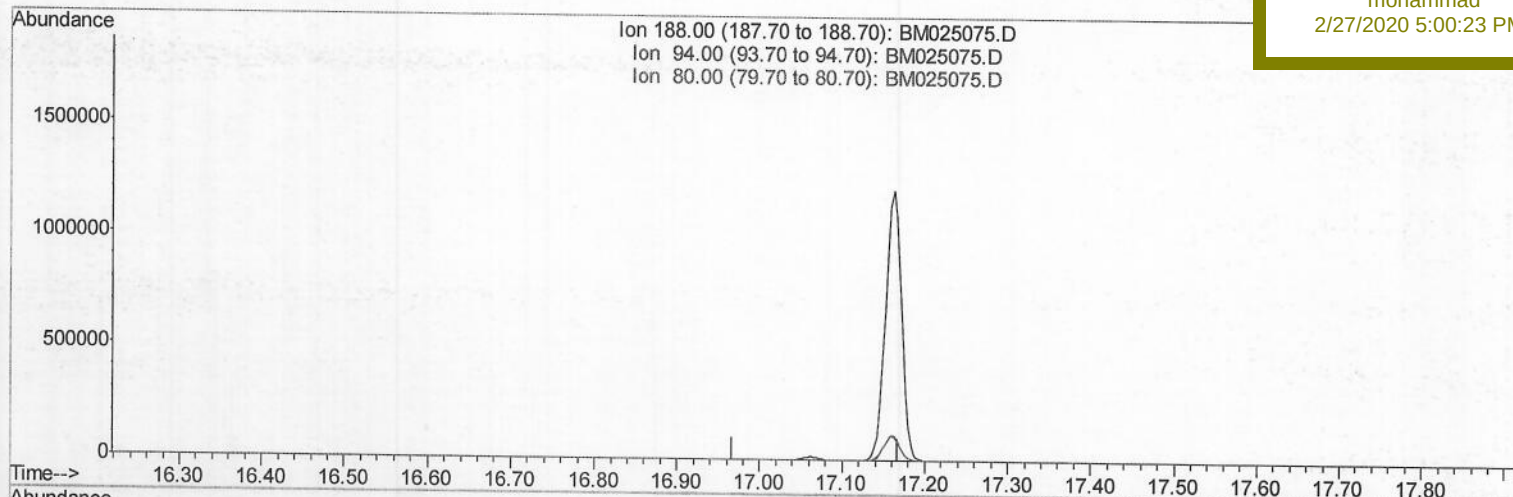

TIC: BM025075.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025075.D

Acq On : 26 Feb 2020 10:30

Operator : CG/JU

Sample : L1541-19

Misc :

ALS Vial : 39 Sample Multiplier: 1

Quant Time: Feb 26 11:35:27 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBD90

Manual Integrations

APPROVED

mohammad

2/27/2020 5:00:23 PM

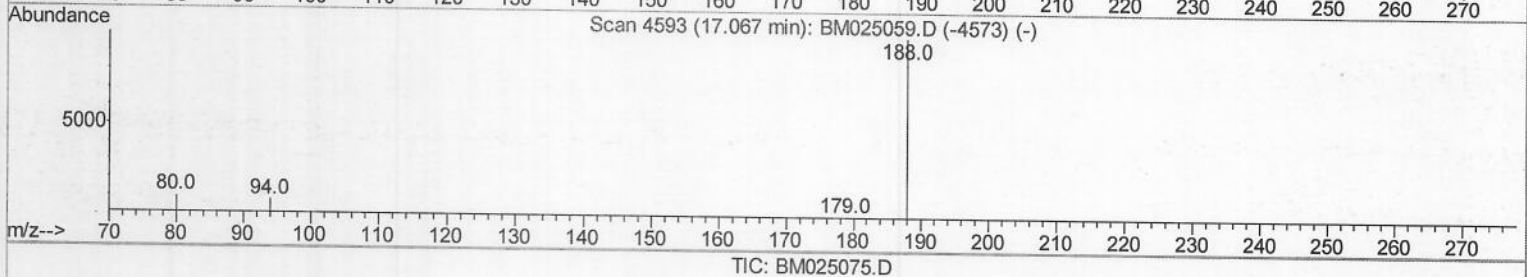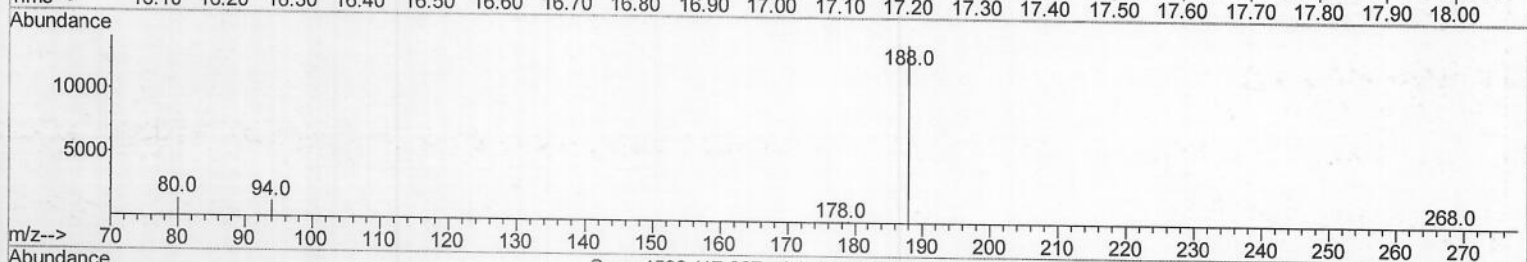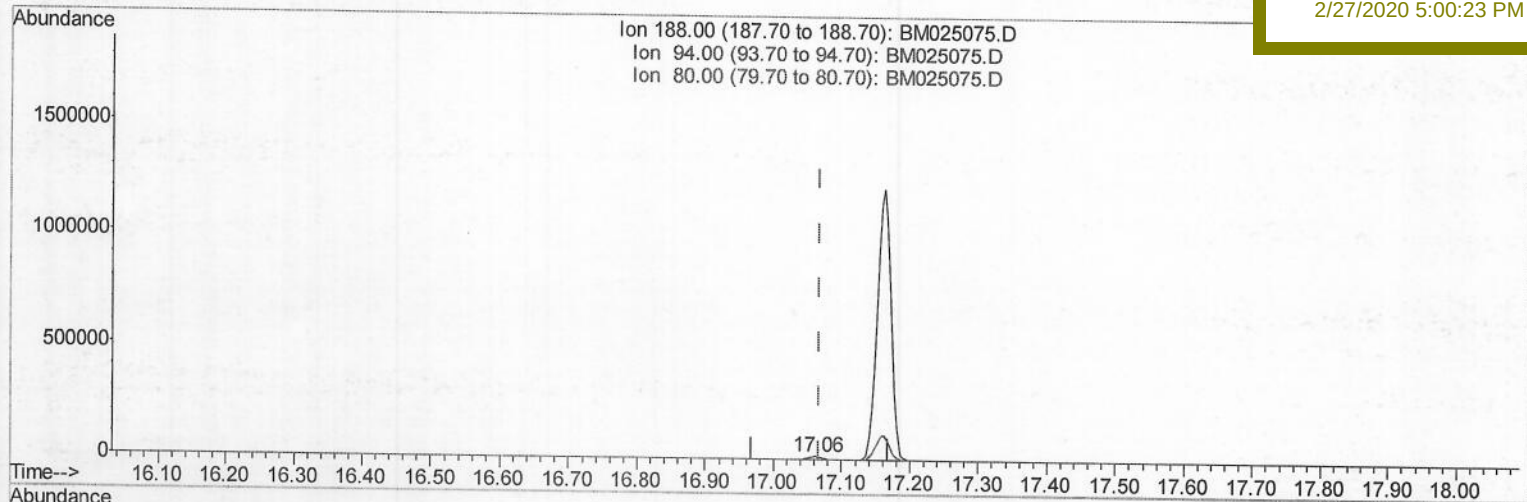

(10) Phenanthrene-d10 (I)

17.062min (-0.006) 0.40ng/ul m > JV 02/27/20

response 19273

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	9.07#
80.00	22.60	10.09#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025075.D
Acq On : 26 Feb 2020 10:30
Operator : CG/JU
Sample : L1541-19
Misc :
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Feb 26 11:36:14 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBD90

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:23 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	3248	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	12965	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	8457	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	19273m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	20677	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	23726	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	6806	0.28	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	22071	0.33	ng/ul	0.00

Target Compounds

(#) = qualifier out of range (m) = manual integration (+) = signals summed