


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025081.D
Acq On : 26 Feb 2020 15:50
Operator : CG/JU
Sample : PB126824BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Feb 26 16:29:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK24

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:50 PM

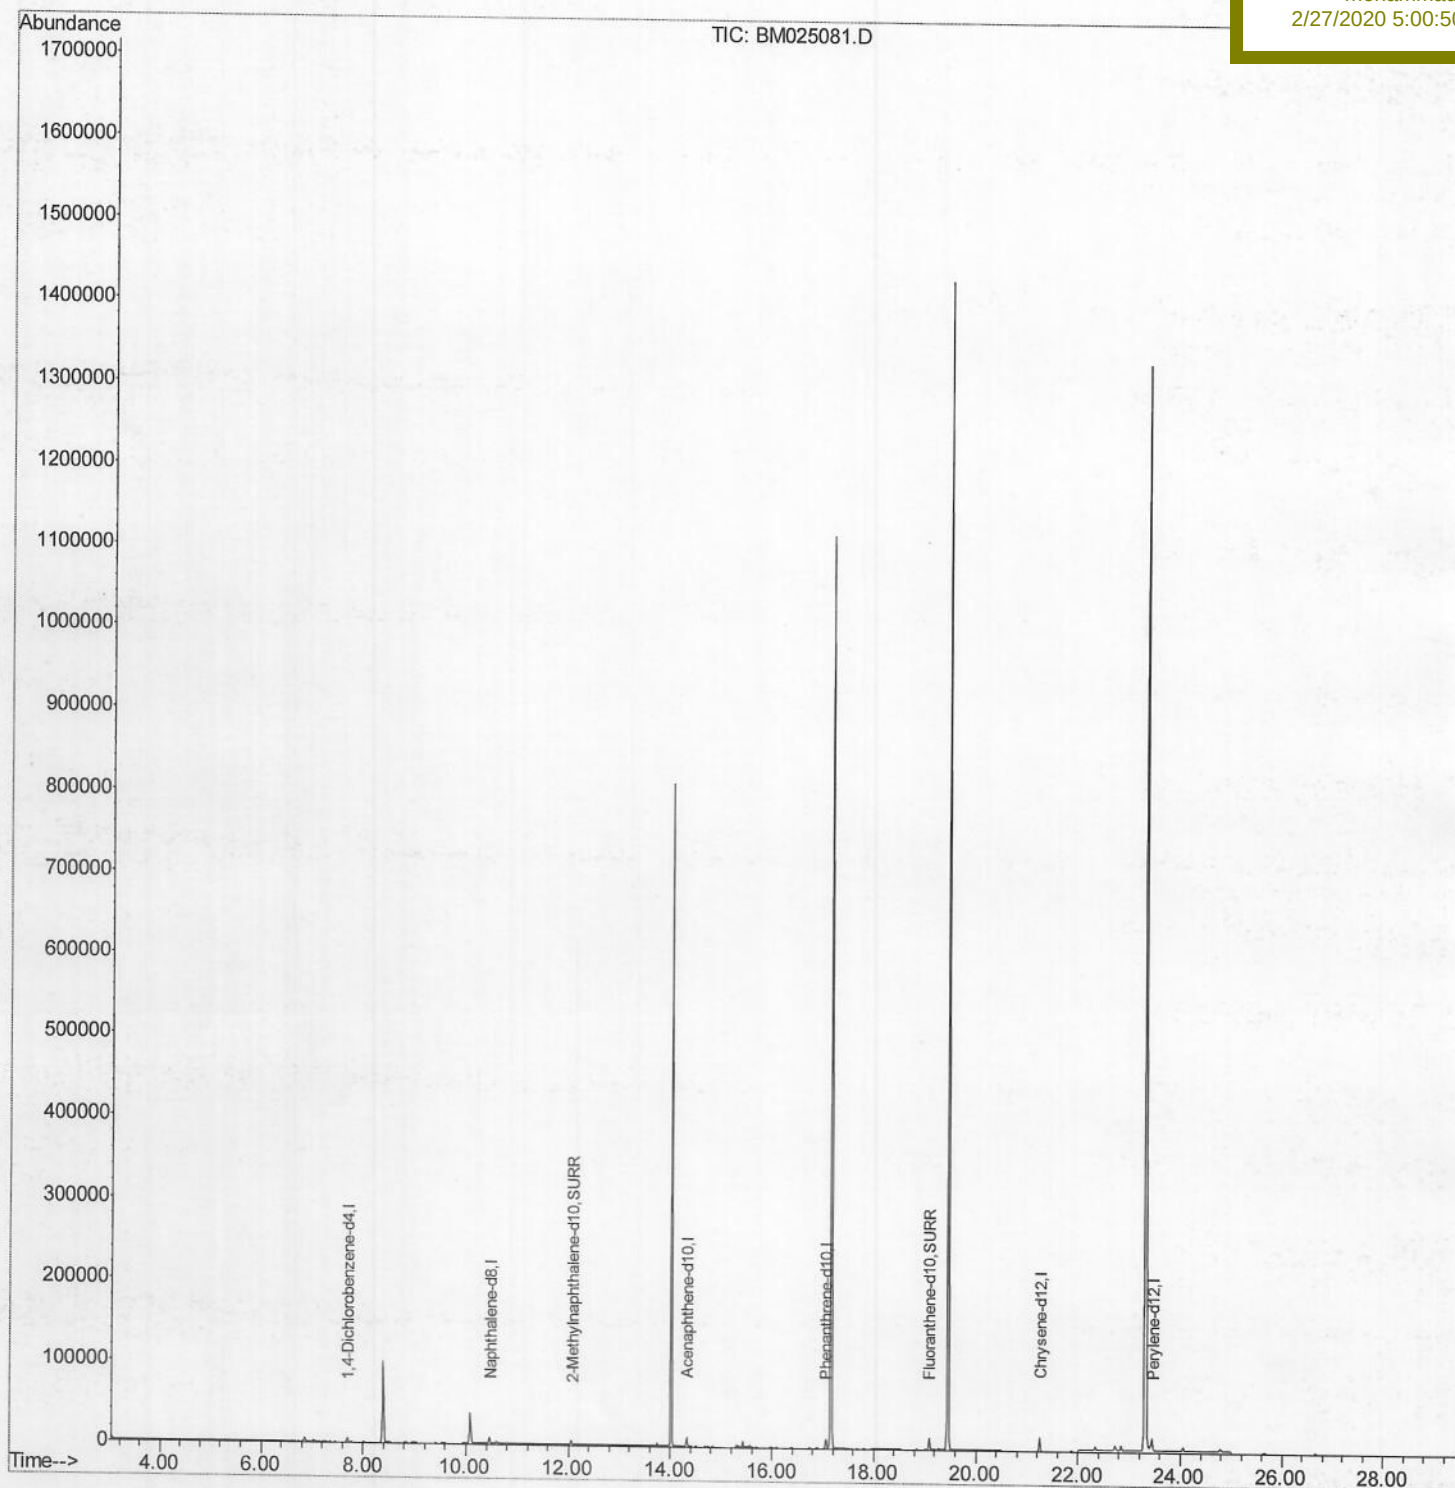

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\

Data File : BM025081.D

Acq On : 26 Feb 2020 15:50

Operator : CG/JU

Sample : PB126824BL

Misc :

ALS Vial : 45 Sample Multiplier: 1

Quant Time: Feb 26 16:28:23 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Feb 25 11:03:43 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK24

Manual Integrations

APPROVED

mohammad

2/27/2020 5:00:50 PM

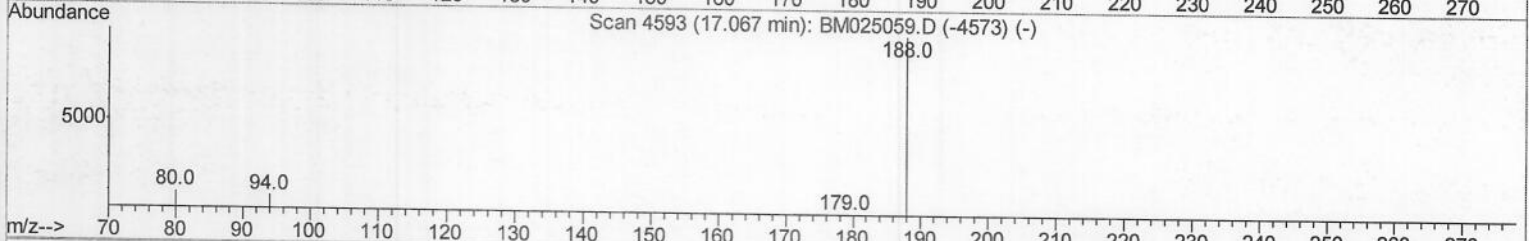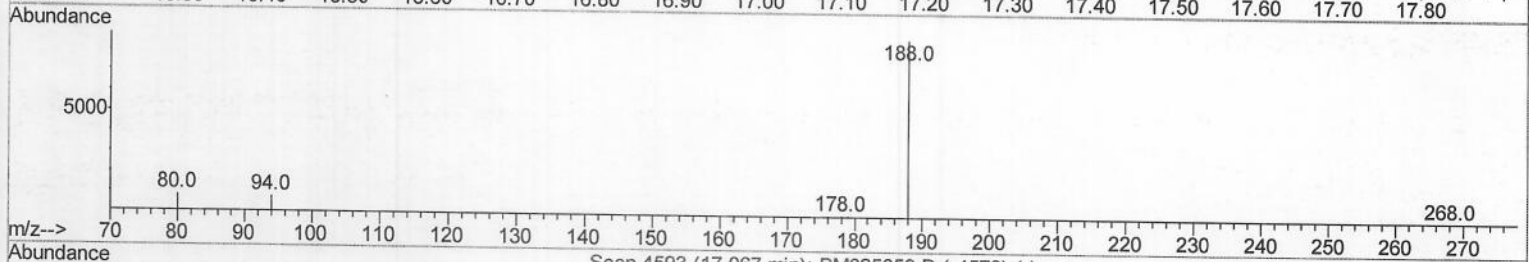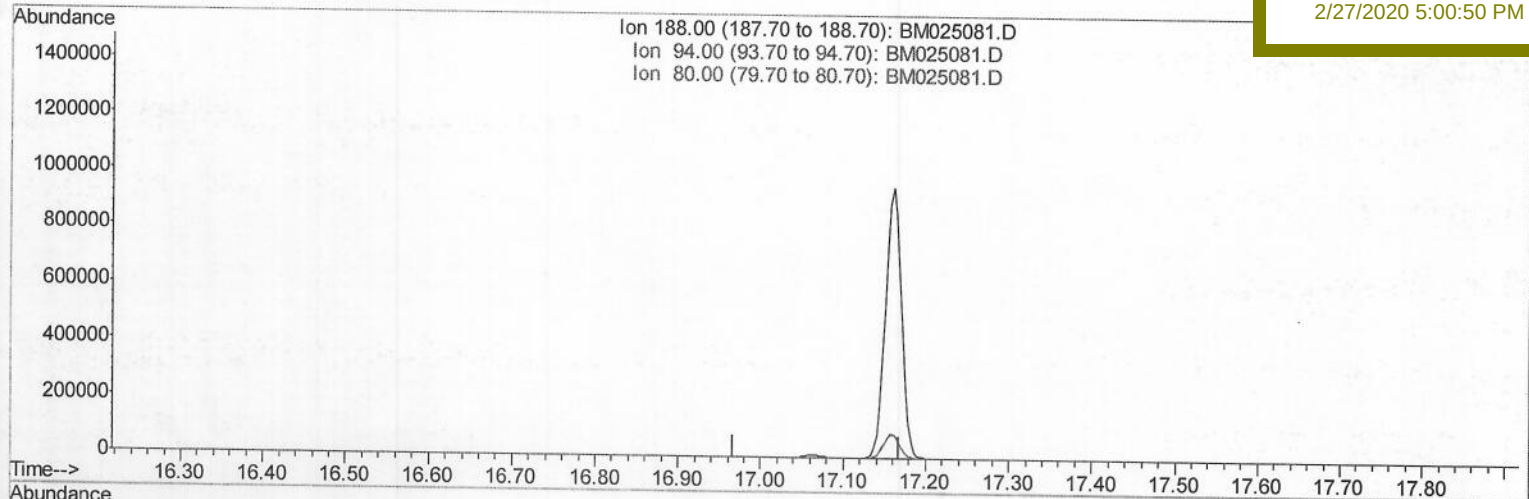

TIC: BM025081.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025081.D
Acq On : 26 Feb 2020 15:50
Operator : CG/JU
Sample : PB126824BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Feb 26 16:28:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK24

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:50 PM

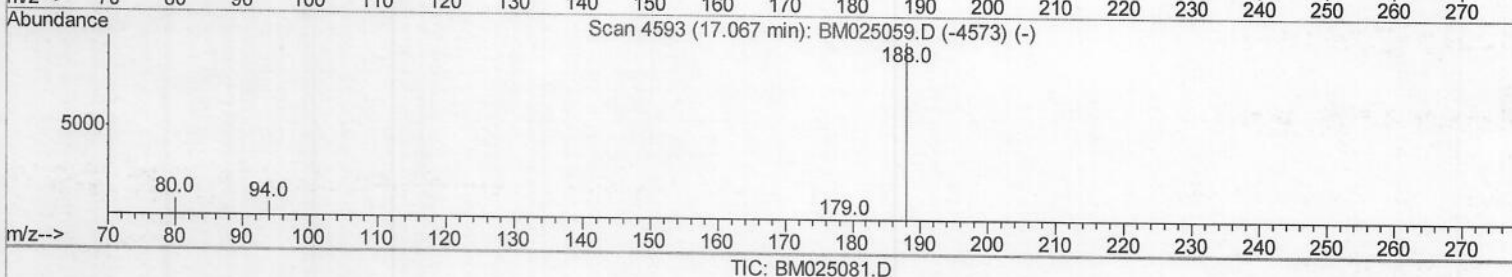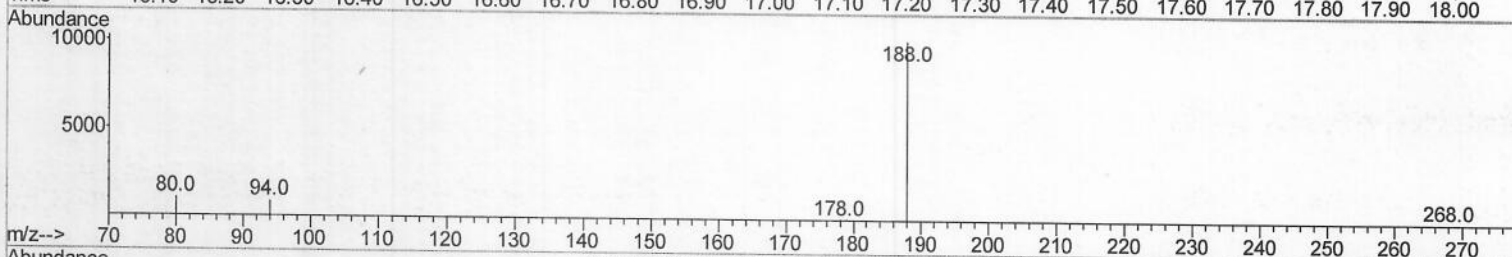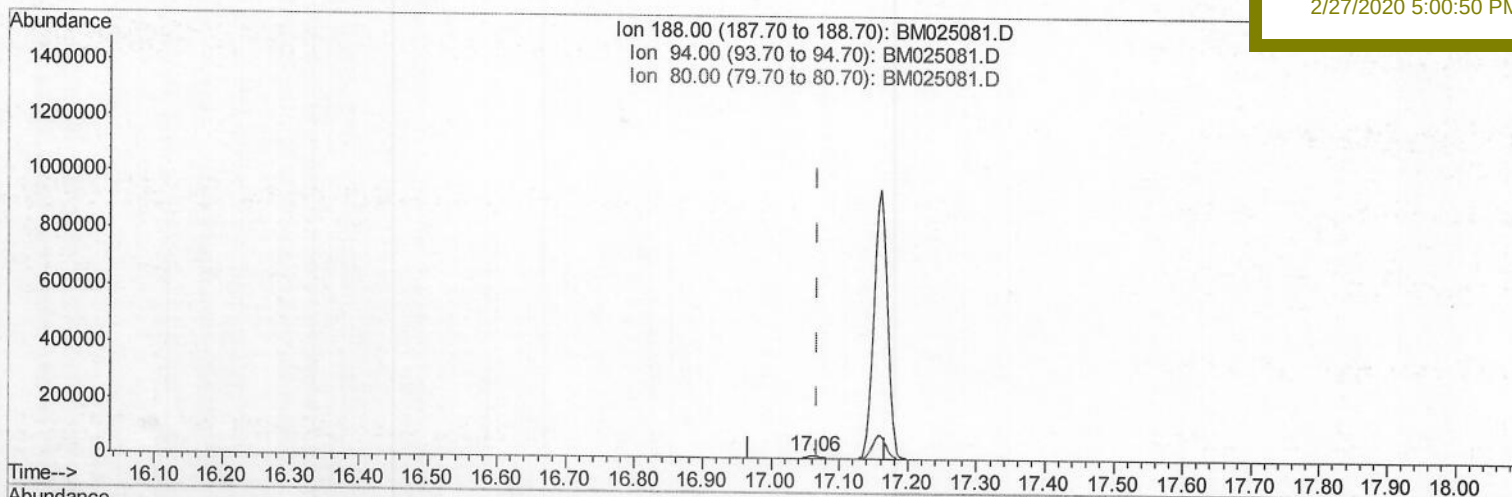

(10) Phenanthrene-d10 (I)

17.060min (-0.008) 0.40ng/ul m > JV 02/27/20

response 14126

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.77#
80.00	22.60	10.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022520\
Data File : BM025081.D
Acq On : 26 Feb 2020 15:50
Operator : CG/JU
Sample : PB126824BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Quant Time: Feb 26 16:29:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK24

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:50 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	2516	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	9790	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.32	164	6299	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	14126m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	14743	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	18208	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	6034	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	16159	0.33	ng/ul	0.00

Target Compounds

					Ovalue
--	--	--	--	--	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed