

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
 Data File : BM025053.D
 Acq On : 25 Feb 2020 20:40
 Operator : CG/JU
 Sample : L1486-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCX1

Manual Integrations
 APPROVED

mohammad
 2/26/2020 6:49:13 AM

Quant Time: Feb 26 00:05:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	2965	0.40	ng/ul	0.00
2) Naphthalene-d8	10.47	136	11621	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.33	164	7438	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	16300m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	16775	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	19110	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	5917	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	16399	0.29	ng/ul	0.00
Target Compounds						
13) Anthracene	17.20	178	1535	0.028	ng/ul#	Ovalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
Data File : BM025053.D
Acq On : 25 Feb 2020 20:40
Operator : CG/JU
Sample : L1486-19
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
DBCX1

Manual Integrations
APPROVED

mohammad
2/26/2020 6:49:13 AM

Quant Time: Feb 26 00:05:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

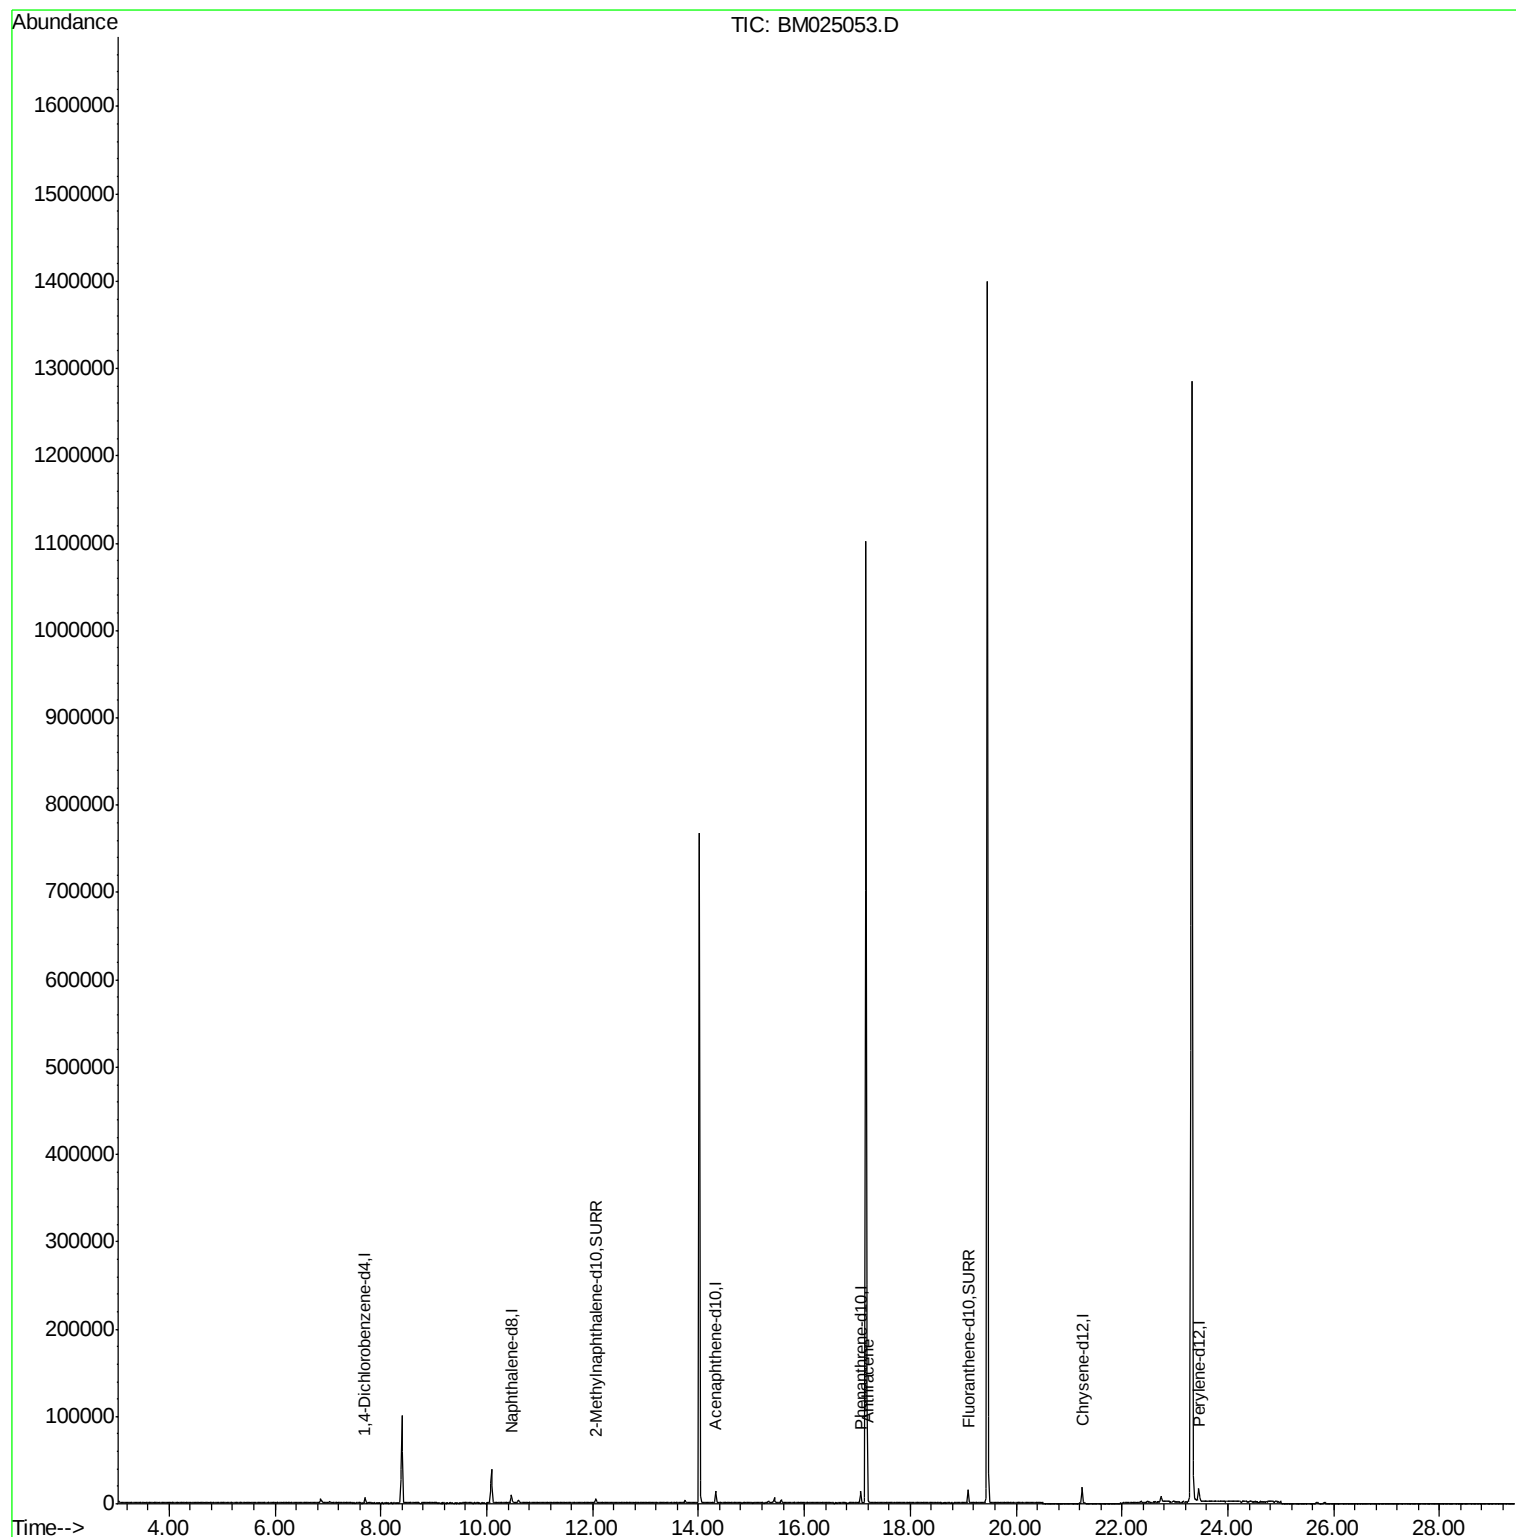

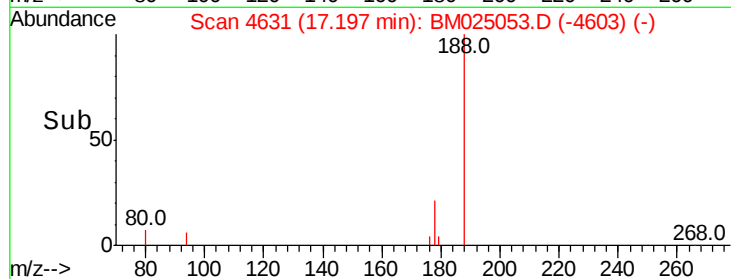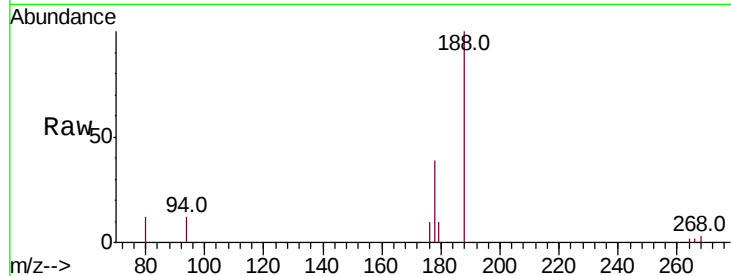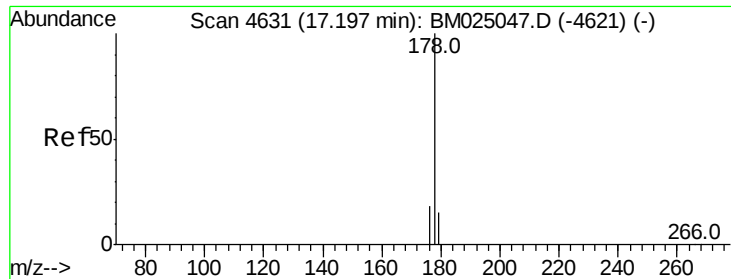

#13

Anthracene

Concen: 0.028 ng/ul

RT: 17.20 min Scan# 4631

Delta R.T. -0.00 min

Lab File: BM025053.D

Acq: 25 Feb 2020 20:40

Instrument :

BNA_M

ClientSampleId :

DBCX1

Tot Ion:	178	Resp:	1535
Ion Ratio	Lower	Upper	
178	100		
179	25.2	14.1	21.1#
176	24.3	16.2	24.4

Manual Integrations
APPROVED

mohammad
2/26/2020 6:49:13 AM

