

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
 Data File : BM025063.D
 Acq On : 26 Feb 2020 03:17
 Operator : CG/JU
 Sample : L1541-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD35

Manual Integrations
 APPROVED

mohammad
 2/27/2020 4:59:54 PM

Quant Time: Feb 26 04:25:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 26 03:38:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	3247	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	12814	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	8192	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	18571m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	19652	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	22764	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	5515	0.23	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	17282	0.27	ng/ul	0.00
Target Compounds						
11) Pentachlorophenol	16.72	266	147	0.026	ng/ul	Ovalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
Data File : BM025063.D
Acq On : 26 Feb 2020 03:17
Operator : CG/JU
Sample : L1541-07
Misc :
ALS Vial : 27 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
DBD35

Manual Integrations
APPROVED

mohammad
2/27/2020 4:59:54 PM

Quant Time: Feb 26 04:25:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 26 03:38:05 2020
Response via : Initial Calibration

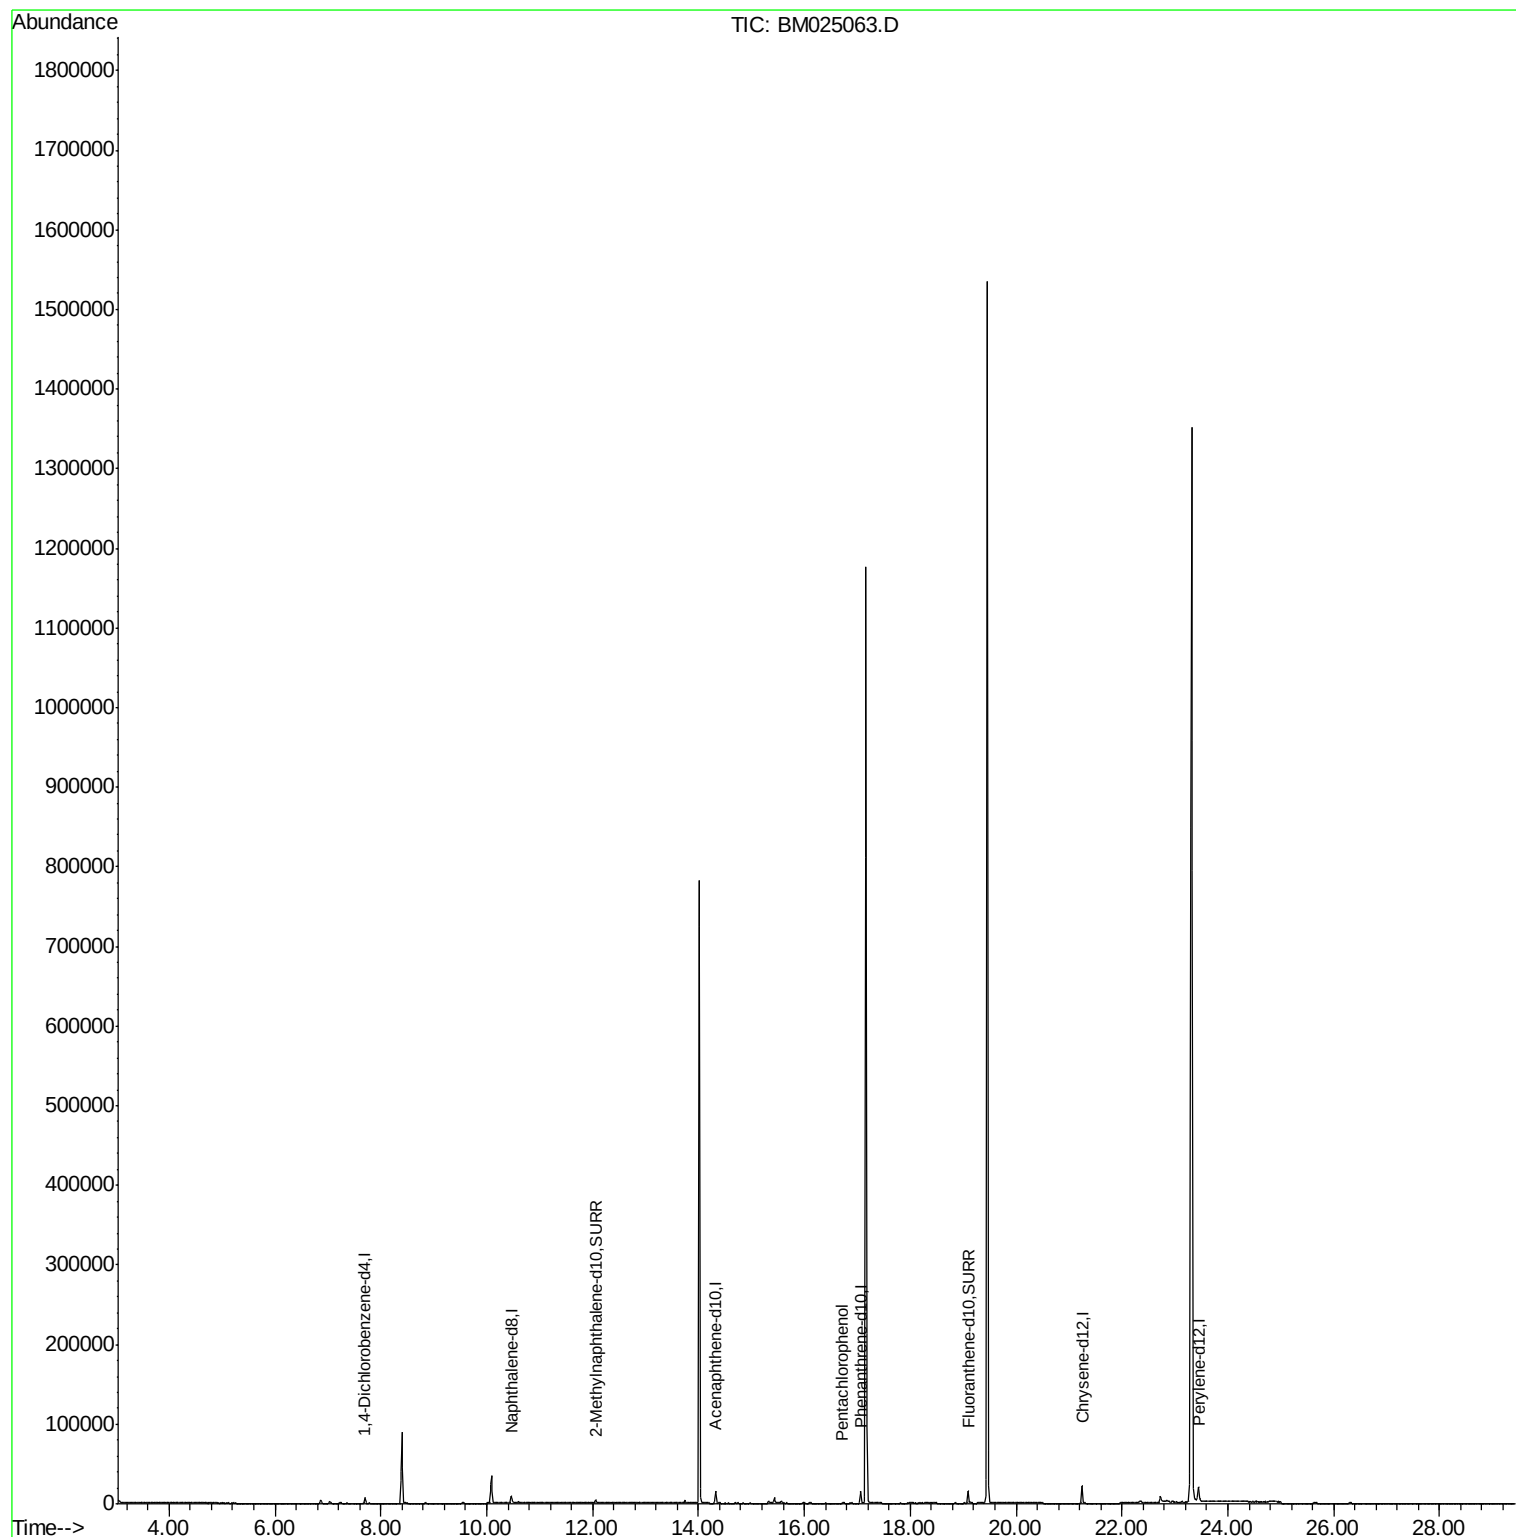

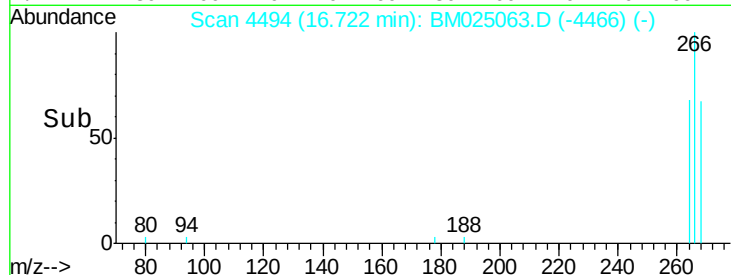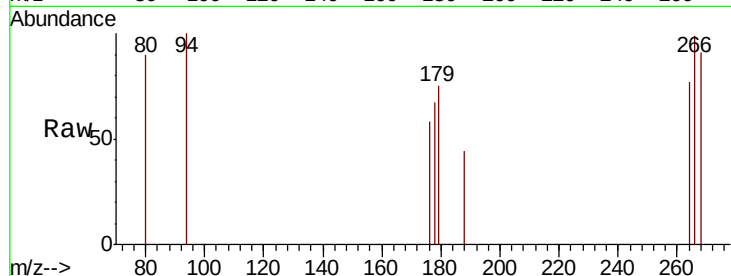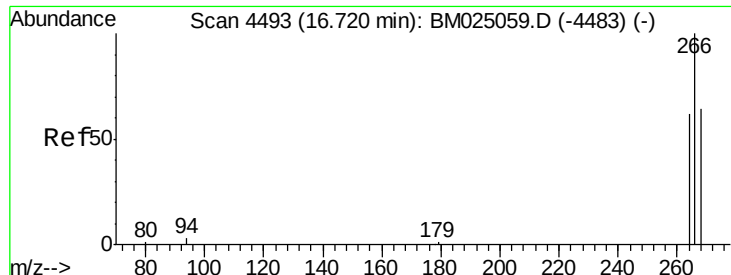

#11
 Pentachlorophenol
 Concen: 0.026 ng/ul
 RT: 16.72 min Scan# 4494
 Delta R.T. -0.00 min
 Lab File: BM025063.D
 Acq: 26 Feb 2020 03:17

Tot Ion:	266	Resp:	147
Ion Ratio	Lower	Upper	
266	100		
264	58.5	49.8	74.6
268	61.9	49.0	73.4

Instrument :
 BNA_M
 ClientSampleId :
 DBD35

Manual Integrations
 APPROVED

mohammad
 2/27/2020 4:59:54 PM

