

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
 Data File : BM025074.D
 Acq On : 26 Feb 2020 09:54
 Operator : CG/JU
 Sample : L1541-18
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD86

Manual Integrations
 APPROVED

mohammad
 2/27/2020 5:00:26 PM

Quant Time: Feb 26 11:35:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.70	152	3538	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	14072	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	9188	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.07	188	20751m	0.40	ng/ul	0.00
16) Chrysene-d12	21.25	240	22179	0.40	ng/ul	0.00
20) Perylene-d12	23.45	264	26557	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	7151	0.27	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	21260	0.30	ng/ul	0.00
Target Compounds						
13) Anthracene	17.20	178	5581	0.079	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
Data File : BM025074.D
Acq On : 26 Feb 2020 09:54
Operator : CG/JU
Sample : L1541-18
Misc :
ALS Vial : 38 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
DBD86

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:26 PM

Quant Time: Feb 26 11:35:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

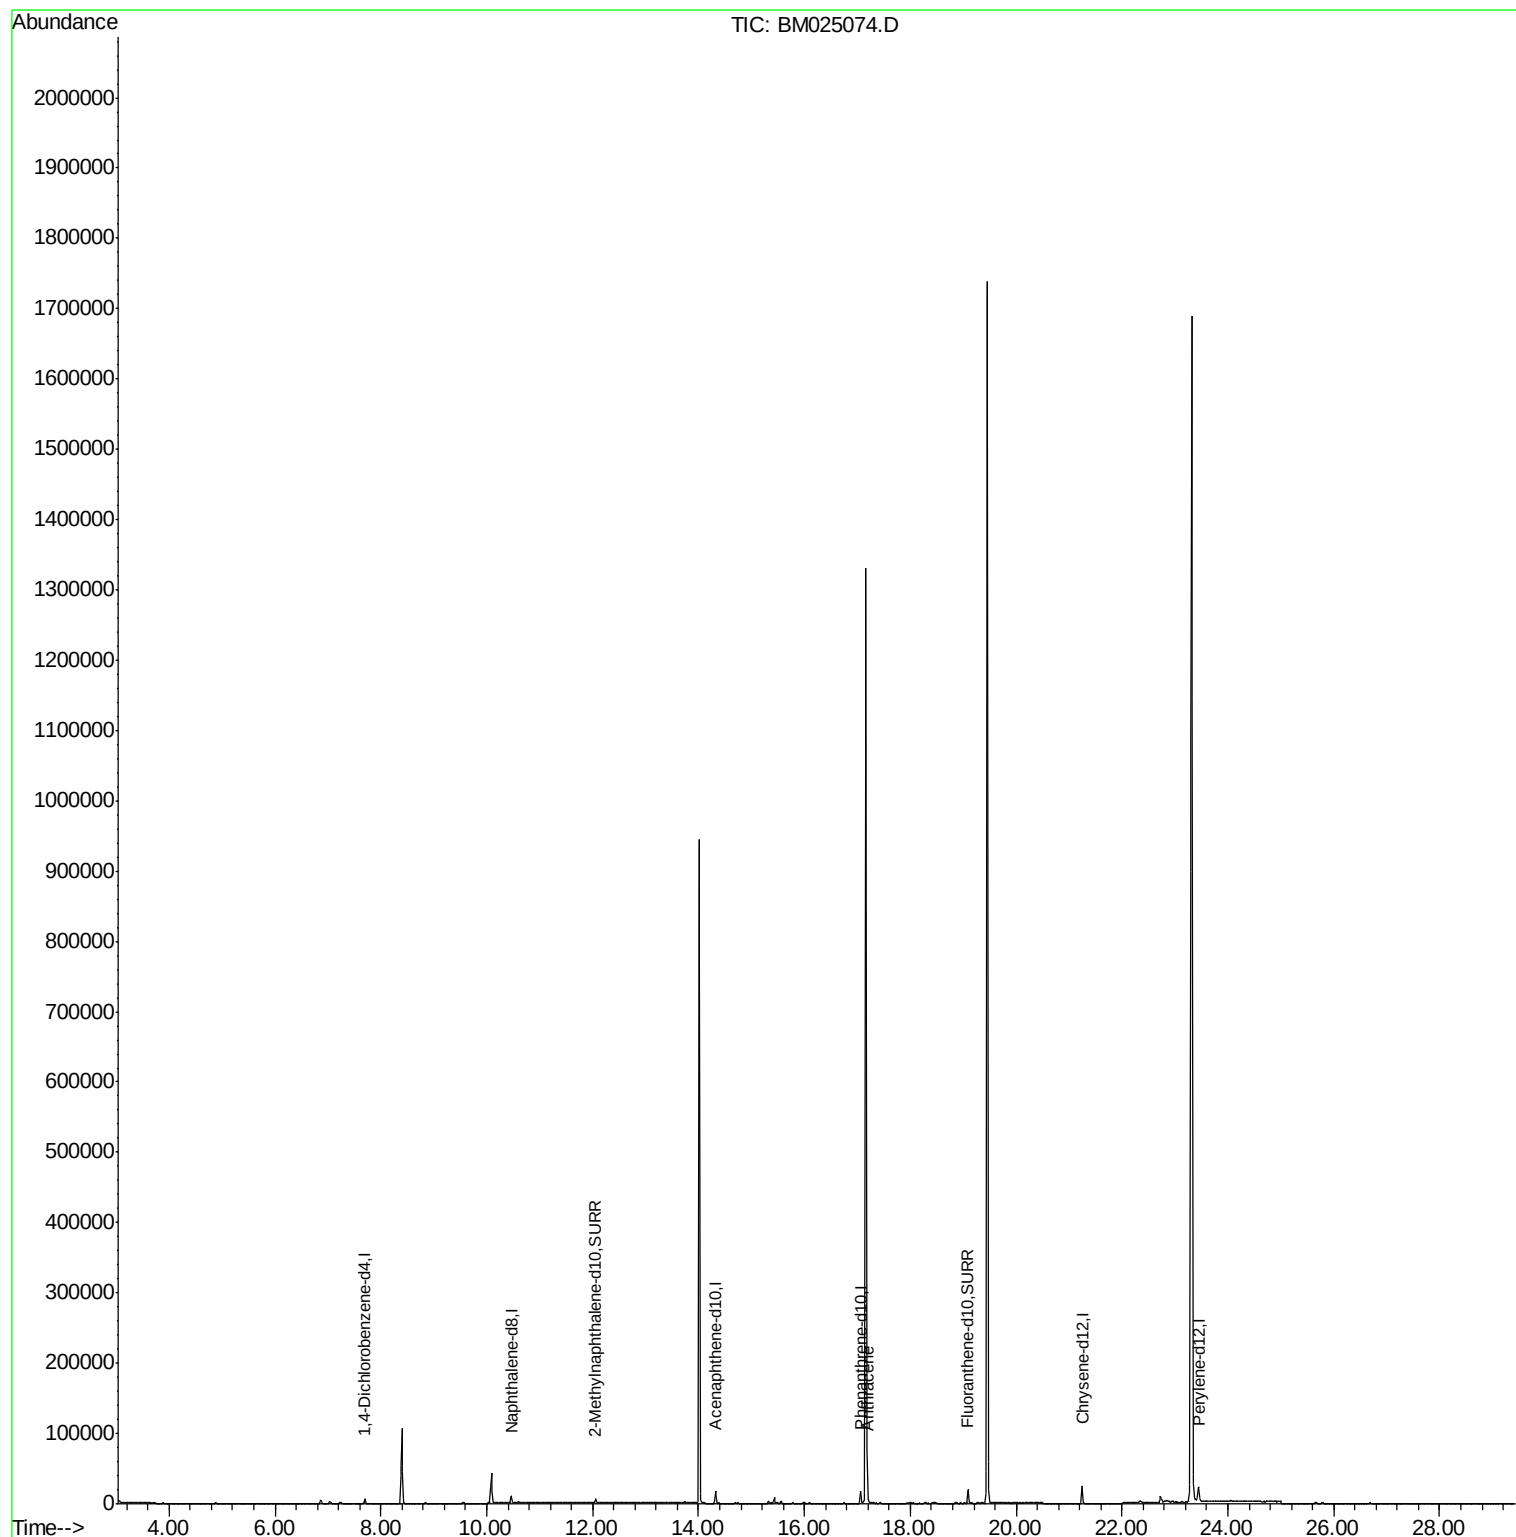

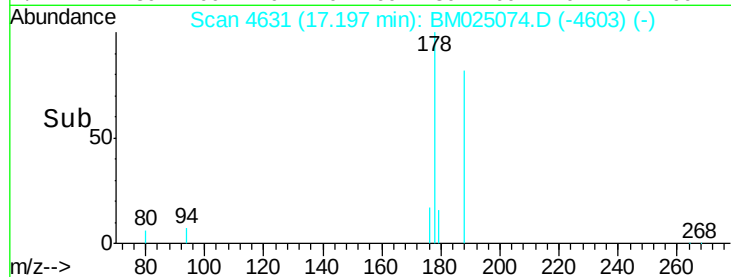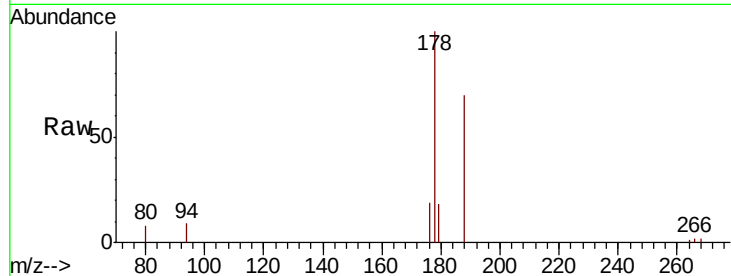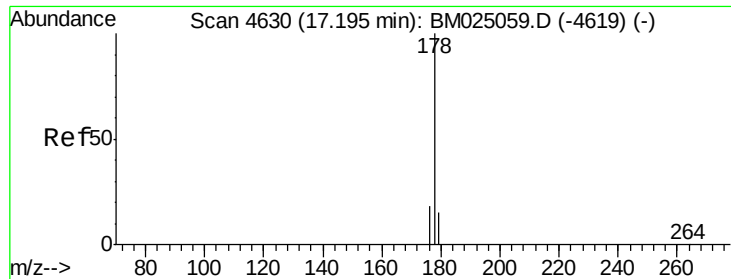

#13

Anthracene

Concen: 0.079 ng/ul

RT: 17.20 min Scan# 4631

Delta R.T. -0.00 min

Lab File: BM025074.D

Acq: 26 Feb 2020 09:54

Tot Ion:	178	Resp:	5581
Ion Ratio	Lower	Upper	
178	100		
179	18.0	14.1	21.1
176	18.8	16.2	24.4

Instrument :

BNA_M

ClientSampleId :

DBD86

Manual Integrations
APPROVED

mohammad
2/27/2020 5:00:26 PM

