

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
 Data File : BM025089.D
 Acq On : 26 Feb 2020 21:41
 Operator : CG/JU
 Sample : L1506-09
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCY7

Manual Integrations
 APPROVED

mohammad
 2/27/2020 5:01:11 PM

Quant Time: Feb 27 05:49:01 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 27 05:28:30 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2208	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	8720	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.32	164	5633	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	12472m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	13424	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	16097	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	6403	0.39	ng/ul	-0.01
14) Fluoranthene-d10	19.09	212	16764	0.39	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.10	178	929	0.021	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022520\
Data File : BM025089.D
Acq On : 26 Feb 2020 21:41
Operator : CG/JU
Sample : L1506-09
Misc :
ALS Vial : 53 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
DBCY7

Manual Integrations
APPROVED

mohammad
2/27/2020 5:01:11 PM

Quant Time: Feb 27 05:49:01 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 27 05:28:30 2020
Response via : Initial Calibration

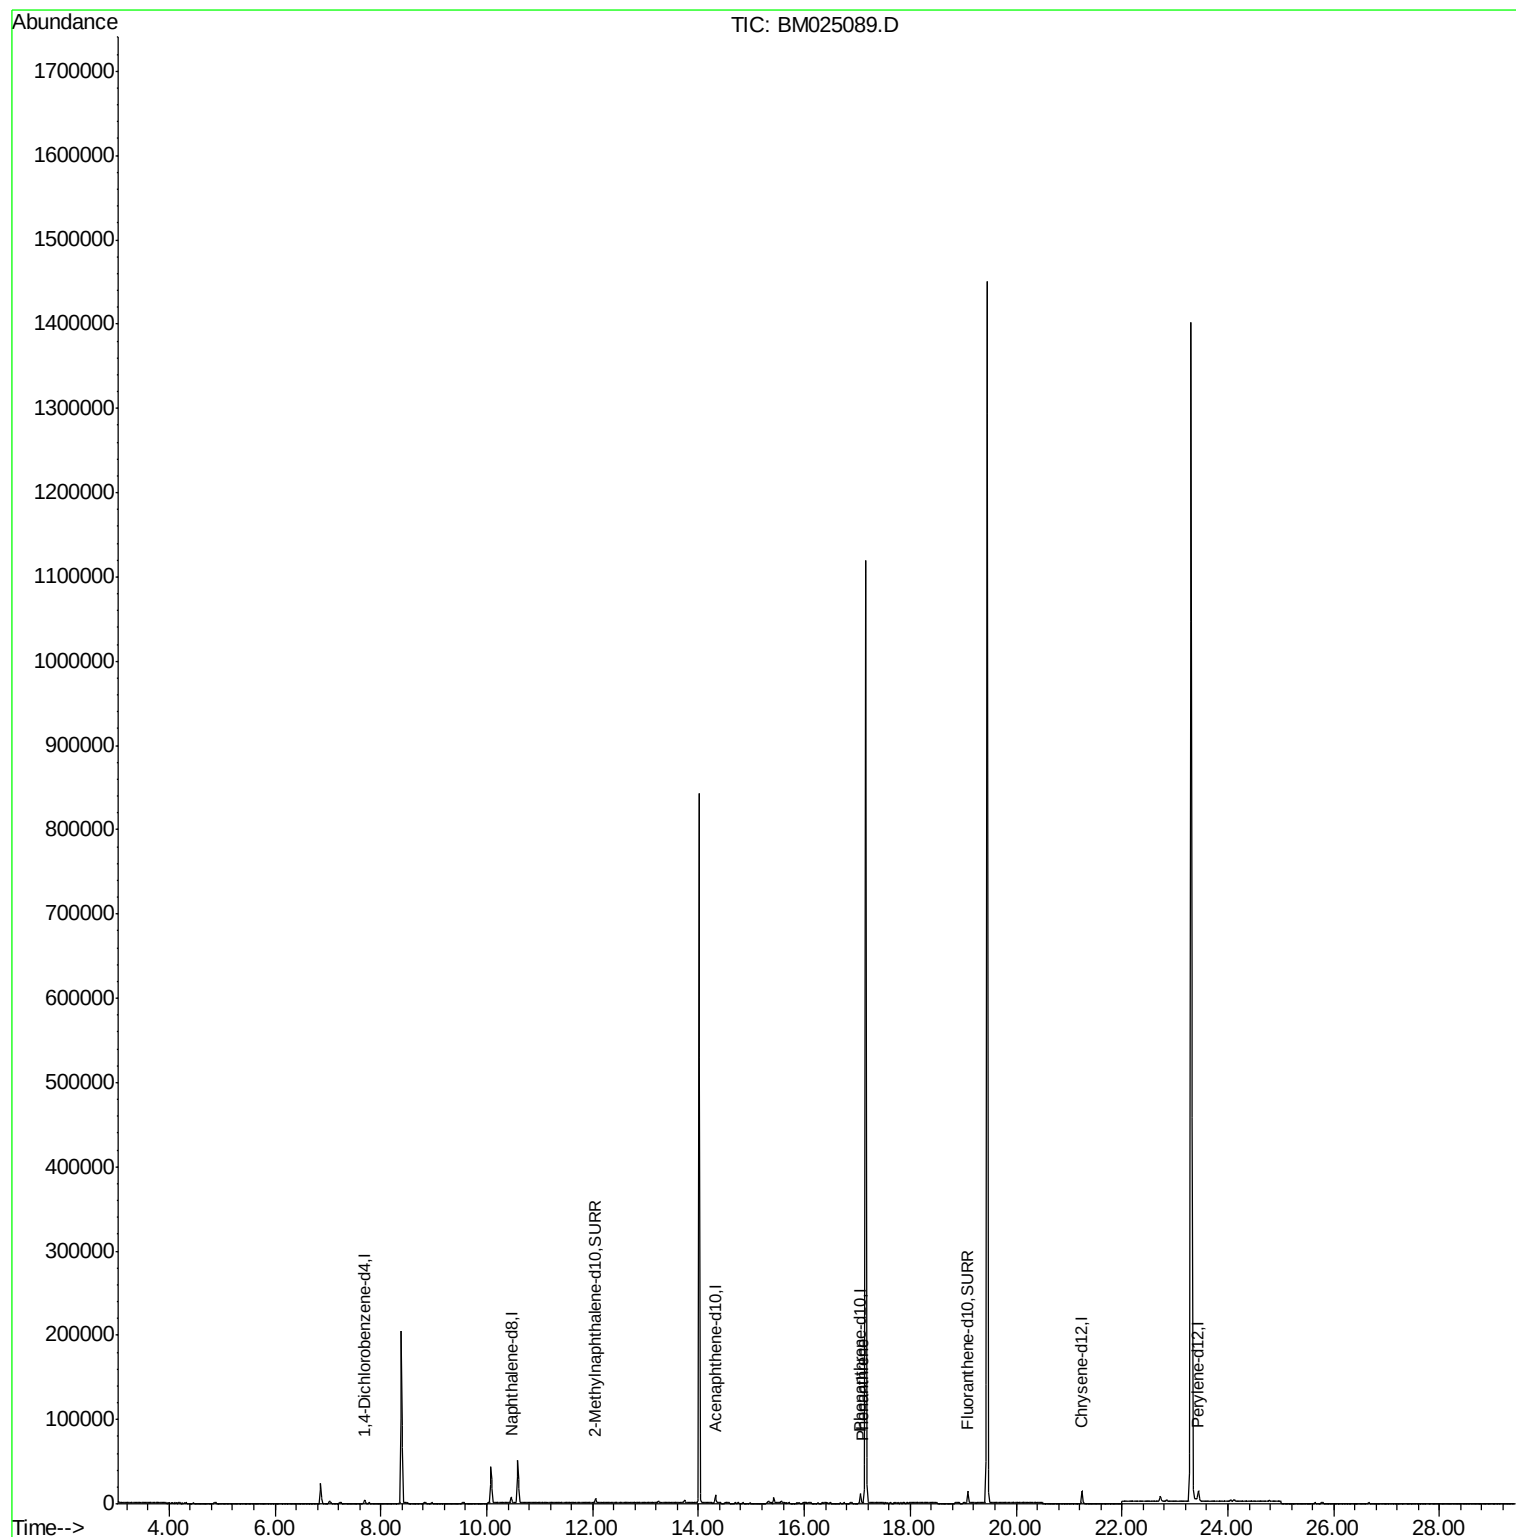

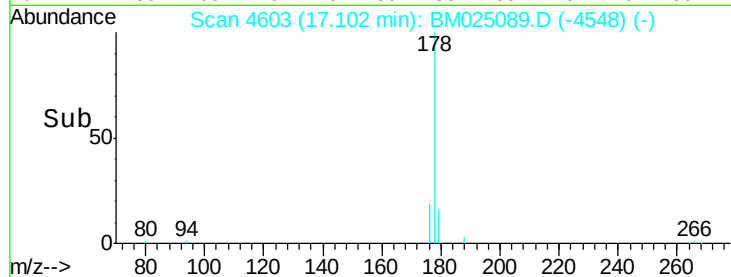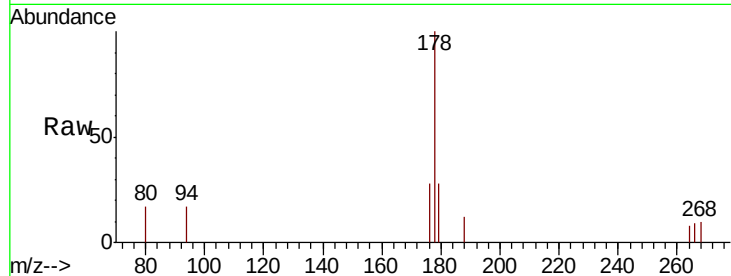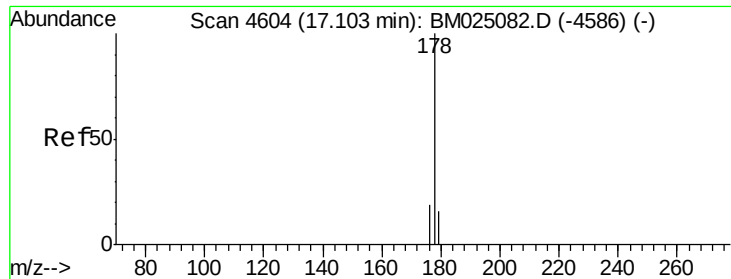

#12

Phenanthrene

Concen: 0.021 ng/ul

RT: 17.10 min Scan# 4603

Delta R.T. -0.01 min

Lab File: BM025089.D

Acq: 26 Feb 2020 21:41

Instrument :

BNA_M

ClientSampleId :

DBCY7

Tot Ion:178 Resp: 929

Ion Ratio Lower Upper

178 100

179 28.4 14.0 21.0#

176 27.6 16.6 24.8#

Manual Integrations
APPROVED

mohammad
2/27/2020 5:01:11 PM

