
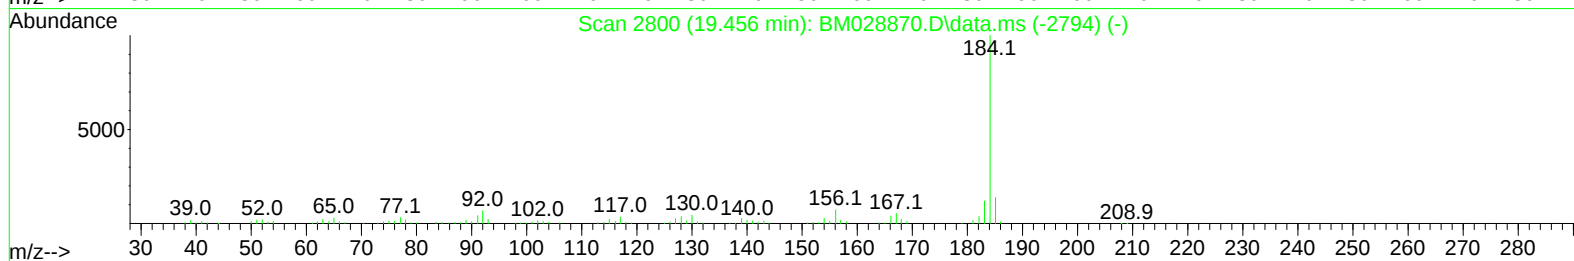
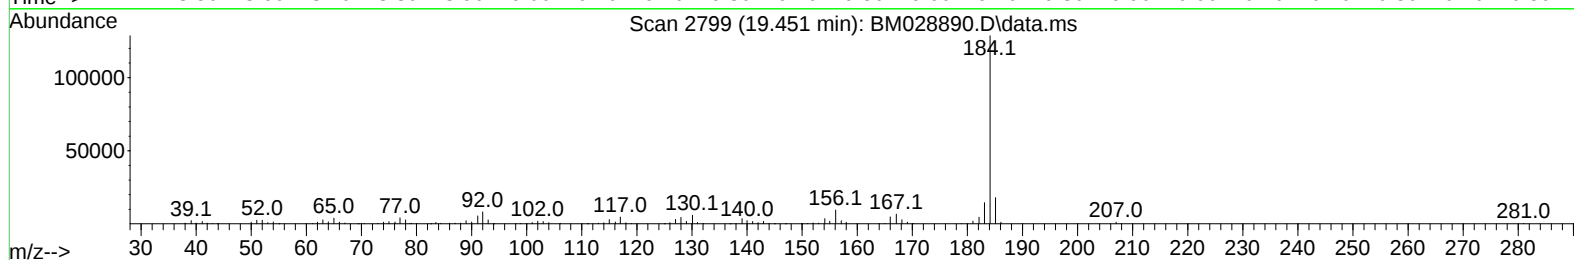


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022521\
Data File : BM028890.D
Acq On : 25 Feb 2021 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 10:33:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

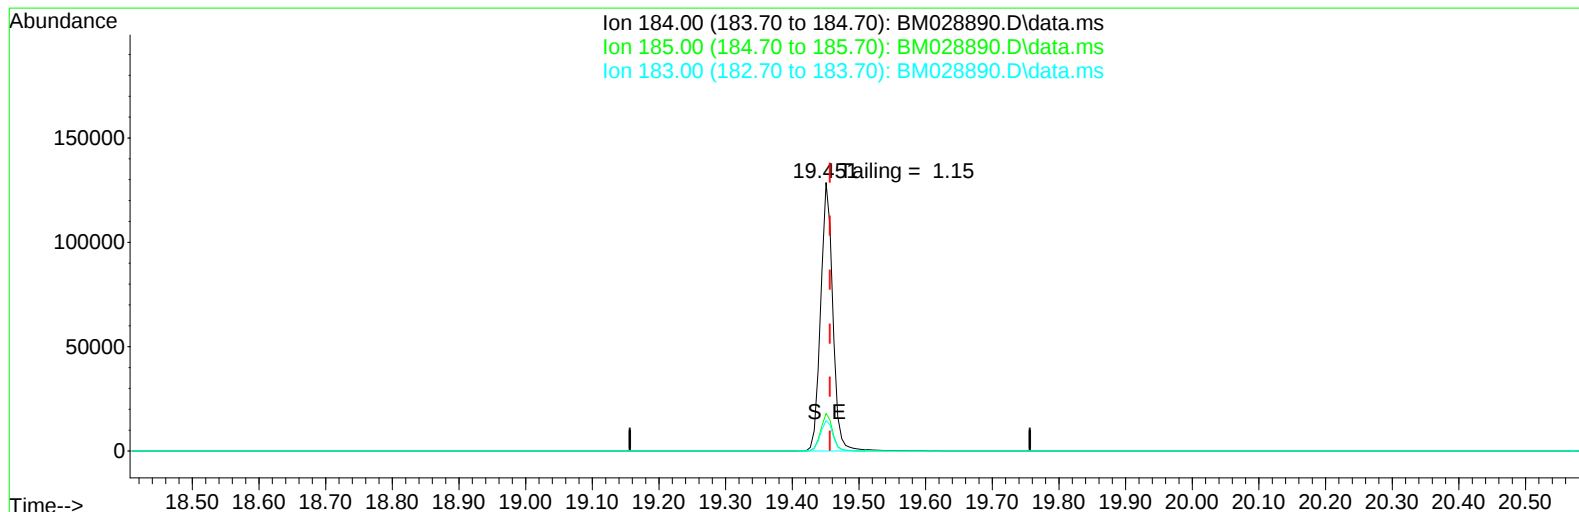

TIC: BM028890.D\data.ms

(77) Benzidine




19.451min (-0.006) 0.00 ng

response 162894

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.01
183.00	12.10	11.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022521\
Data File : BM028890.D
Acq On : 25 Feb 2021 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 10:33:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

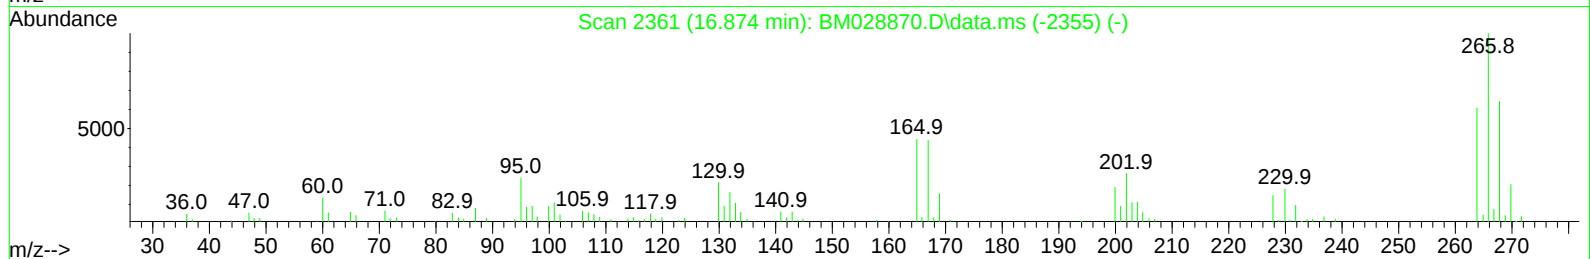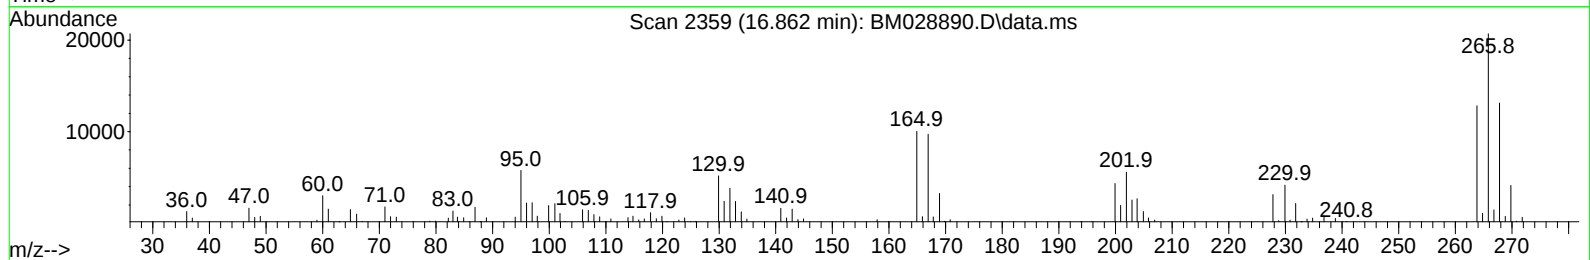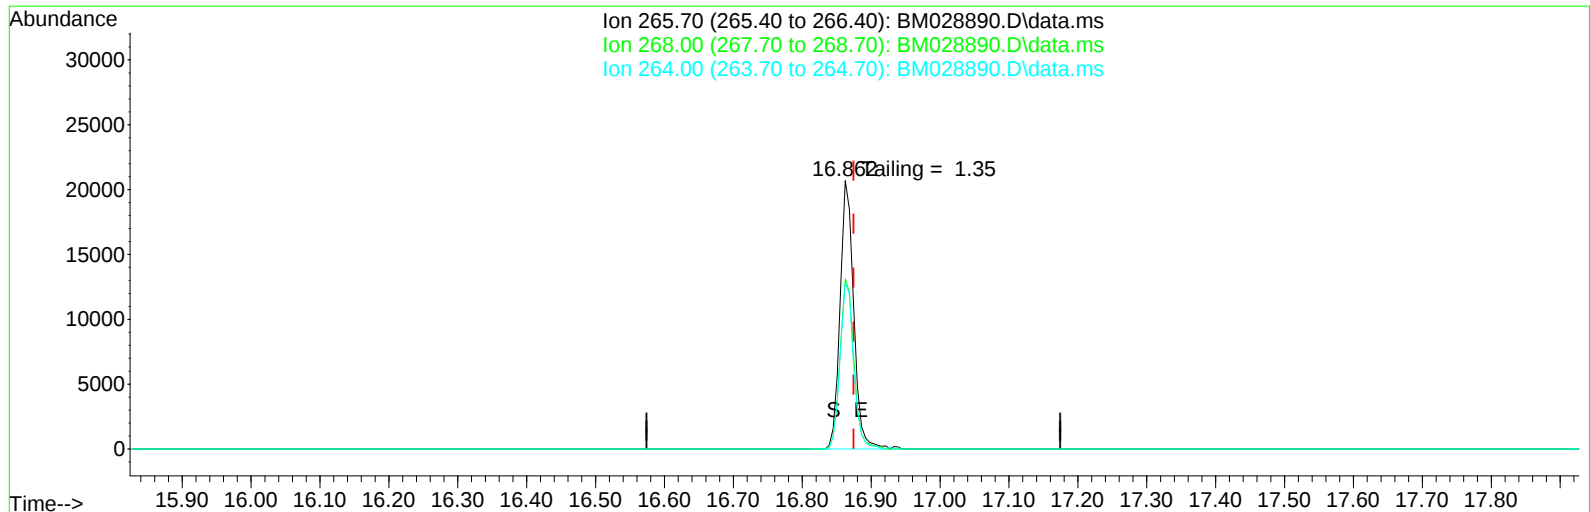

TIC: BM028890.D\data.ms

(70) Pentachlorophenol (C)

16.862min (-0.012) 0.00 ng

response 28476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.47
264.00	63.30	62.00
0.00	0.00	0.00