


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022521\
 Data File : BM028890.D
 Acq On : 25 Feb 2021 09:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 23 16:39:41 2021

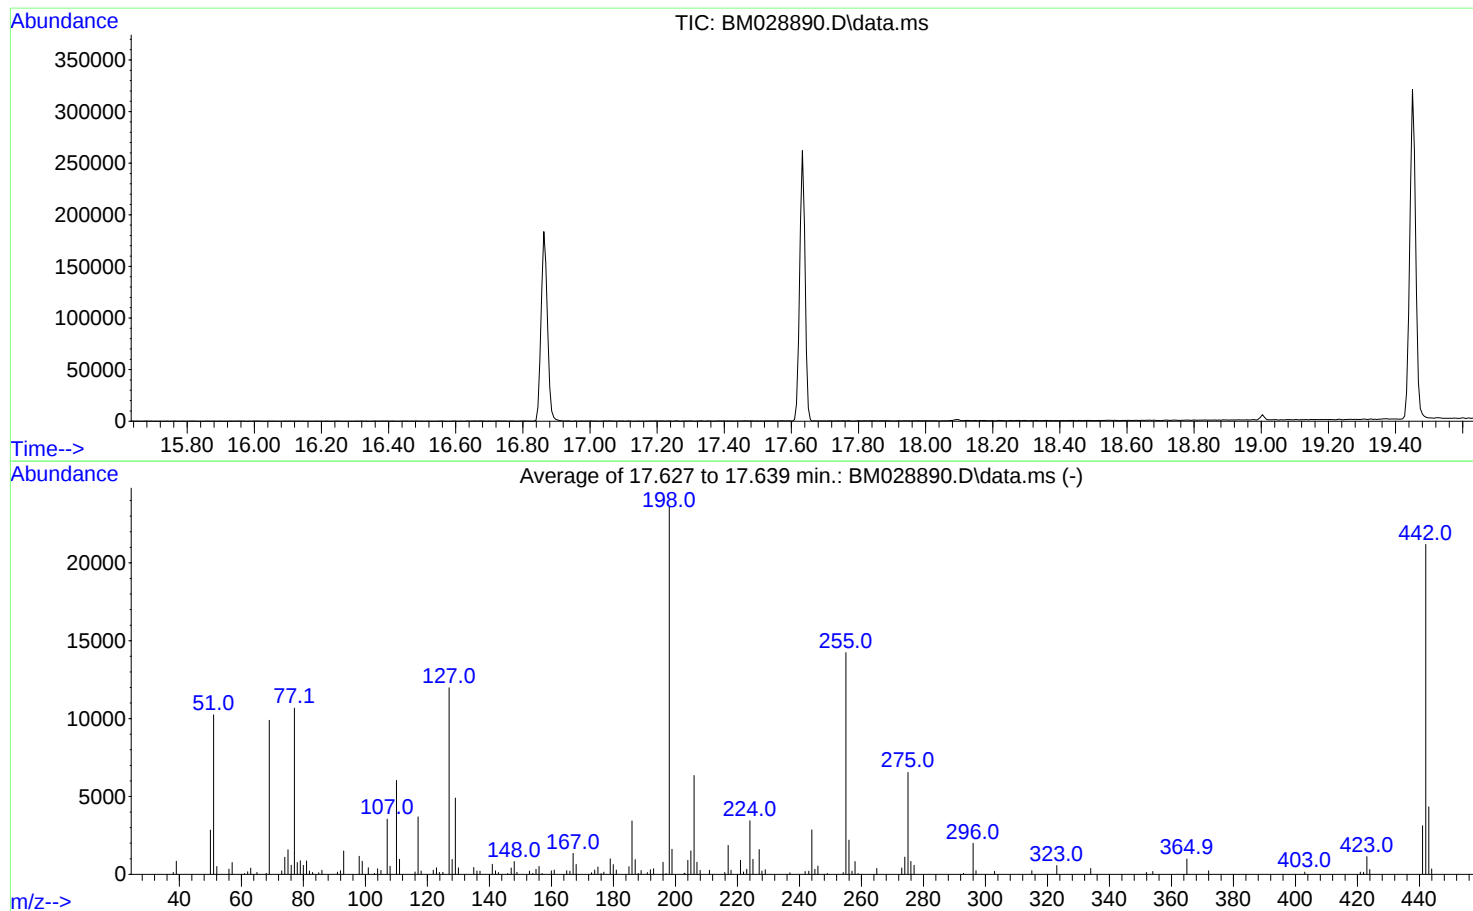

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.4	10241	PASS
68	69	0.00	2	0.6	64	PASS
69	198	0.00	100	41.9	9890	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	11974	PASS
197	198	0.00	2	0.2	54	PASS
198	198	100	100	100.0	23619	PASS
199	198	5	9	6.8	1614	PASS
275	198	10	60	27.7	6549	PASS
365	198	1	100	4.2	987	PASS
441	198	0.01	100	13.2	3123	PASS
442	442	50	100	100.0	21183	PASS
443	442	15	24	20.5	4335	PASS




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

	DDT Breakdown	
Date	Instrument Name	DFTPP Data File
2/25/2021	BNA_M	<u>BM028890.D</u>
Compound Name	Response	Retention Time
DDT	81672	20.668
DDD	787	20.233
DDE	0	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
787	82459	0.95

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022521\
Data File : BM028890.D
Acq On : 25 Feb 2021 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 25 10:33:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

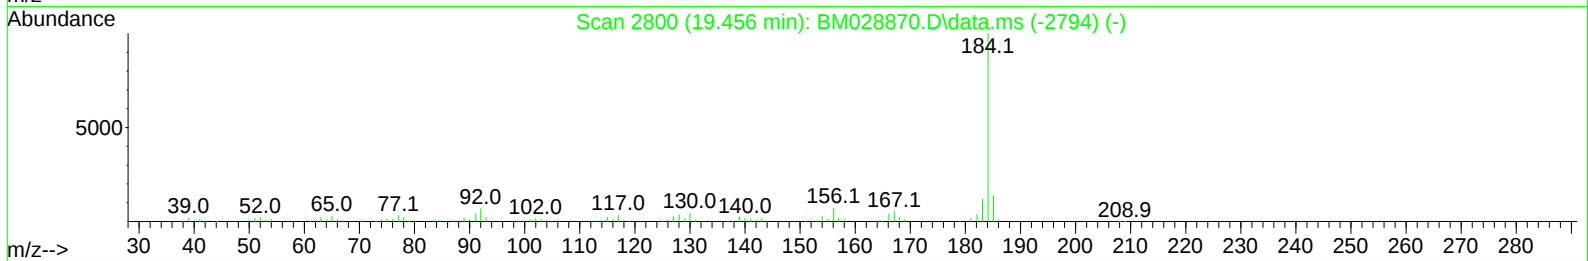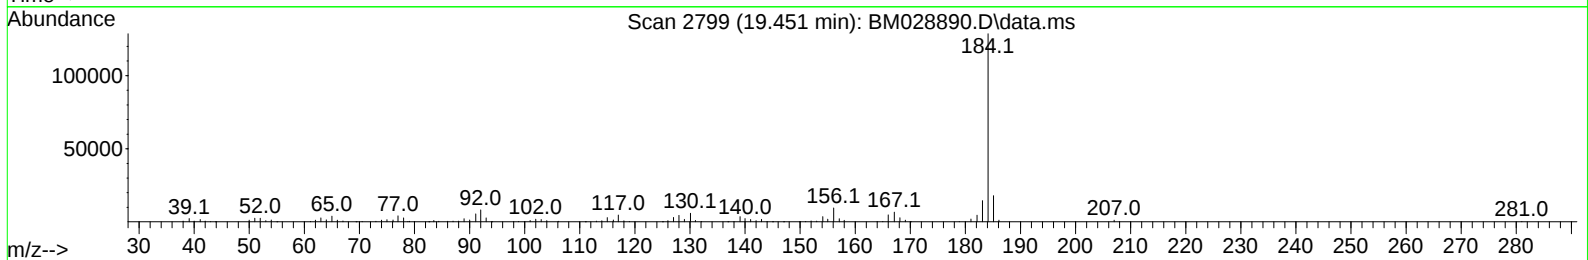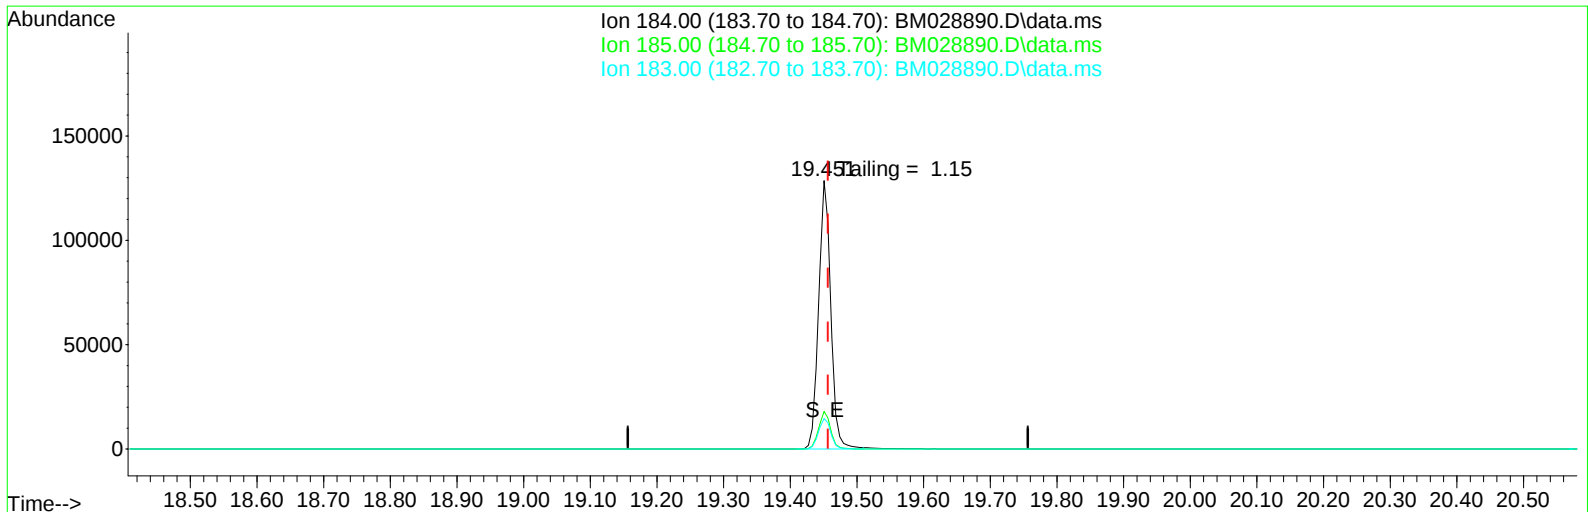

TIC: BM028890.D\data.ms

(77) Benzidine

19.451min (-0.006) 0.00 ng




response 162894

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.01
183.00	12.10	11.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022521\
Data File : BM028890.D
Acq On : 25 Feb 2021 09:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 25 10:33:08 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 16:39:41 2021
Response via : Initial Calibration

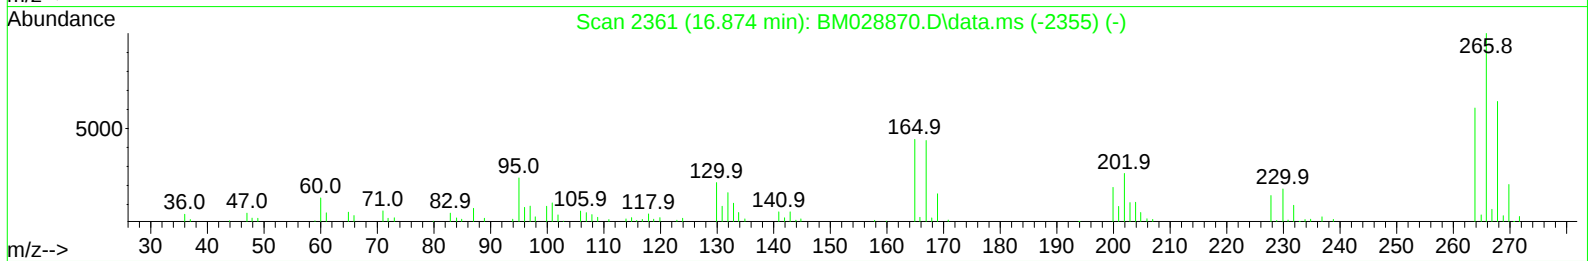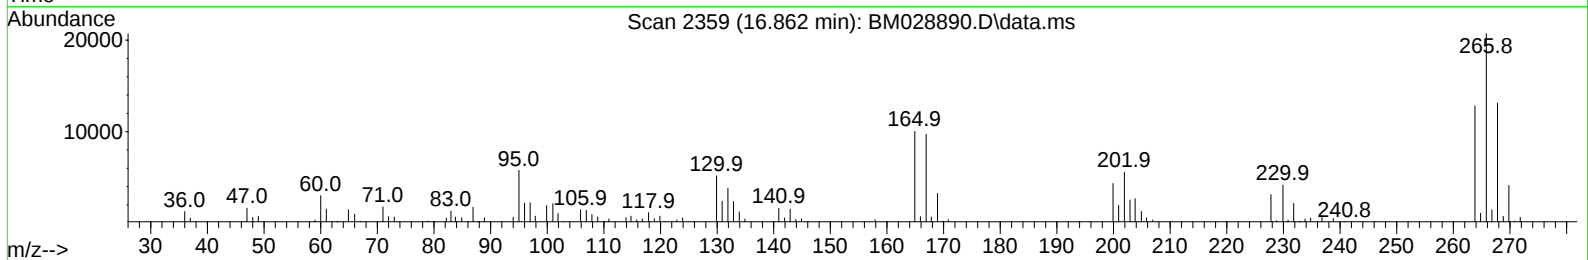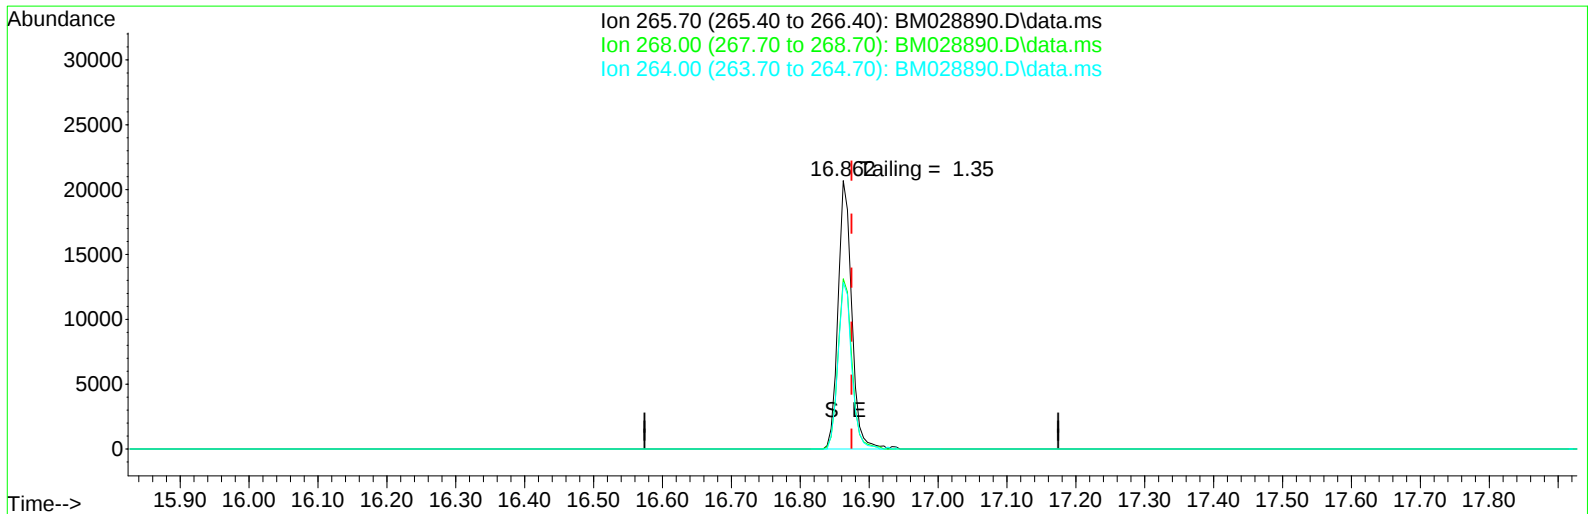

TIC: BM028890.D\data.ms

(70) Pentachlorophenol (C)

16.862min (-0.012) 0.00 ng

response 28476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.47
264.00	63.30	62.00
0.00	0.00	0.00