

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022719\
 Data File : BM018962.D
 Acq On : 27 Feb 2019 22:50
 Operator : JU/SJ
 Sample : K1633-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SR-11-S

Quant Time: Feb 28 03:16:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	253034	20.00	ng	-0.02
21) Naphthalene-d8	10.48	136	1059994	20.00	ng	-0.02
39) Acenaphthene-d10	14.34	164	640663	20.00	ng	-0.02
64) Phenanthrene-d10	17.10	188	1444089	20.00	ng	-0.02
76) Chrysene-d12	21.29	240	1305162	20.00	ng	-0.02
87) Perylene-d12	23.54	264	1113641	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	2251519	145.79	ng	-0.02
7) Phenol-d6	6.87	99	2920629	134.25	ng	-0.02
23) Nitrobenzene-d5	8.86	82	2331788	101.72	ng	-0.02
42) 2,4,6-Tribromophenol	15.84	330	1481421	160.41	ng	-0.02
45) 2-Fluorobiphenyl	12.96	172	4842111	100.33	ng	-0.02
79) Terphenyl-d14	19.73	244	7956910	125.76	ng	-0.01
Target Compounds						
9) Benzaldehyde	6.86	77	6440	Below Cal	Qvalue #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022719\
Data File : BM018962.D
Acq On : 27 Feb 2019 22:50
Operator : JU/SJ
Sample : K1633-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SR-11-S

Quant Time: Feb 28 03:16:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

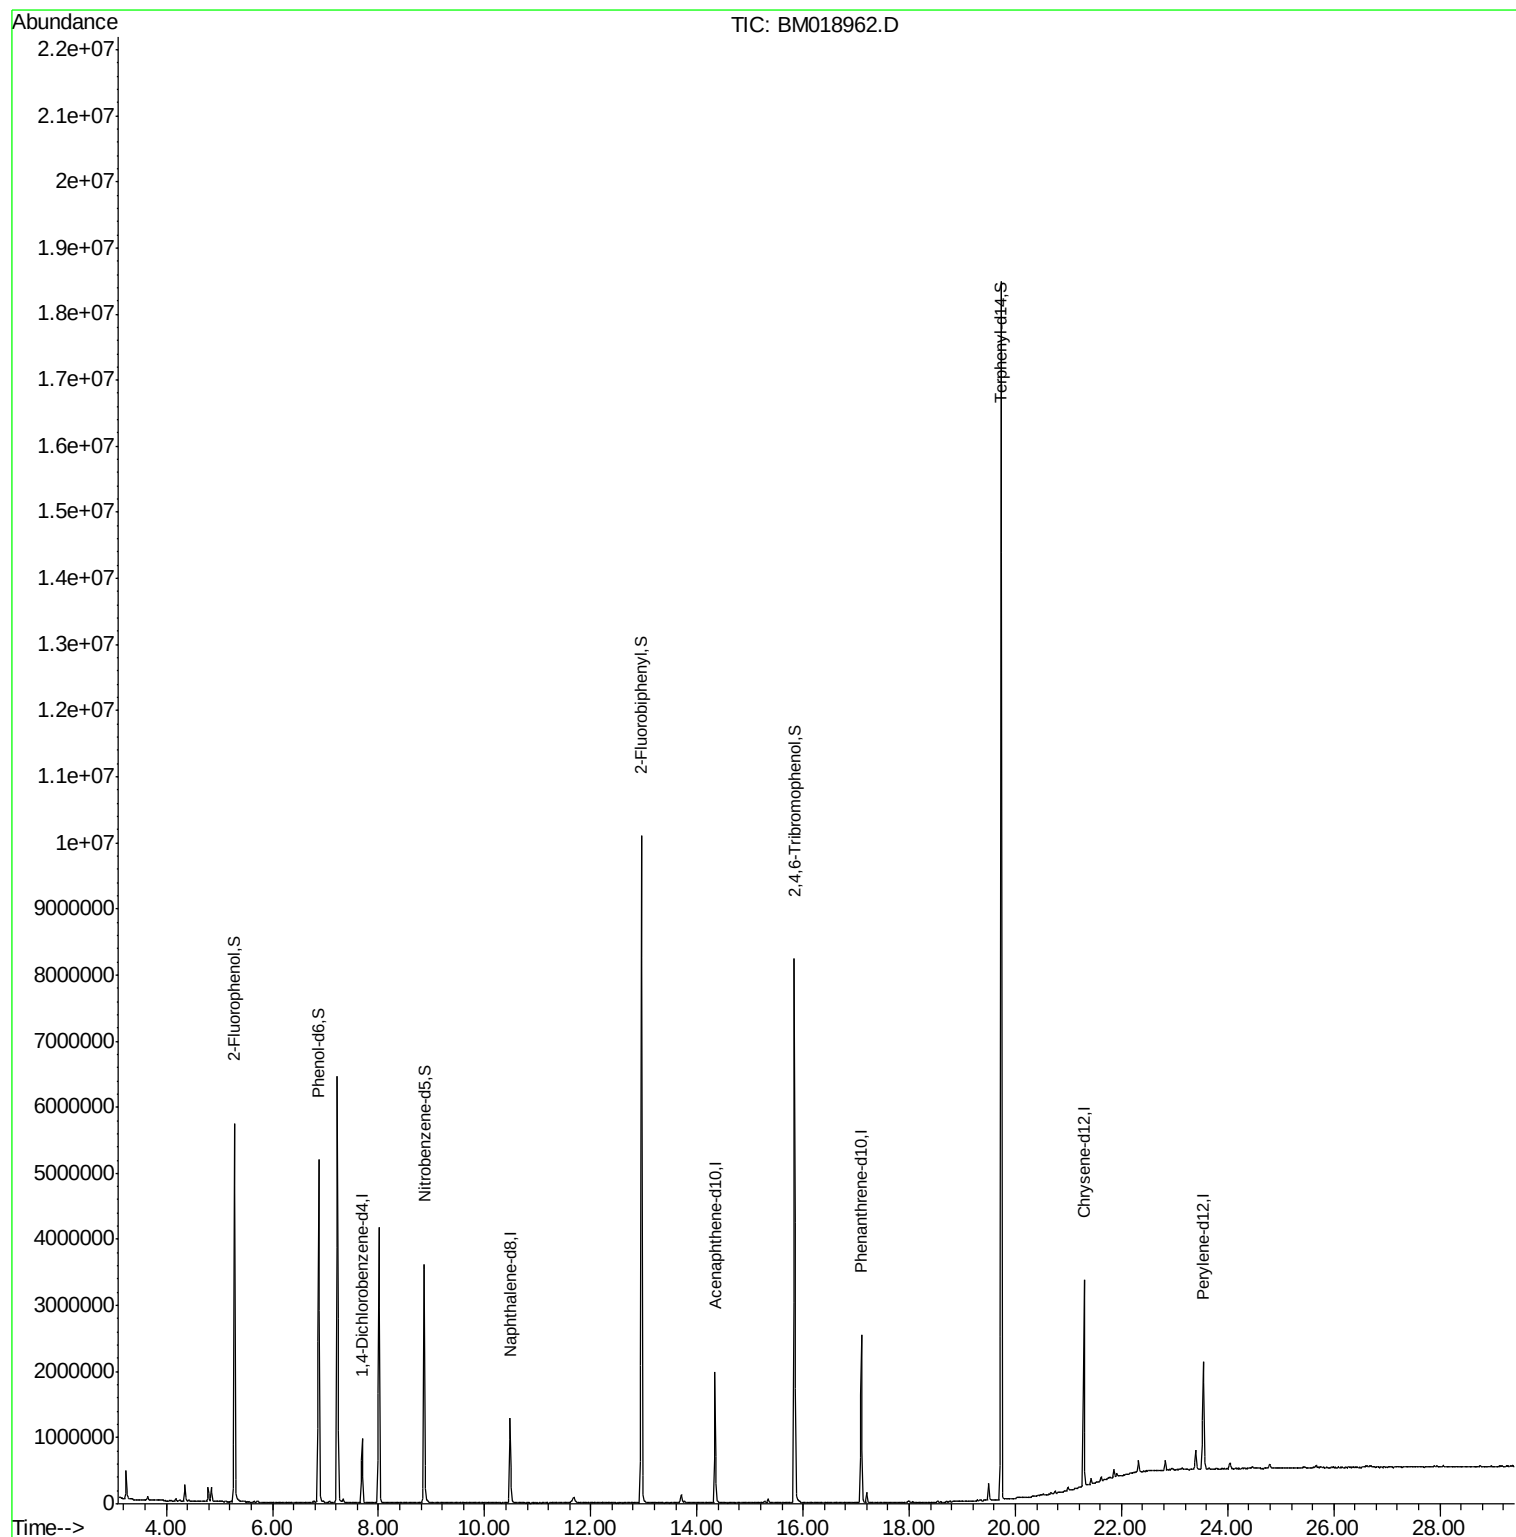

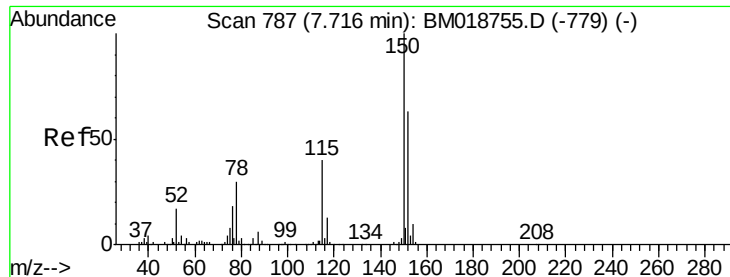


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.69 min Scan# 783
Delta R.T. -0.02 min
Lab File: BM018962.D
Acq: 27 Feb 2019 22:50

Instrument :
BNA_M
ClientSampleId :
SR-11-S

Tgt Ion:152 Resp: 253034
Ion Ratio Lower Upper
152 100
150 153.6 127.3 190.9
115 62.0 50.8 76.2

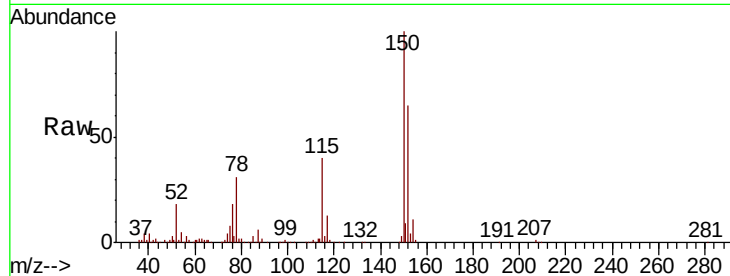


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

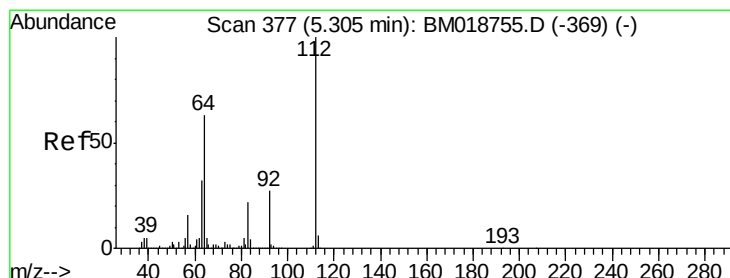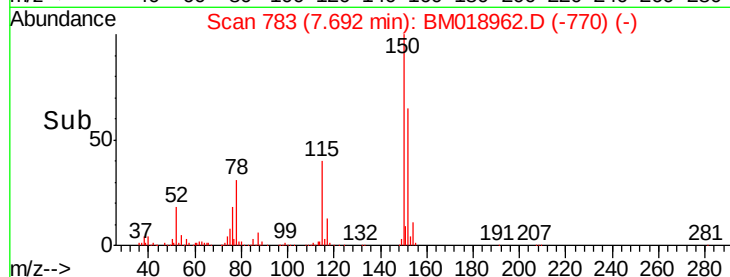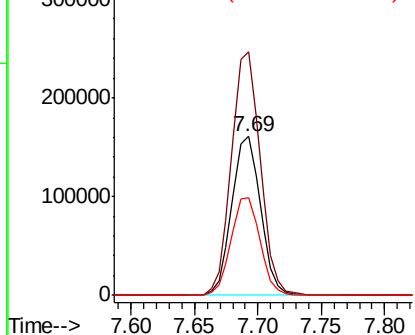



#5


2-Fluorophenol
Concen: 145.793 ng
RT: 5.29 min Scan# 374
Delta R.T. -0.02 min
Lab File: BM018962.D
Acq: 27 Feb 2019 22:50

Tgt Ion:112 Resp: 2251519
Ion Ratio Lower Upper
112 100
64 64.1 50.6 75.8
63 32.9 25.7 38.5

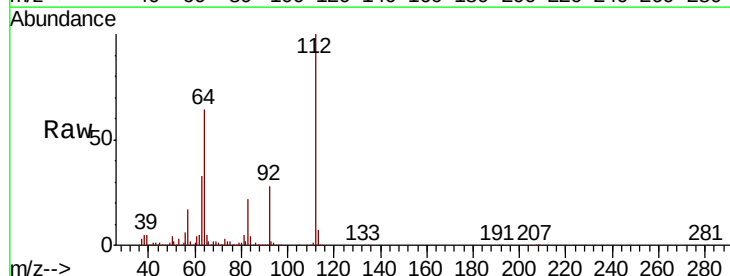

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

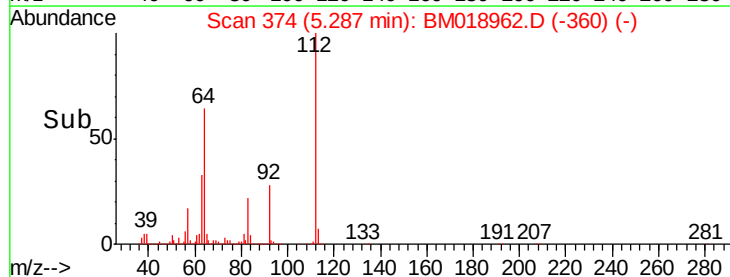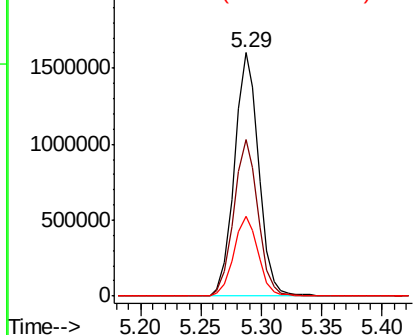

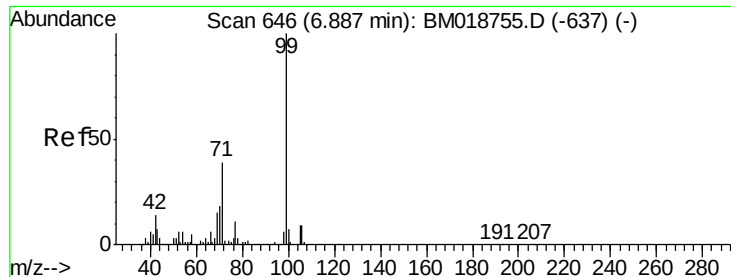

#7

Phenol-d6

Concen: 134.246 ng

RT: 6.87 min Scan# 643

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50

Instrument :

BNA_M

ClientSampleId :

SR-11-S


Tgt Ion: 99 Resp: 2920629

Ion Ratio Lower Upper

99 100

42 14.2 11.0 16.6

71 38.7 31.3 46.9



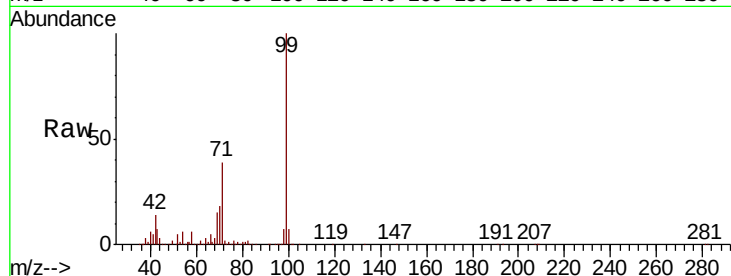


Abundance

Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

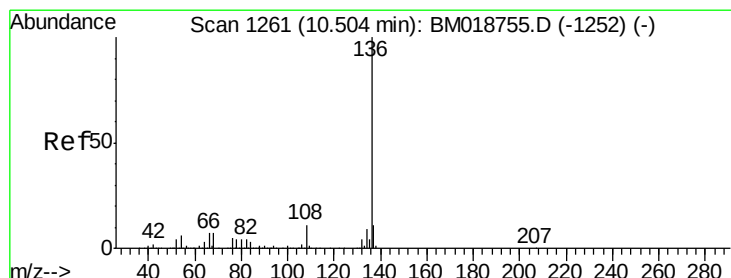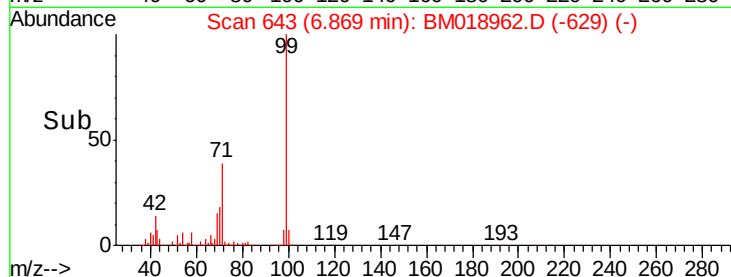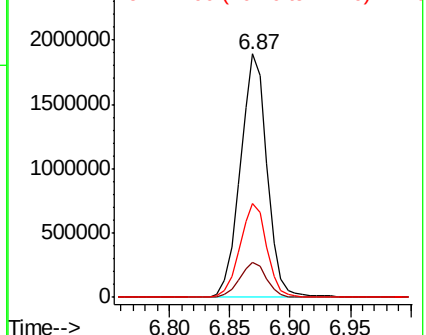

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.48 min Scan# 1257

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50

Tgt Ion: 136 Resp: 1059994


Ion Ratio Lower Upper

136 100

137 10.7 8.8 13.2

54 7.3 5.0 7.6

68 7.3 5.5 8.3

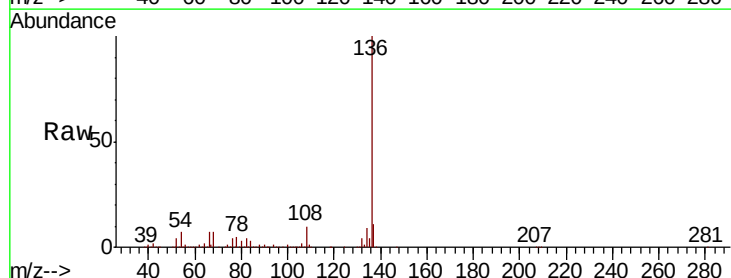



Abundance


Ion 136.00 (135.70 to 136.70): BM018755.D (-1252) (-)

Ion 137.00 (136.70 to 137.70): BM018755.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018755.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018755.D (-1252) (-)

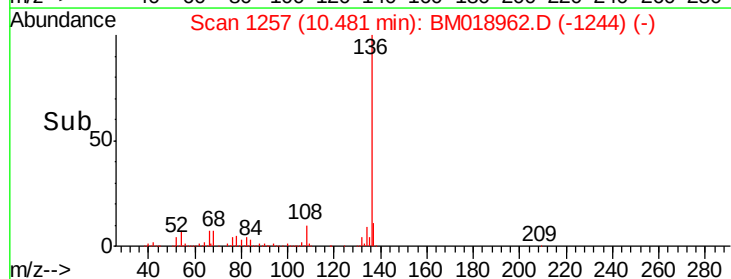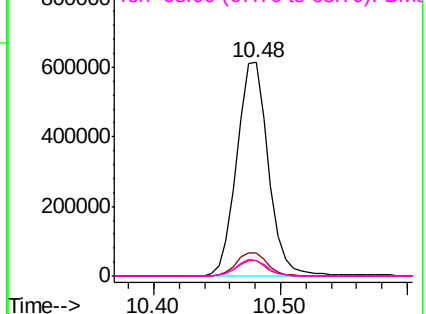

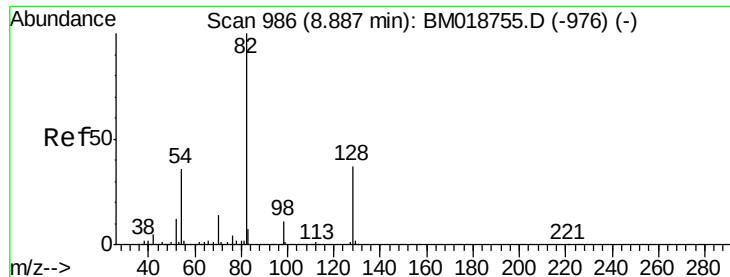

#23

Nitrobenzene-d5

Concen: 101.716 ng

RT: 8.86 min Scan# 982

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50

Instrument :

BNA_M

ClientSampleId :

SR-11-S


Tgt Ion: 82 Resp: 2331788

Ion Ratio Lower Upper

82 100

128 37.1 29.9 44.9




54 36.6 29.1 43.7

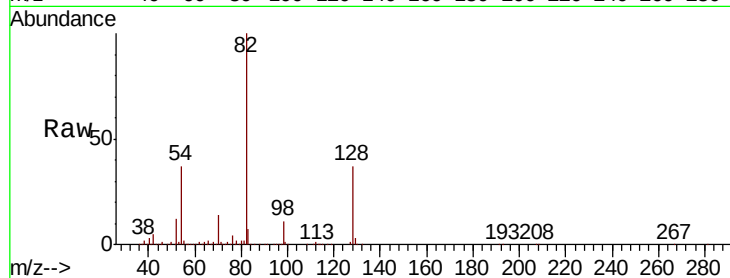

Abundance Ion 82.00 (81.70 to 82.70): BM018962.D (-969) (-)

Ion 128.00 (127.70 to 128.70): BM018962.D (-969) (-)

Ion 54.00 (53.70 to 54.70): BM018962.D (-969) (-)

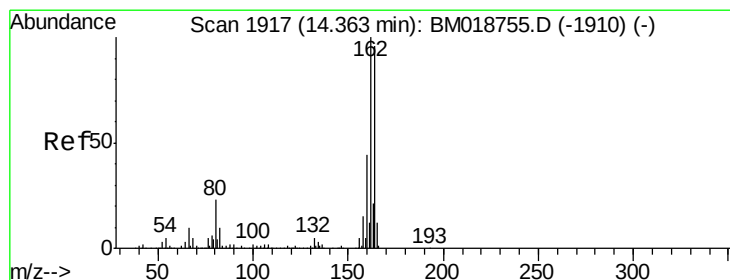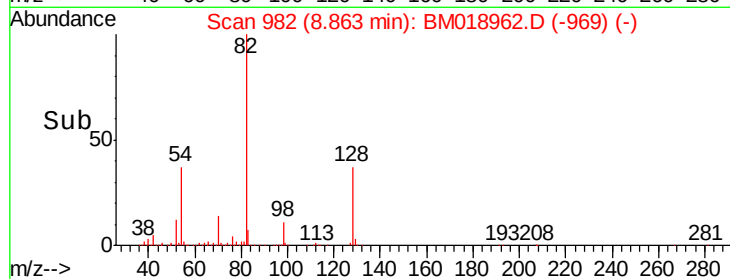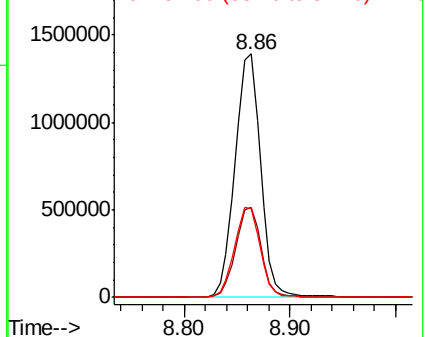

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.34 min Scan# 1913

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50


Tgt Ion: 164 Resp: 640663

Ion Ratio Lower Upper

164 100

162 102.0 83.4 125.0



160 45.5 36.6 55.0

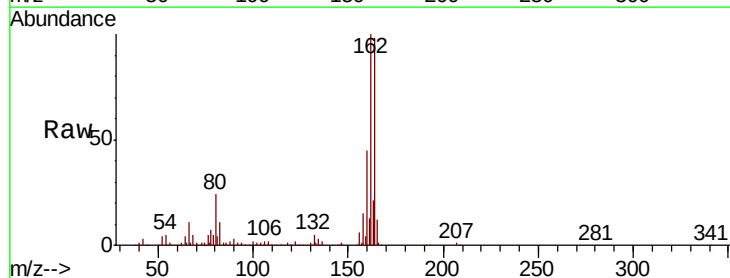


Abundance Ion 164.00 (163.70 to 164.70): BM018962.D (-1900) (-)

Ion 162.00 (161.70 to 162.70): BM018962.D (-1900) (-)

Ion 160.00 (159.70 to 160.70): BM018962.D (-1900) (-)

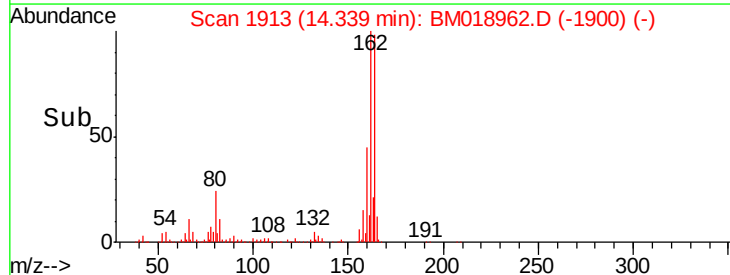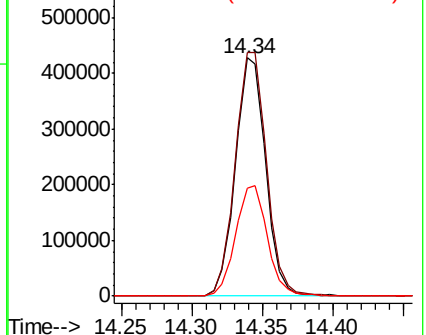

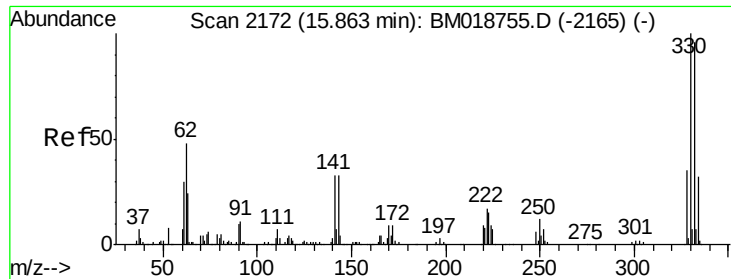

#42

2,4,6-Tribromophenol

Concen: 160.414 ng

RT: 15.84 min Scan# 2168

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50

Instrument :

BNA_M

ClientSampleId :

SR-11-S


Tgt Ion:330 Resp: 1481421

Ion Ratio Lower Upper

330 100

332 96.4 76.9 115.3




141 34.6 28.7 43.1

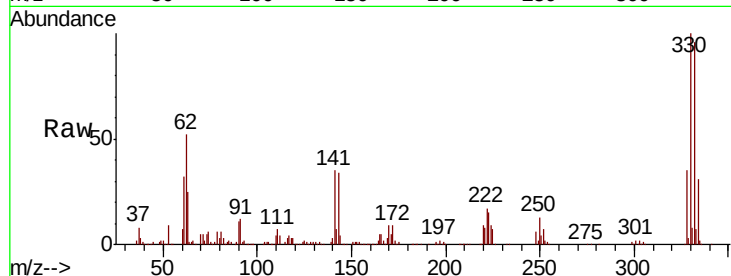

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

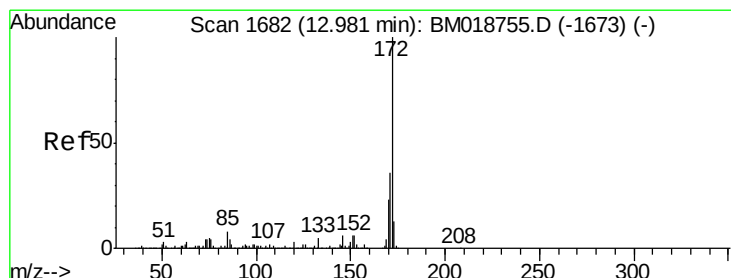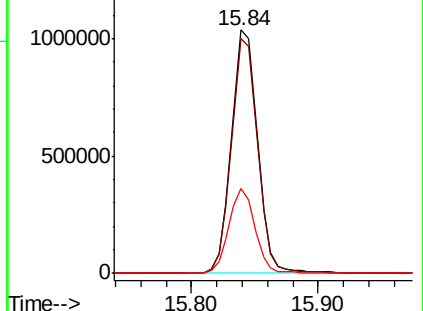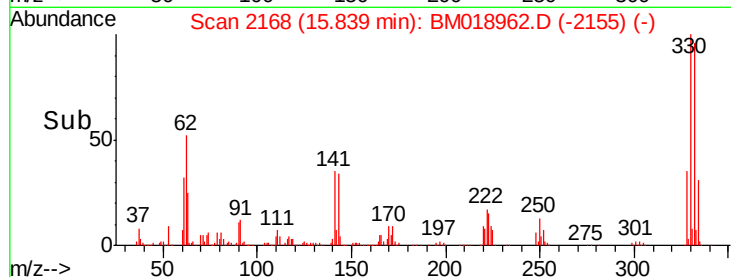

#45

2-Fluorobiphenyl

Concen: 100.330 ng

RT: 12.96 min Scan# 1678

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50


Tgt Ion:172 Resp: 4842111

Ion Ratio Lower Upper

172 100

171 36.0 29.0 43.6



170 23.6 18.6 28.0

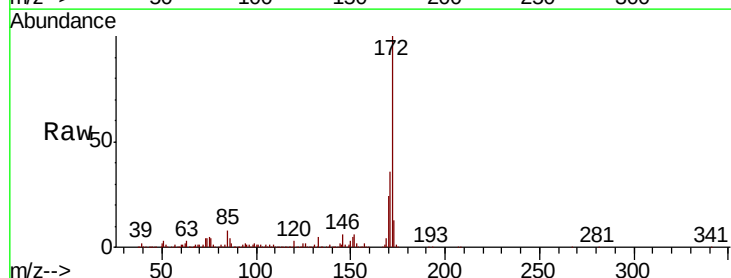


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

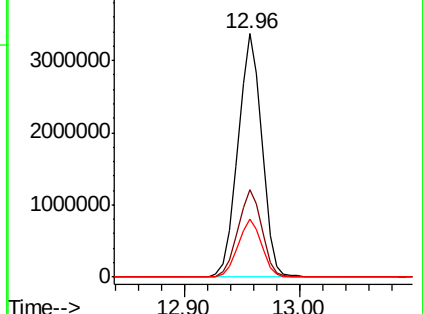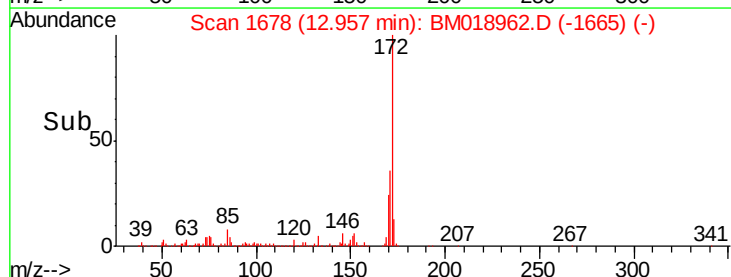

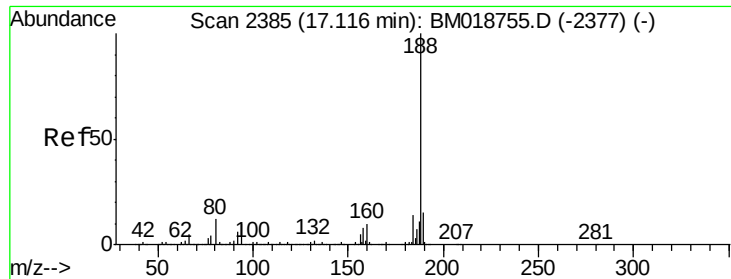

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.10 min Scan# 2382

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50

Instrument :

BNA_M

ClientSampleId :

SR-11-S


Tgt Ion:188 Resp: 1444089

Ion Ratio Lower Upper

188 100

94 9.9 8.2 12.2




80 11.9 9.7 14.5

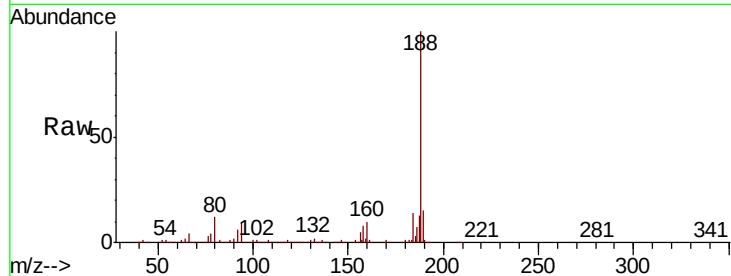

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

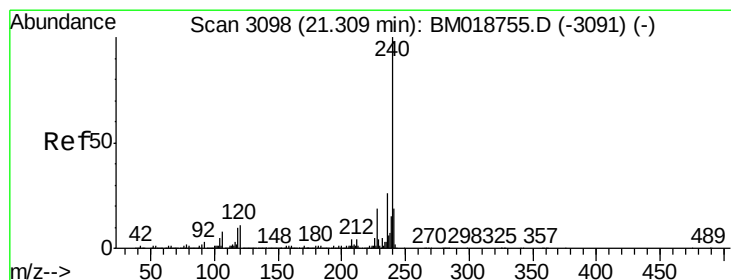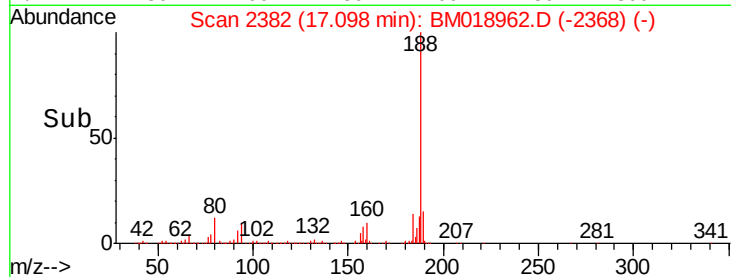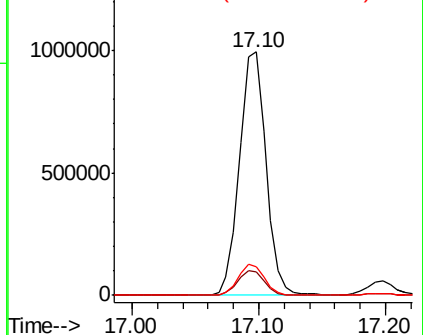

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.29 min Scan# 3095

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50


Tgt Ion:240 Resp: 1305162

Ion Ratio Lower Upper

240 100

120 11.3 8.9 13.3



236 25.8 20.9 31.3

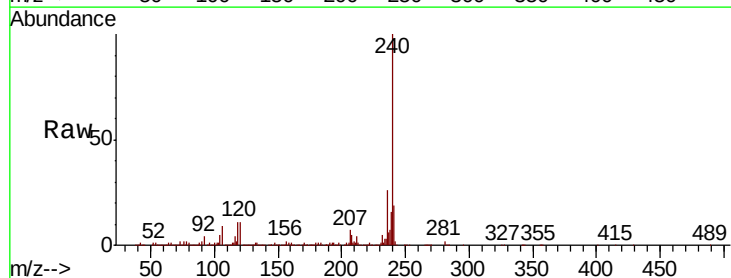


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

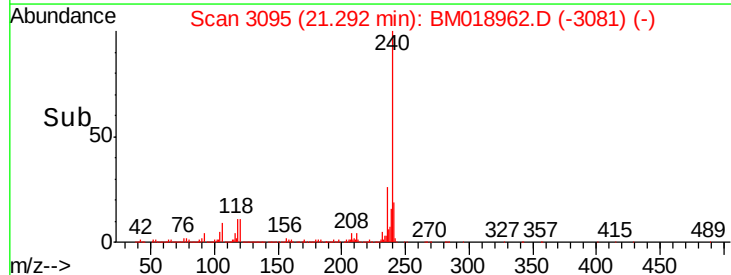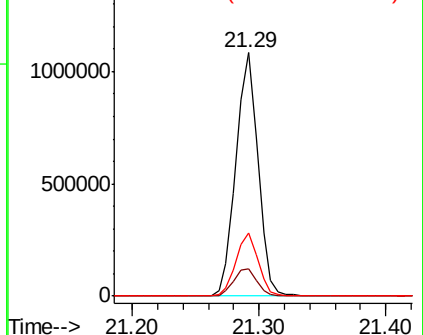

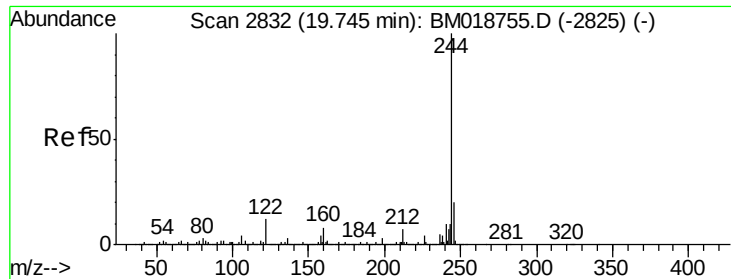

#79

Terphenyl-d14

Concen: 125.764 ng

RT: 19.73 min Scan# 2830

Delta R.T. -0.01 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50

Instrument :

BNA_M

ClientSampleId :

SR-11-S


Tgt Ion:244 Resp: 7956910

Ion Ratio Lower Upper




244 100

212 7.1 5.6 8.4

122 11.9 9.3 13.9

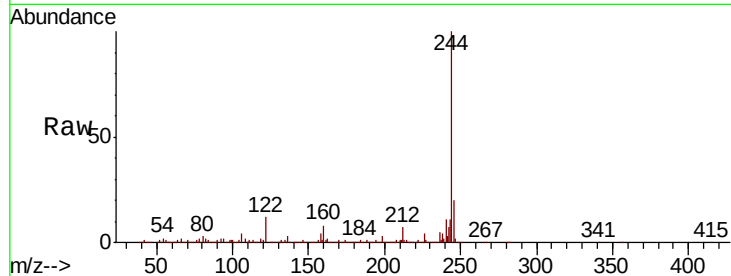

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

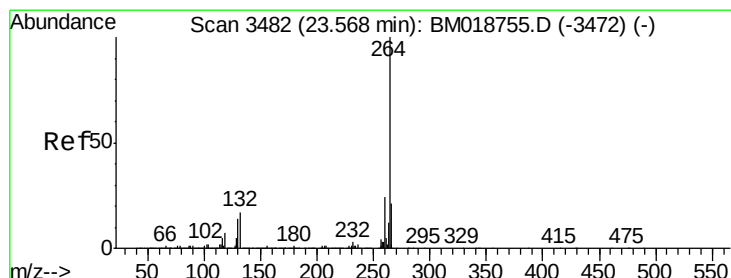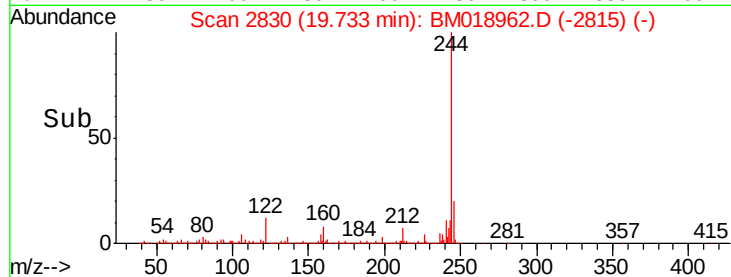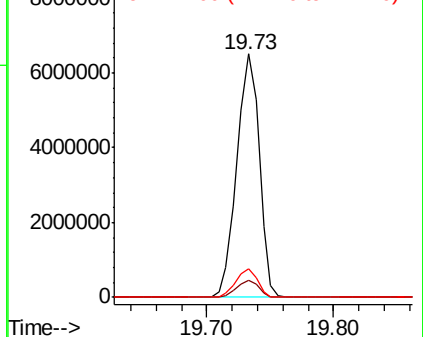

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.54 min Scan# 3478

Delta R.T. -0.02 min

Lab File: BM018962.D

Acq: 27 Feb 2019 22:50


Tgt Ion:264 Resp: 1113641

Ion Ratio Lower Upper

264 100

260 23.7 18.9 28.3

265 20.7 17.3 25.9

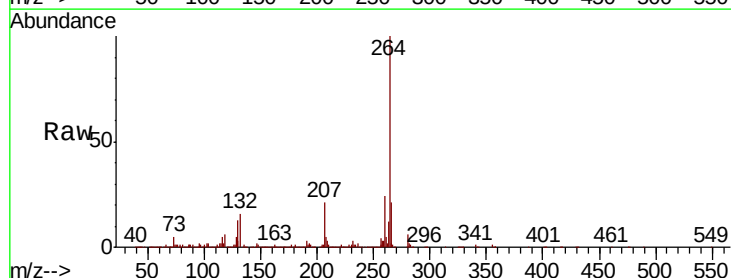

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

