
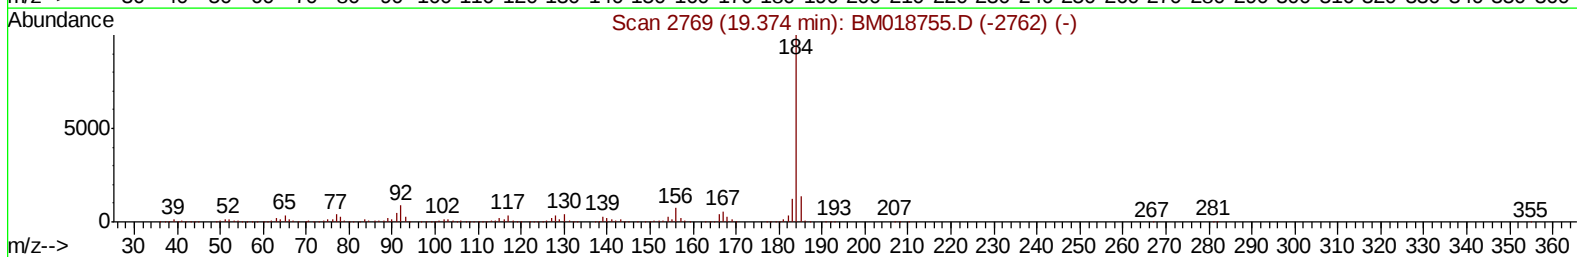
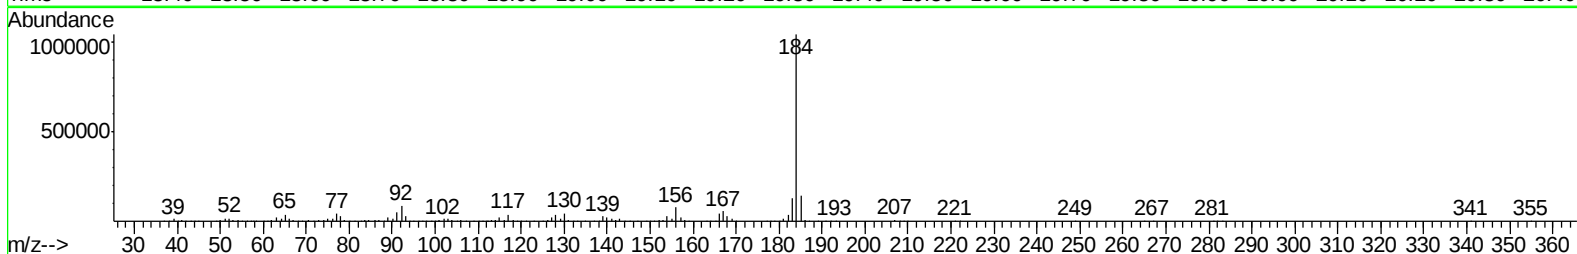


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022719\
Data File : BM018946.D
Acq On : 27 Feb 2019 12:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 04:25:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

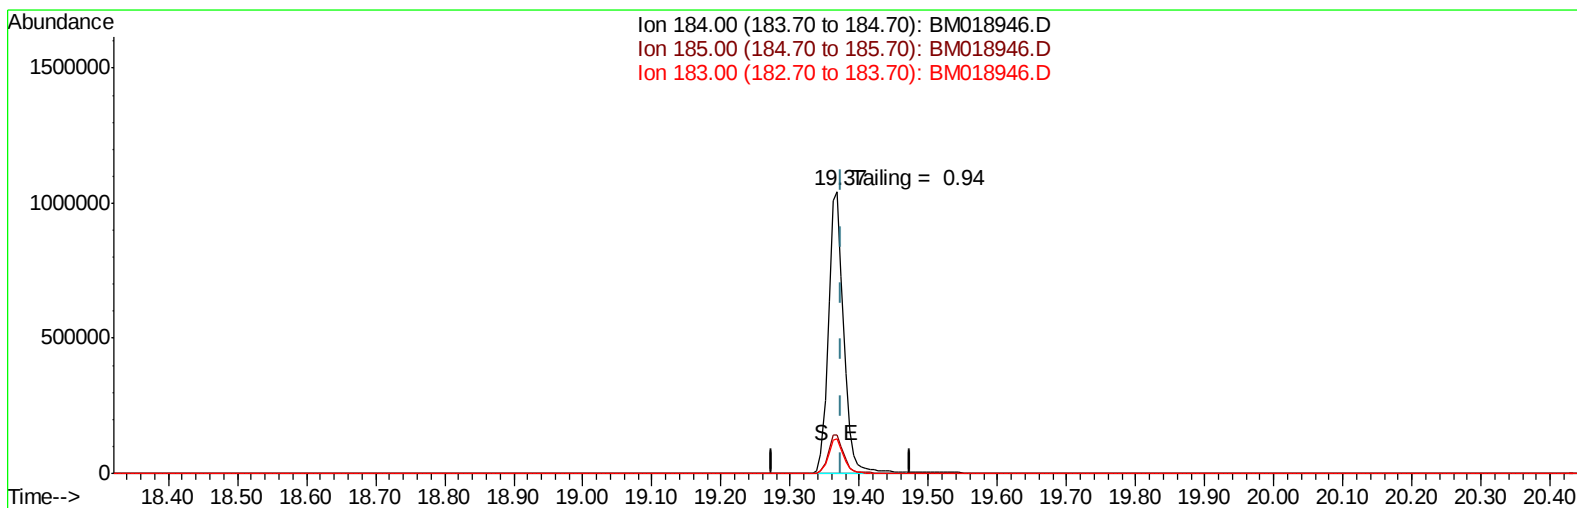

TIC: BM018946.D

(77) Benzidine



19.368min (-0.006) 8596.53ng

response 1588151

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.73
183.00	12.10	12.29
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022719\
Data File : BM018946.D
Acq On : 27 Feb 2019 12:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 04:25:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

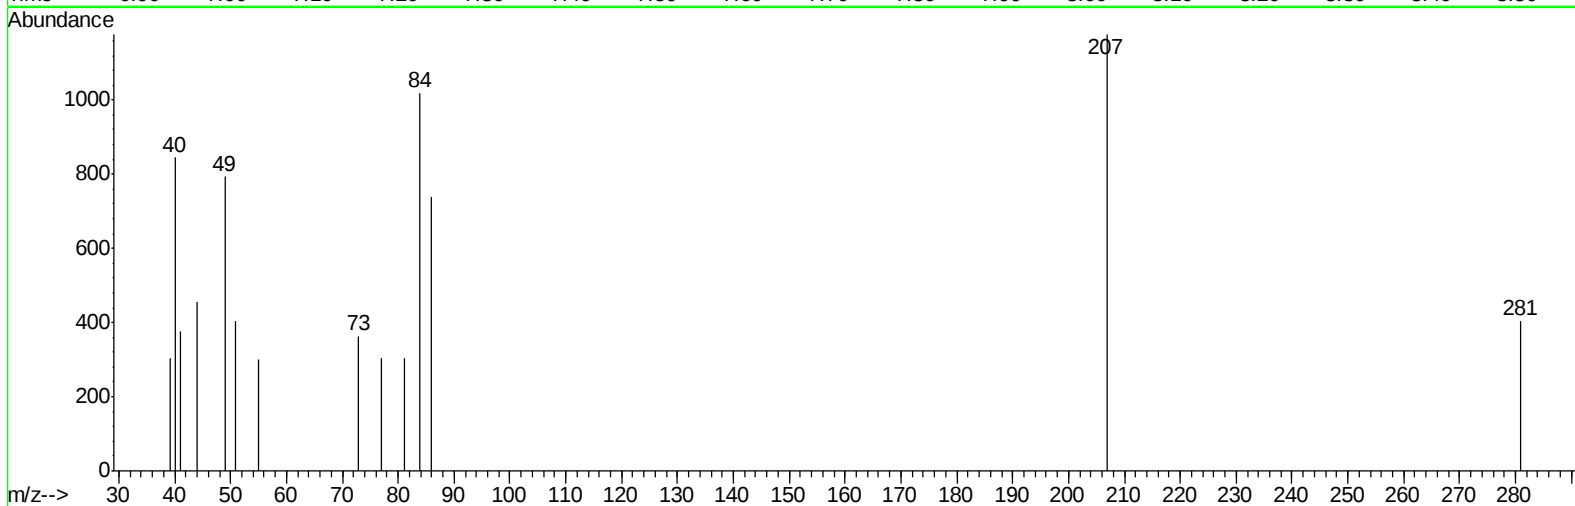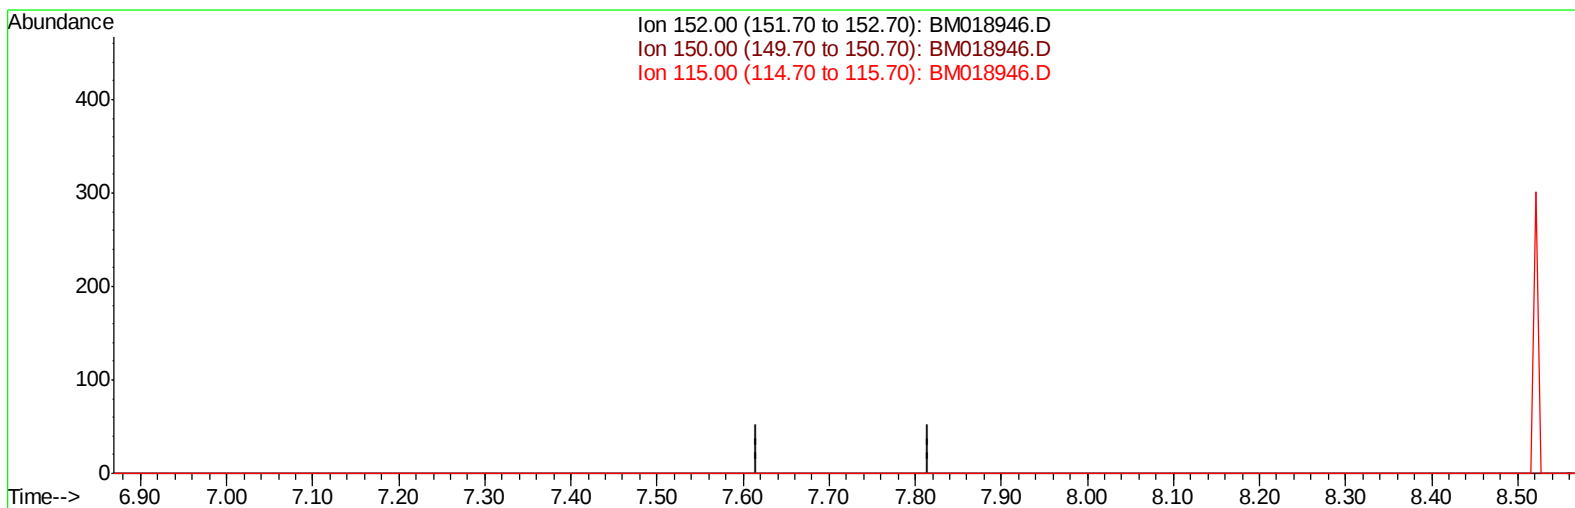

TIC: BM018946.D

(1) 1,4-Dichlorobenzene-d4 (I)




7.716min (-7.716) 0.00ng

response 0

Ion	Exp%	Act%
152.00	100	0.00
150.00	159.10	0.00#
115.00	63.50	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022719\
Data File : BM018946.D
Acq On : 27 Feb 2019 12:25
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 28 04:25:04 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

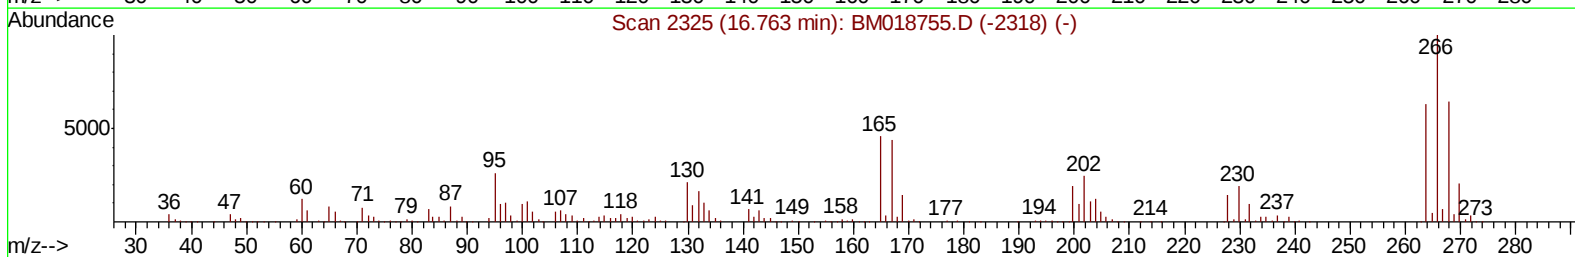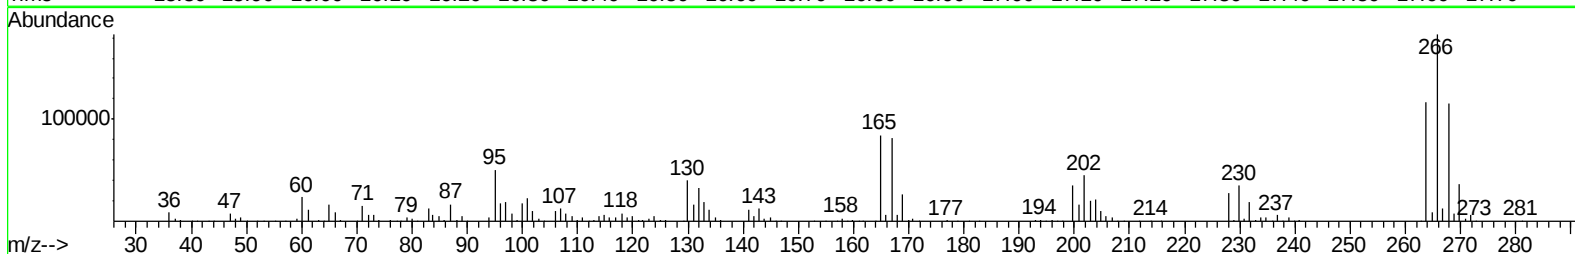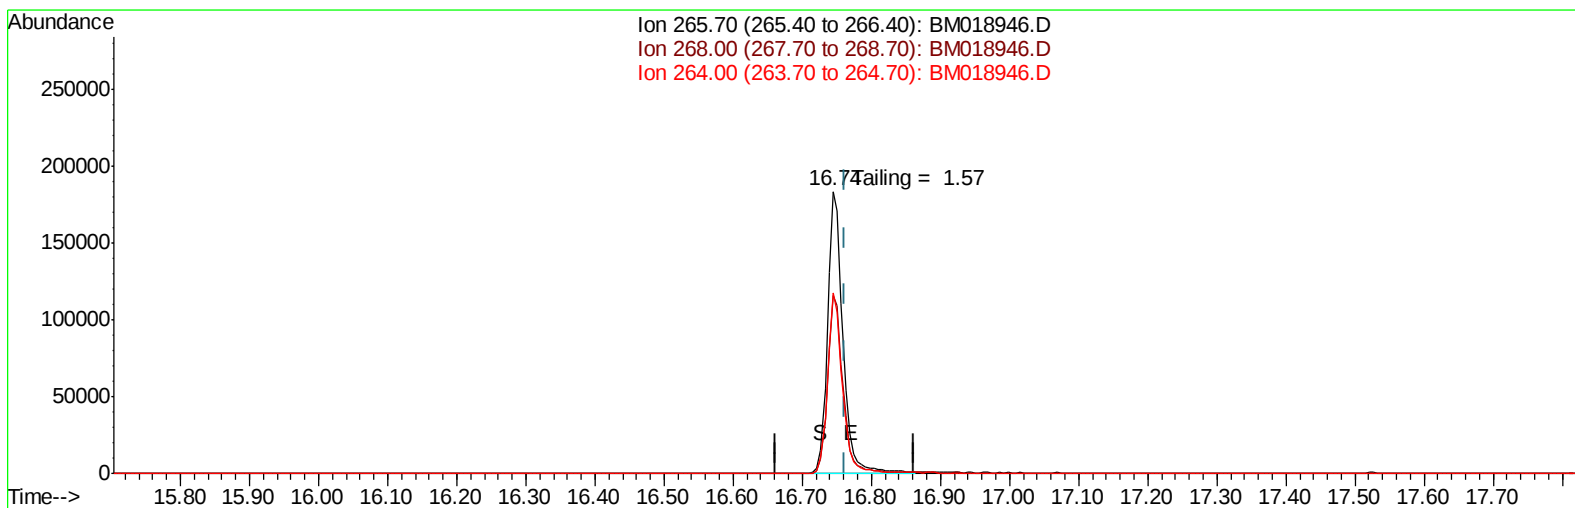

TIC: BM018946.D

(70) Pentachlorophenol (C)

16.745min (-0.018) 150044.07ng

response 280299

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.32
264.00	63.20	64.00
0.00	0.00	0.00