

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022719\
 Data File : BM018950.D
 Acq On : 27 Feb 2019 15:32
 Operator : JU/SJ
 Sample : PB117349BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB117349BL

Quant Time: Feb 28 03:30:41 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 11 16:02:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	213683	20.00	ng	-0.02
21) Naphthalene-d8	10.48	136	891358	20.00	ng	-0.02
39) Acenaphthene-d10	14.34	164	518573	20.00	ng	-0.02
64) Phenanthrene-d10	17.10	188	1149780	20.00	ng	-0.02
76) Chrysene-d12	21.29	240	1243053	20.00	ng	-0.02
87) Perylene-d12	23.54	264	1096683	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.29	112	2140431	164.12	ng	-0.02
7) Phenol-d6	6.87	99	3066448	166.91	ng	-0.02
23) Nitrobenzene-d5	8.86	82	1913749	99.27	ng	-0.02
42) 2,4,6-Tribromophenol	15.84	330	1156668	154.74	ng	-0.02
45) 2-Fluorobiphenyl	12.96	172	3929379	100.59	ng	-0.02
79) Terphenyl-d14	19.73	244	6315762	104.81	ng	-0.01


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022719\
Data File : BM018950.D
Acq On : 27 Feb 2019 15:32
Operator : JU/SJ
Sample : PB117349BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB117349BL

Quant Time: Feb 28 03:30:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 11 16:02:12 2019
Response via : Initial Calibration

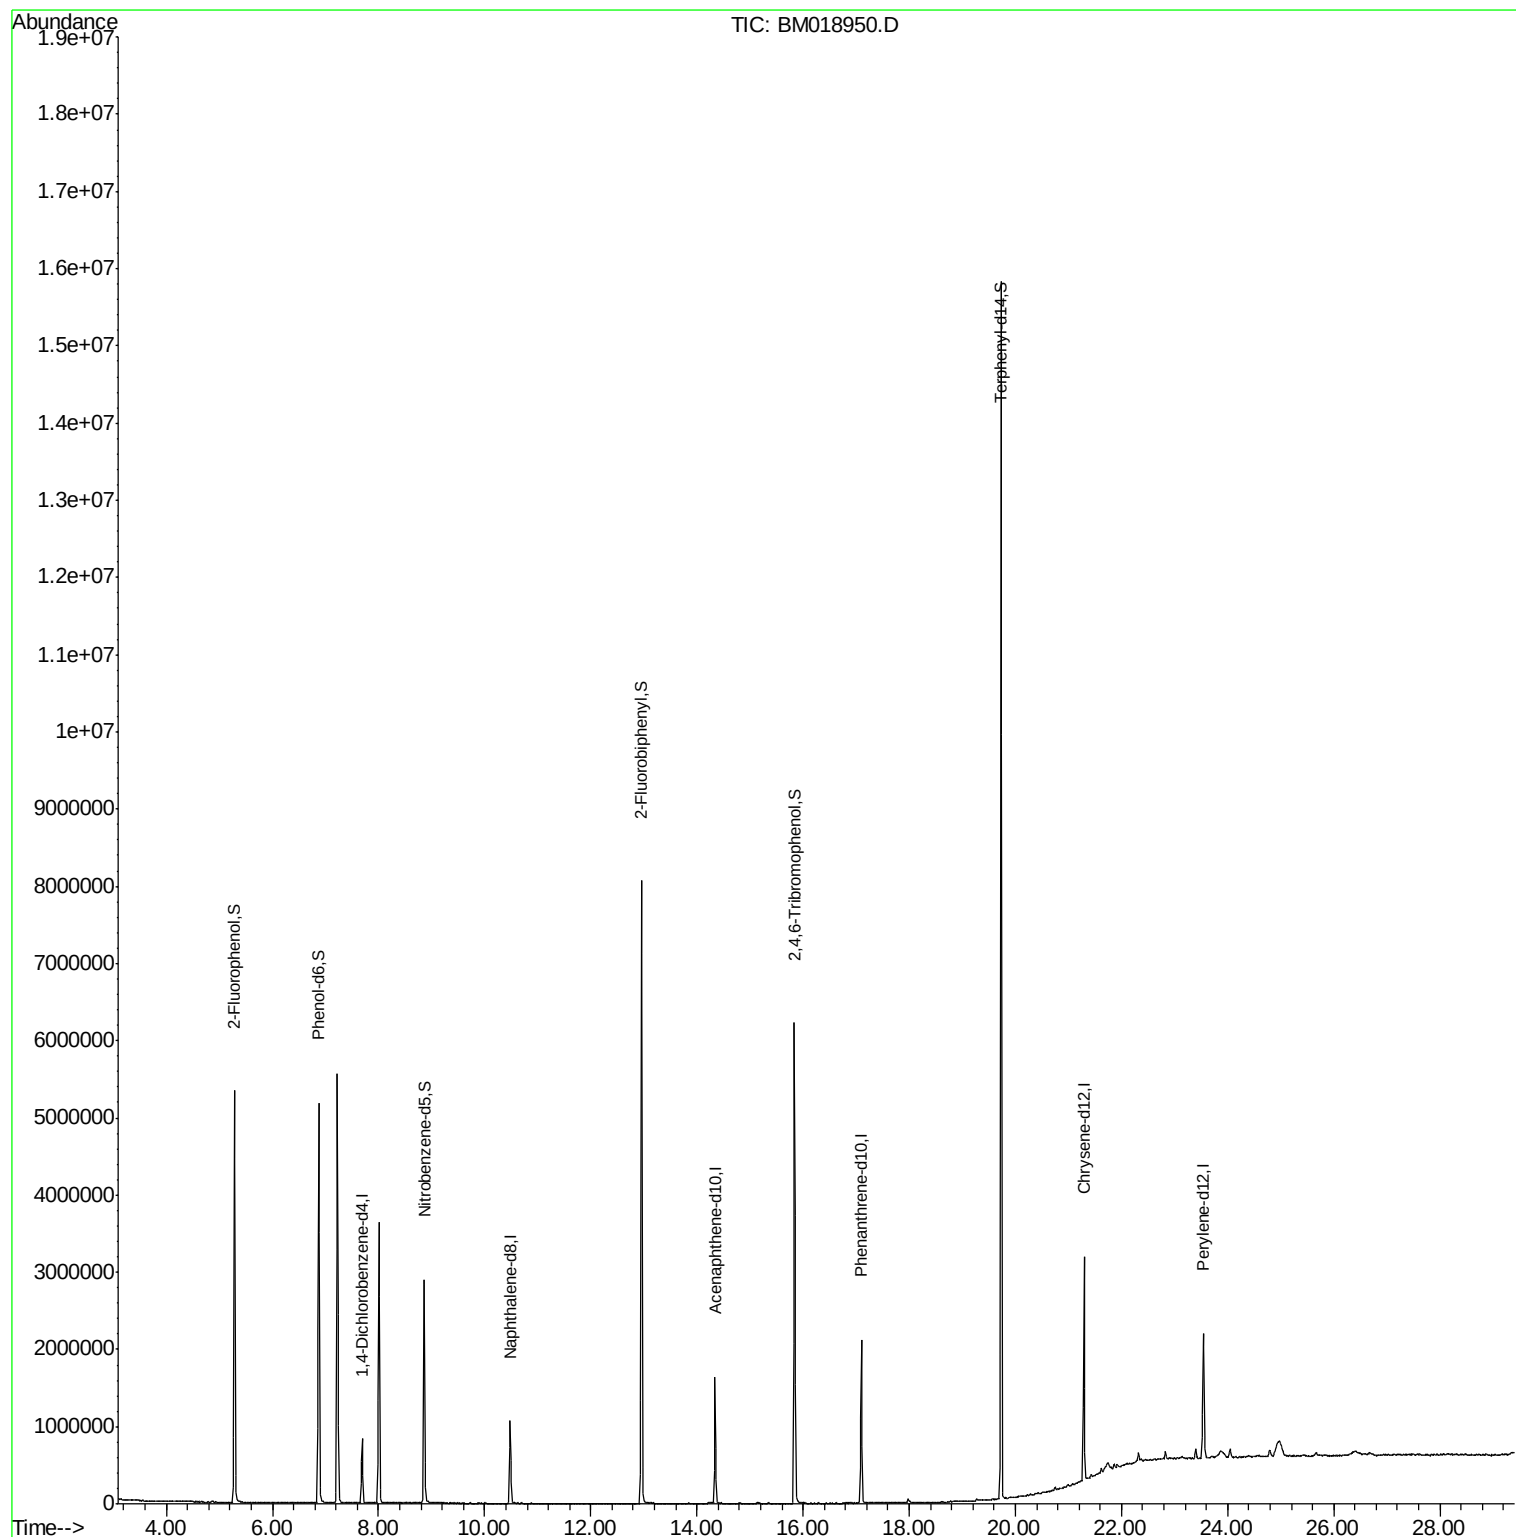




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.69 min Scan# 783
Delta R.T. -0.02 min
Lab File: BM018950.D
Acq: 27 Feb 2019 15:32

Instrument :
BNA_M
ClientSampleId :
PB117349BL

Tot Ion:152 Resp: 213683
Ion Ratio Lower Upper
152 100
150 159.1 127.3 190.9
115 62.4 50.8 76.2

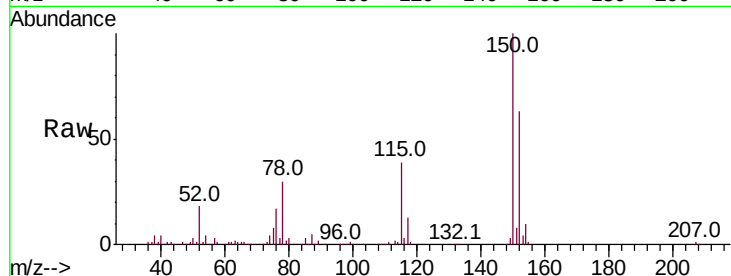


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

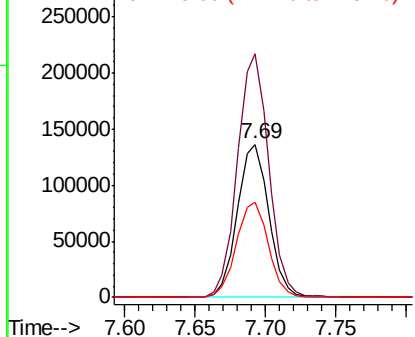



#5


2-Fluorophenol
Concen: 164.124 ng
RT: 5.29 min Scan# 374
Delta R.T. -0.02 min
Lab File: BM018950.D
Acq: 27 Feb 2019 15:32

Tgt Ion:112 Resp: 2140431
Ion Ratio Lower Upper
112 100
64 64.1 50.6 75.8
63 32.2 25.7 38.5



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 63.00 (62.70 to 63.70): BM0

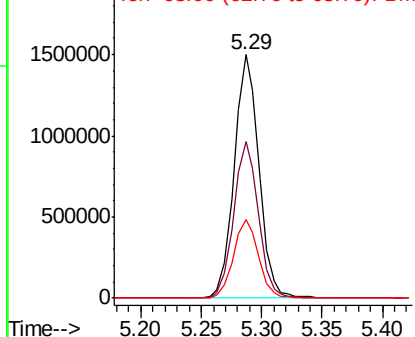



#7

Phenol-d6

Concen: 166.905 ng

RT: 6.87 min Scan# 643

Delta R.T. -0.02 min

Lab File: BM018950.D

Acq: 27 Feb 2019 15:32

Instrument :

BNA_M

ClientSampleId :

PB117349BL


Tot Ion: 99 Resp: 3066448

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.6

71 38.4 31.3 46.9




Abundance Ion 99.00 (98.70 to 99.70): BM018755.D (-637) (-)

Ion 42.00 (41.70 to 42.70): BM018755.D (-637) (-)

Ion 71.00 (70.70 to 71.70): BM018755.D (-637) (-)

6.87

Time-->




Abundance Ion 99.00 (98.70 to 99.70): BM018950.D (-629) (-)

Ion 42.00 (41.70 to 42.70): BM018950.D (-629) (-)

Ion 71.00 (70.70 to 71.70): BM018950.D (-629) (-)

6.87

Time-->



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.48 min Scan# 1257

Delta R.T. -0.02 min

Lab File: BM018950.D

Acq: 27 Feb 2019 15:32

Tgt Ion: 136 Resp: 891358


Ion Ratio Lower Upper

136 100

137 11.1 8.8 13.2

54 7.1 5.0 7.6

68 7.7 5.5 8.3



Abundance Ion 136.00 (135.70 to 136.70): BM018755.D (-1252) (-)


Ion 137.00 (136.70 to 137.70): BM018755.D (-1252) (-)

Ion 54.00 (53.70 to 54.70): BM018755.D (-1252) (-)

Ion 68.00 (67.70 to 68.70): BM018755.D (-1252) (-)

10.48

Time-->



Abundance Ion 136.00 (135.70 to 136.70): BM018950.D (-1244) (-)


Ion 137.00 (136.70 to 137.70): BM018950.D (-1244) (-)

Ion 54.00 (53.70 to 54.70): BM018950.D (-1244) (-)

Ion 68.00 (67.70 to 68.70): BM018950.D (-1244) (-)

10.48


Time-->






#23
Nitrobenzene-d5
Concen: 99.275 ng
RT: 8.86 min Scan# 982
Delta R.T. -0.02 min
Lab File: BM018950.D
Acq: 27 Feb 2019 15:32

Instrument :
BNA_M
ClientSampleId :
PB117349BL

Tot Ion: 82 Resp: 1913749
Ion Ratio Lower Upper
82 100
128 37.6 29.9 44.9
54 36.6 29.1 43.7

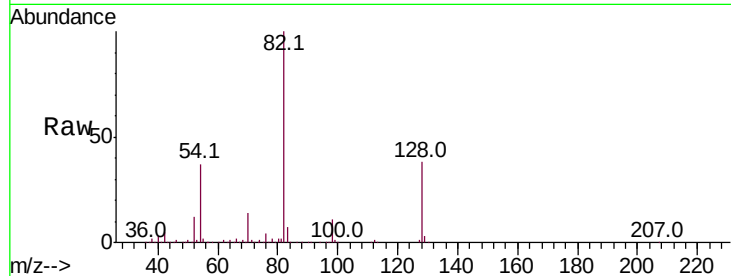


Abundance Ion 82.00 (81.70 to 82.70): BM018755.D (-976) (-)
Ion 128.00 (127.70 to 128.70): BM018755.D (-976) (-)
Ion 54.00 (53.70 to 54.70): BM018755.D (-976) (-)


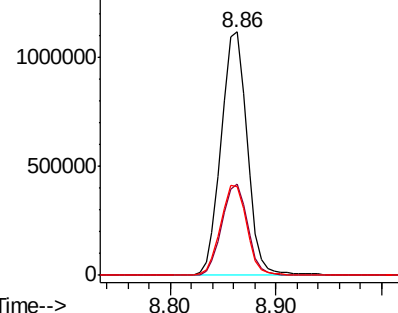



#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.34 min Scan# 1914
Delta R.T. -0.02 min
Lab File: BM018950.D
Acq: 27 Feb 2019 15:32

Tgt Ion:164 Resp: 518573
Ion Ratio Lower Upper
164 100
162 108.2 83.4 125.0
160 47.9 36.6 55.0

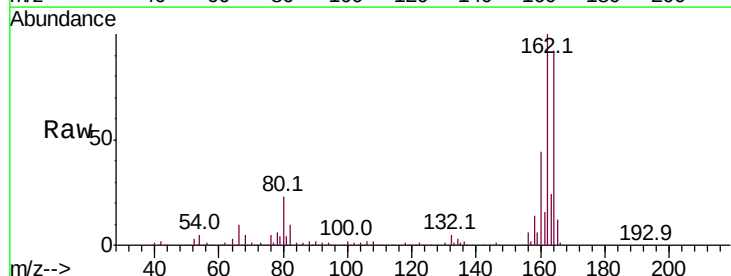

Abundance Ion 164.00 (163.70 to 164.70): BM018755.D (-1910) (-)
Ion 162.00 (161.70 to 162.70): BM018755.D (-1910) (-)
Ion 160.00 (159.70 to 160.70): BM018755.D (-1910) (-)

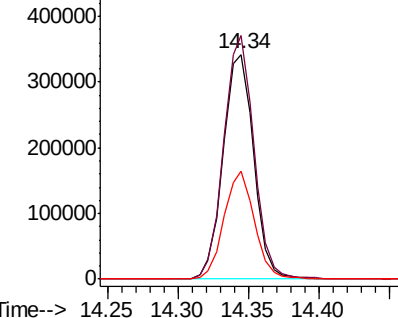







#42
 2,4,6-Tribromophenol
 Concen: 154.736 ng
 RT: 15.84 min Scan# 2169
 Delta R.T. -0.02 min
 Lab File: BM018950.D
 Acq: 27 Feb 2019 15:32

Instrument :
 BNA_M
 ClientSampleId :
 PB117349BL

Tot Ion:330 Resp: 1156668
 Ion Ratio Lower Upper
 330 100
 332 96.7 76.9 115.3
 141 34.5 28.7 43.1

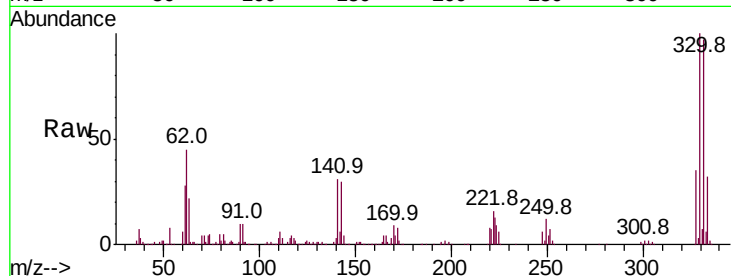


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


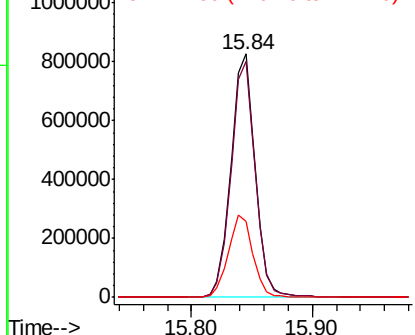



#45
 2-Fluorobiphenyl
 Concen: 100.587 ng
 RT: 12.96 min Scan# 1678
 Delta R.T. -0.02 min
 Lab File: BM018950.D
 Acq: 27 Feb 2019 15:32

Tgt Ion:172 Resp: 3929379
 Ion Ratio Lower Upper
 172 100
 171 36.1 29.0 43.6
 170 23.6 18.6 28.0



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

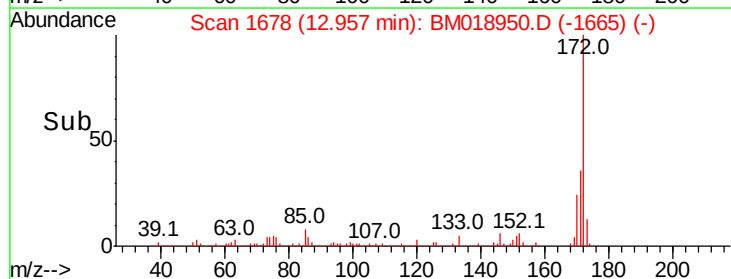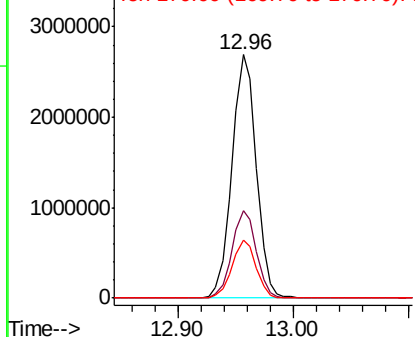

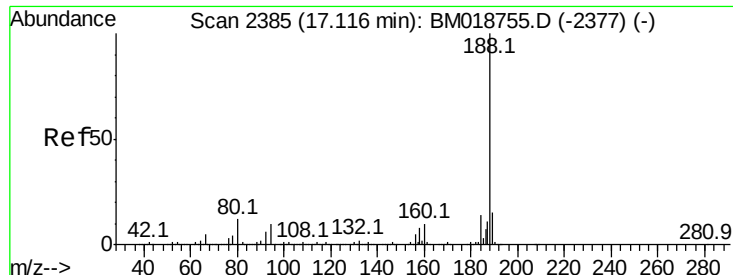

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.10 min Scan# 2382

Delta R.T. -0.02 min

Lab File: BM018950.D

Acq: 27 Feb 2019 15:32

Instrument :

BNA_M

ClientSampleId :

PB117349BL


Tot Ion:188 Resp: 1149780

Ion Ratio Lower Upper

188 100

94 10.1 8.2 12.2




80 12.0 9.7 14.5

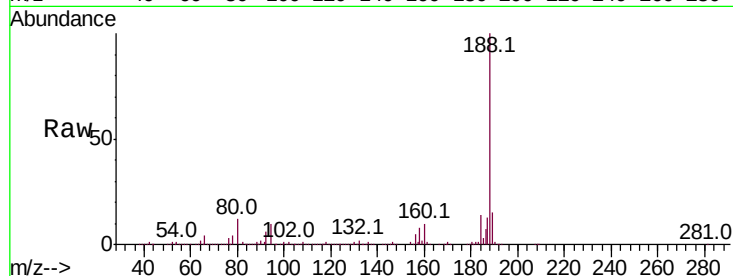

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM

Ion 80.00 (79.70 to 80.70): BM

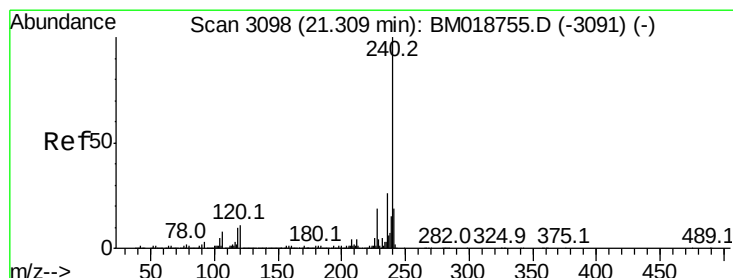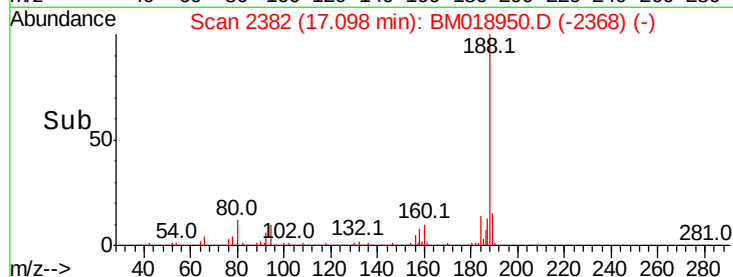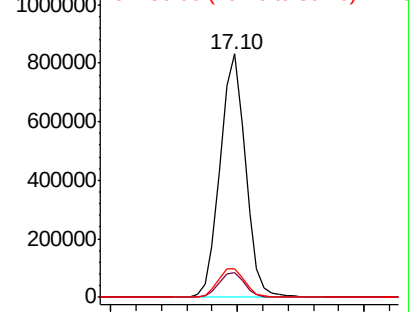

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.29 min Scan# 3095

Delta R.T. -0.02 min

Lab File: BM018950.D

Acq: 27 Feb 2019 15:32


Tgt Ion:240 Resp: 1243053

Ion Ratio Lower Upper

240 100

120 11.8 8.9 13.3



236 25.3 20.9 31.3

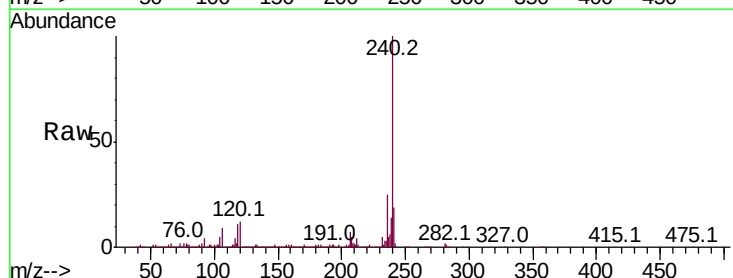


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

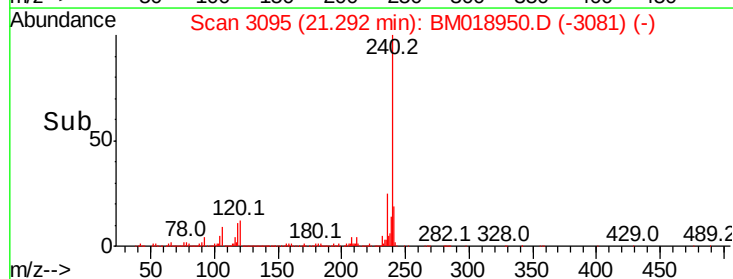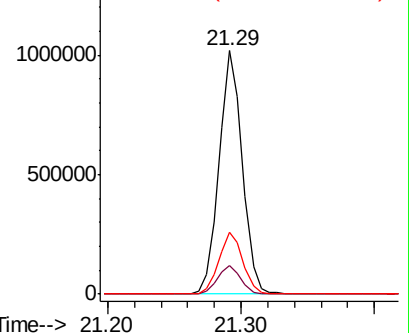



#79

Terphenyl-d14

Concen: 104.813 ng

RT: 19.73 min Scan# 2830

Delta R.T. -0.01 min

Lab File: BM018950.D

Acq: 27 Feb 2019 15:32

Instrument :

BNA_M

ClientSampleId :

PB117349BL


Tot Ion:244 Resp: 6315762

Ion Ratio Lower Upper

244 100

212 6.9 5.6 8.4




122 11.3 9.3 13.9



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

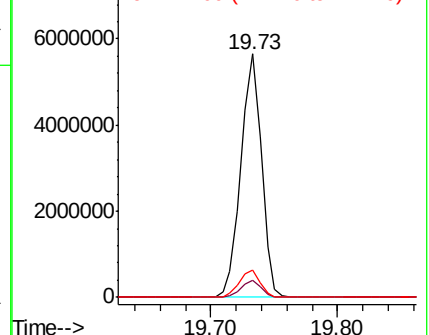

#87

Perylene-d12

Concen: 20.000 ng

RT: 23.54 min Scan# 3478

Delta R.T. -0.02 min

Lab File: BM018950.D

Acq: 27 Feb 2019 15:32


Tgt Ion:264 Resp: 1096683

Ion Ratio Lower Upper

264 100

260 24.3 18.9 28.3

265 21.8 17.3 25.9



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

