


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022719\
 Data File : BM018946.D
 Acq On : 27 Feb 2019 12:25
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

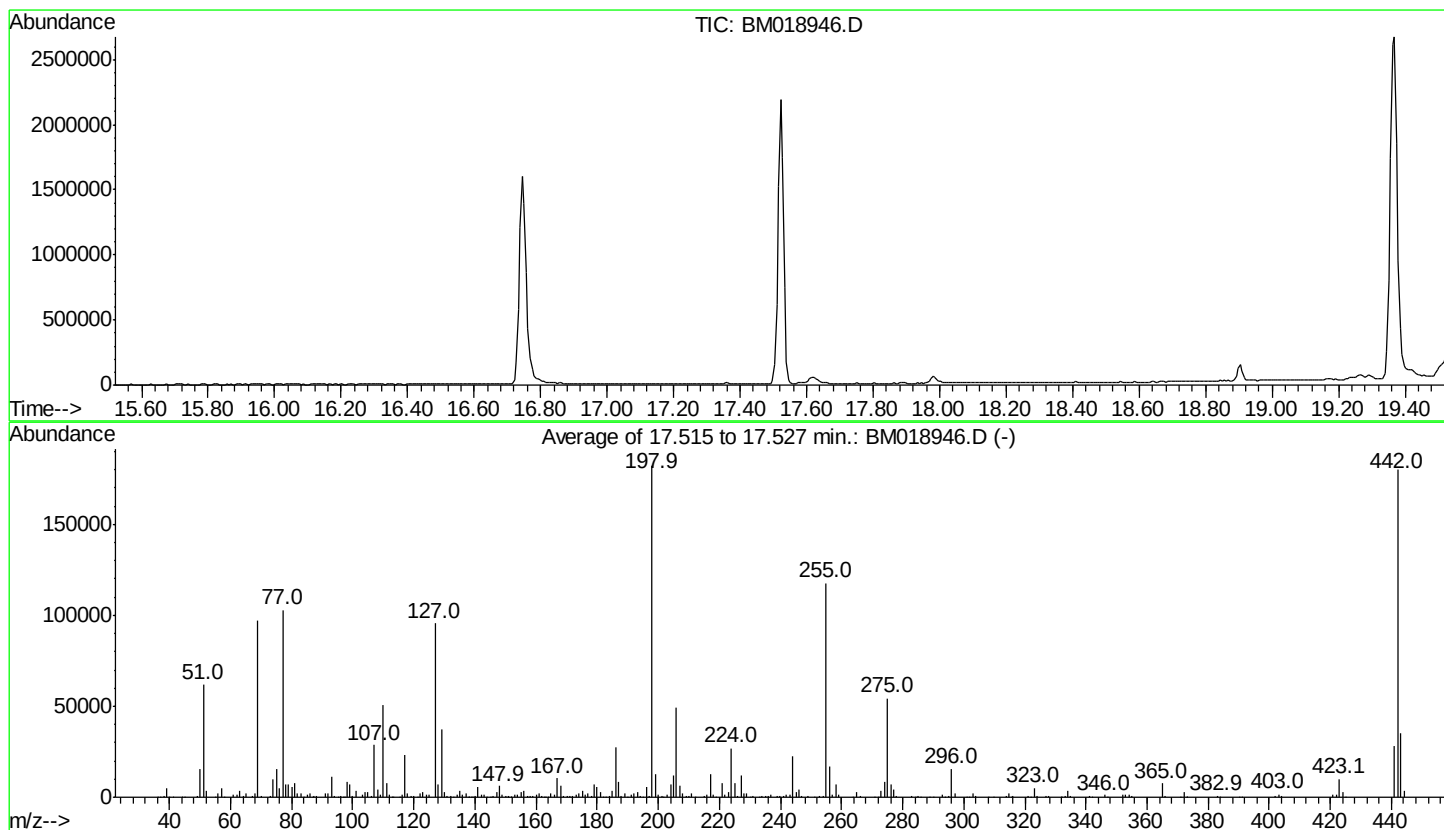

AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	61656	PASS
68	69	0.00	2	2.0	1929	PASS
69	198	0.00	100	53.2	97008	PASS
70	69	0.00	2	0.7	710	PASS
127	198	10	80	52.4	95408	PASS
197	198	0.00	2	0.6	1014	PASS
198	198	100	100	100.0	182229	PASS
199	198	5	9	6.9	12515	PASS
275	198	10	60	29.8	54309	PASS
365	198	1	100	4.1	7459	PASS
441	198	0.01	100	15.4	28061	PASS
442	198	50	100	98.8	180013	PASS
443	442	15	24	19.7	35392	PASS