

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022720\
 Data File : BM025121.D
 Acq On : 28 Feb 2020 01:51
 Operator : CG/JU
 Sample : L1582-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Feb 28 04:27:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2372	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.46	136	9202	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.32	164	5933	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.07
16) Chrysene-d12	21.24	240	13751	0.40	ng/ul	-0.01
20) Perylene-d12	23.44	264	15913	0.40	ng/ul	-0.02
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	5477	0.32	ng/ul	-0.01
14) Fluoranthene-d10	19.09	212	17016	0.00	ng/ul	-0.01
Target Compounds						
3) Naphthalene	10.51	128	7834	0.280	ng/ul#	84
5) 2-Methylnaphthalene	12.12	142	761	0.038	ng/ul	97
17) Pyrene	19.45	202	2742	0.044	ng/ul#	1
23) Benzo(a)pyrene	23.30	252	6014	0.106	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022720\
Data File : BM025121.D
Acq On : 28 Feb 2020 01:51
Operator : CG/JU
Sample : L1582-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Feb 28 04:27:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

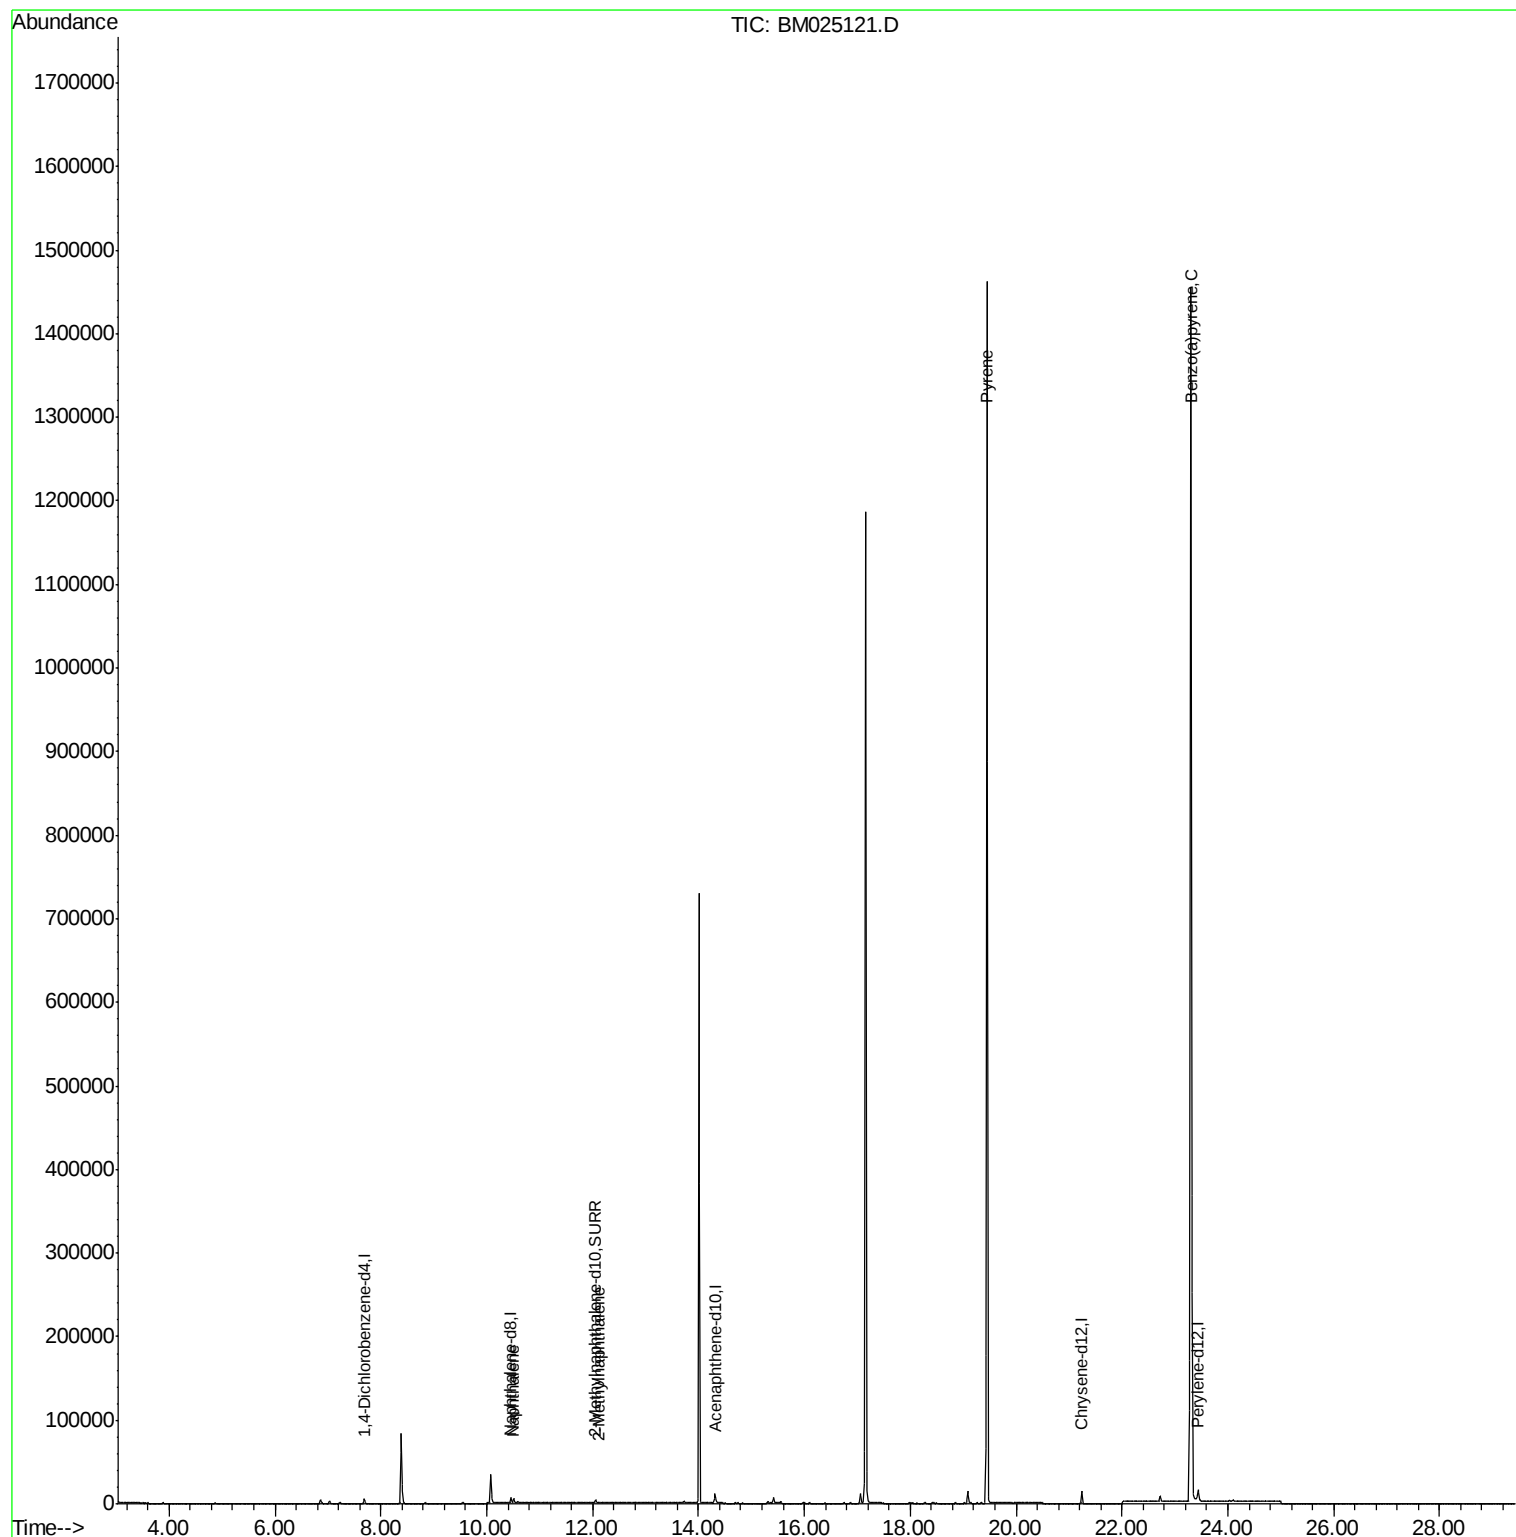

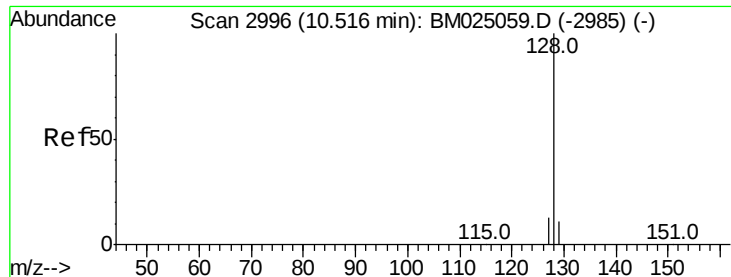

#3

Naphthalene

Concen: 0.280 ng/ul

RT: 10.51 min Scan# 2995

Delta R.T. -0.01 min

Lab File: BM025121.D

Acq: 28 Feb 2020 01:51

Instrument :

BNA_M

ClientSampleId :


Tot Ion:128 Resp: 7834

Ion Ratio Lower Upper

128 100

129 12.5 17.0 25.6#




127 13.7 15.7 23.5#

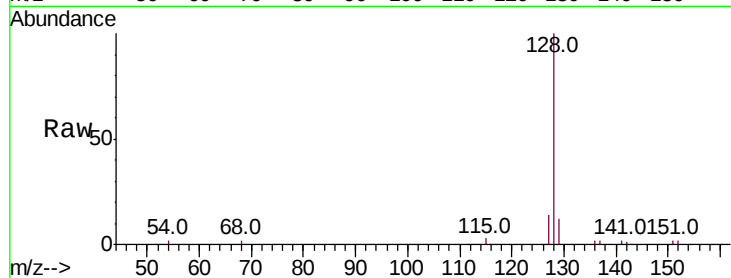

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

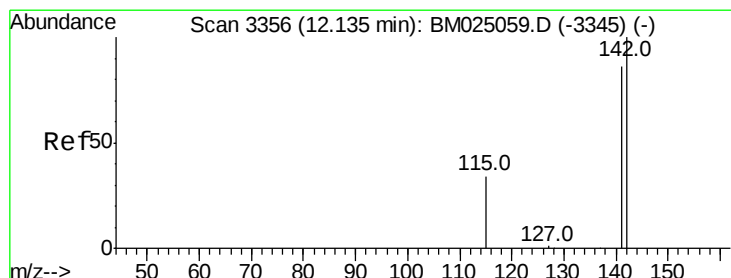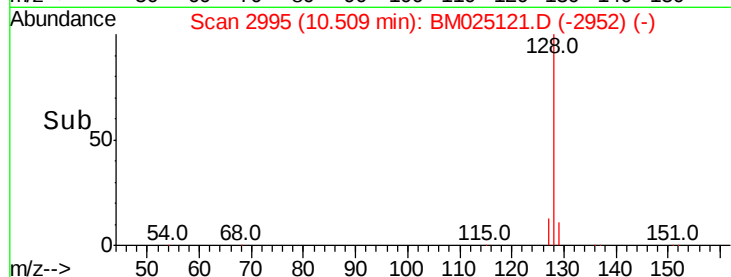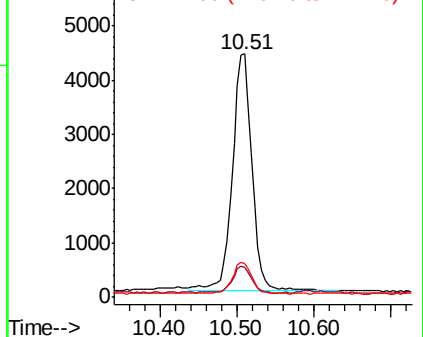

#5

2-Methylnaphthalene

Concen: 0.038 ng/ul

RT: 12.12 min Scan# 3354

Delta R.T. -0.02 min

Lab File: BM025121.D


Acq: 28 Feb 2020 01:51

Tgt Ion:142 Resp: 761

Ion Ratio Lower Upper



142 100


141 89.9 69.8 104.8

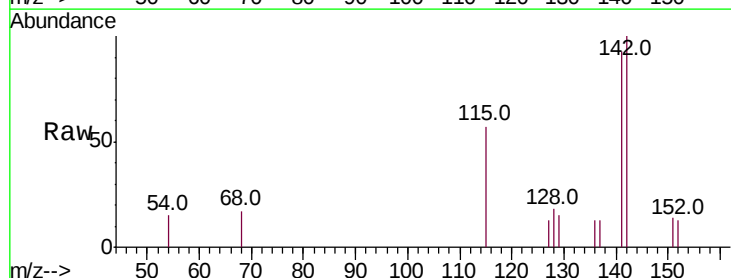

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

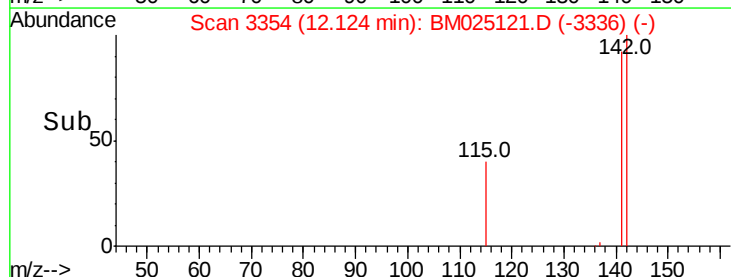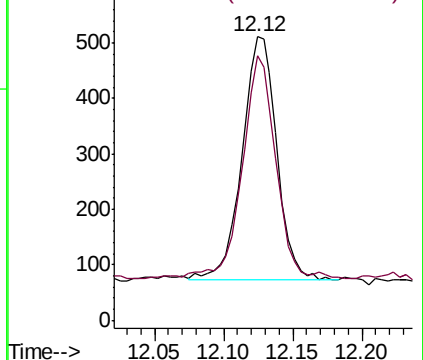

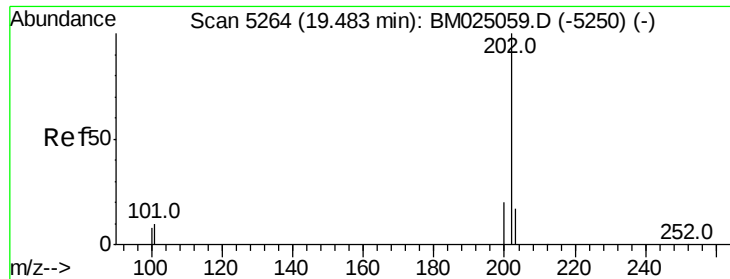

#17

Pvrene

Concen: 0.044 ng/ul

RT: 19.45 min Scan# 5256

Delta R.T. -0.04 min

Lab File: BM025121.D

Acq: 28 Feb 2020 01:51

Instrument :

BNA_M

ClientSampled :


Tot Ion:202 Resp: 2742

Ion Ratio Lower Upper

202 100

101 140.3 8.7 13.1#




100 958.4 7.3 10.9#

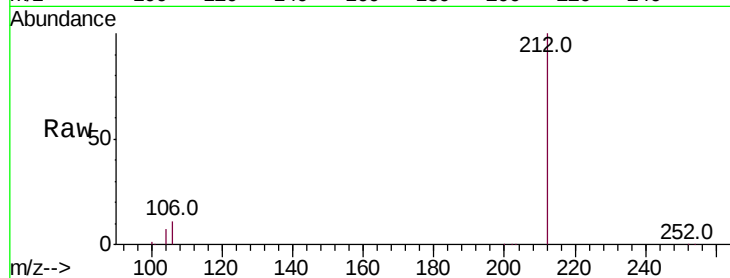

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

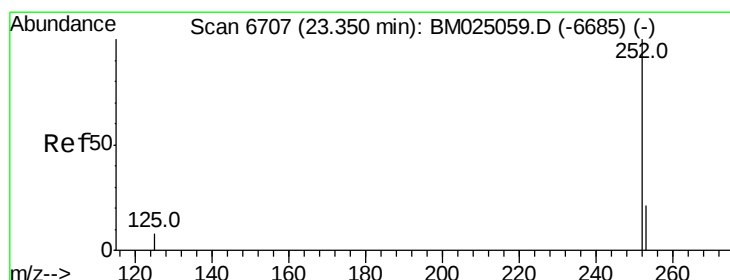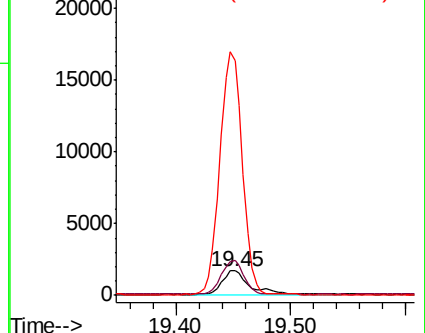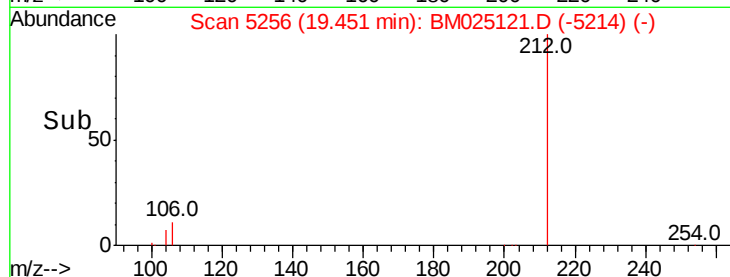

#23

Benzo(a)pyrene

Concen: 0.106 ng/ul

RT: 23.30 min Scan# 6688

Delta R.T. -0.06 min

Lab File: BM025121.D

Acq: 28 Feb 2020 01:51


Tgt Ion:252 Resp: 6014

Ion Ratio Lower Upper

252 100

253 35.1 20.3 30.5#

125 24.8 13.0 19.4#

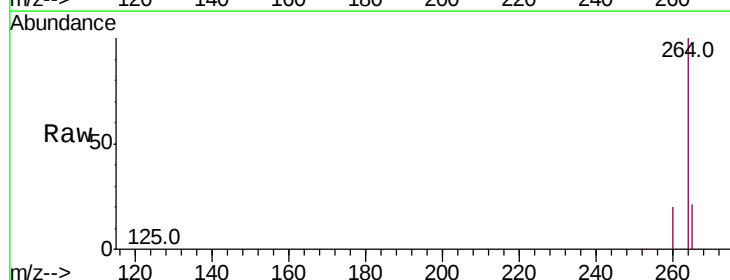

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

