




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022720\
Data File : BM025124.D
Acq On : 28 Feb 2020 03:39
Operator : CG/JU
Sample : SP5066
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP5066

Manual Integrations
APPROVED

mohammad
2/28/2020 2:41:15 PM

Quant Time: Feb 28 04:27:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

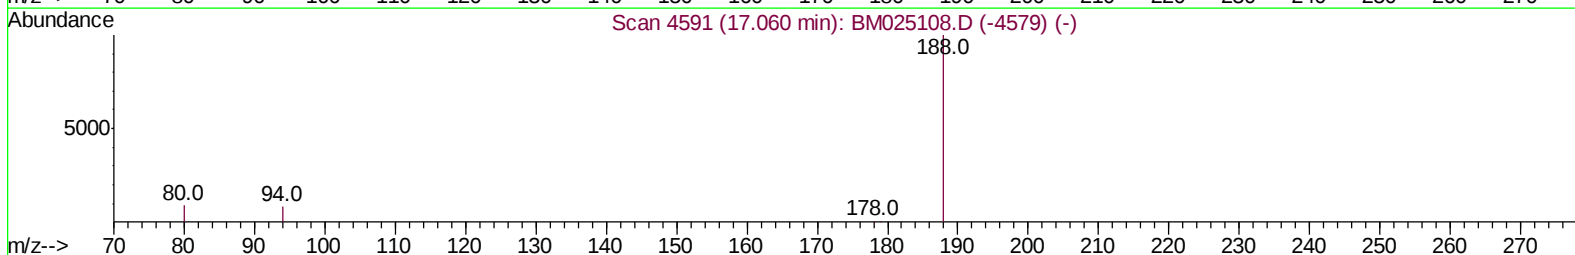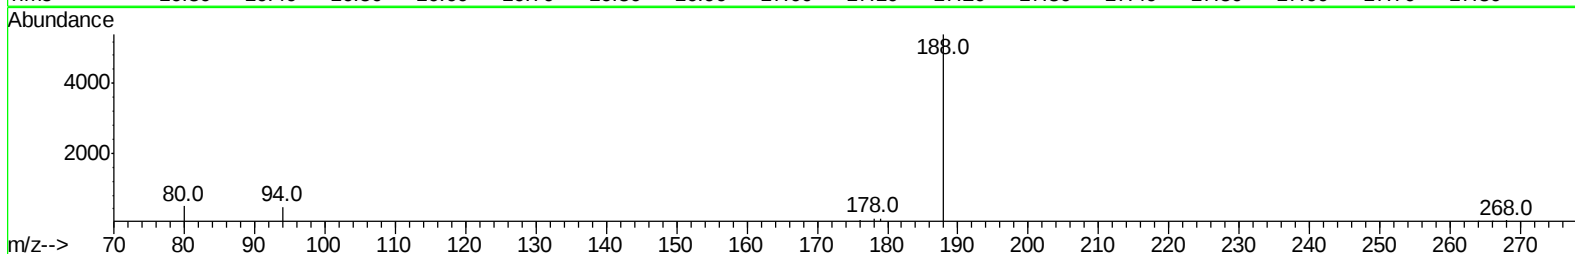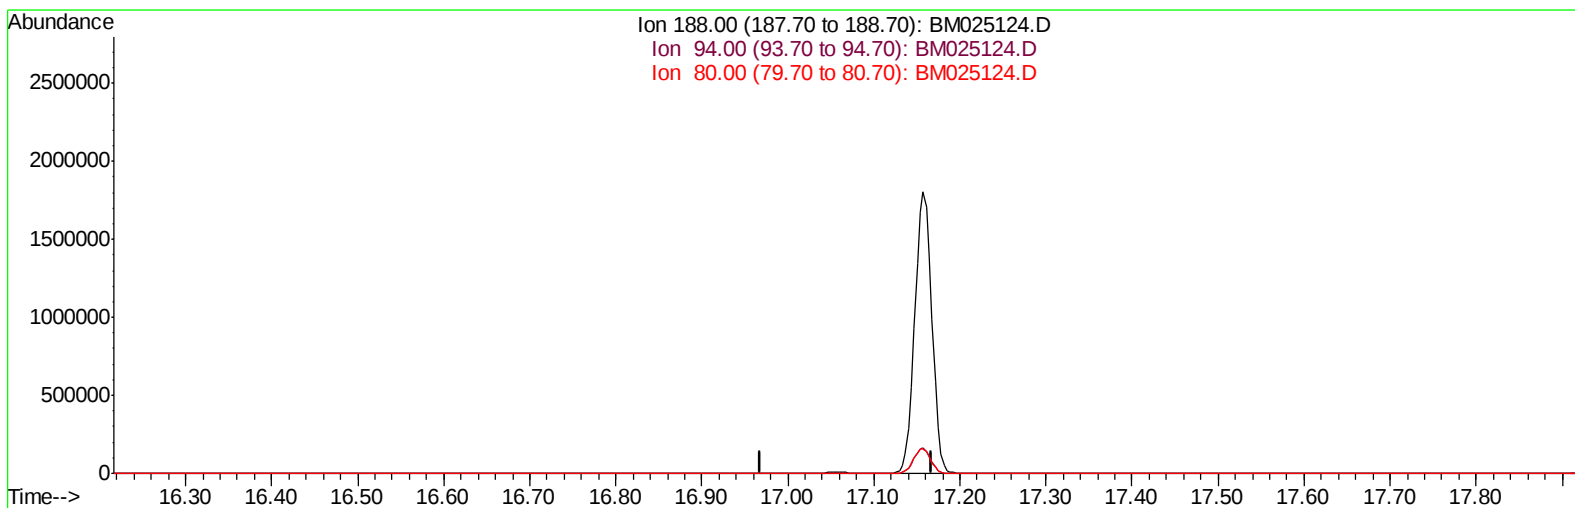

TIC: BM025124.D

(10) Phenanthrene-d10 (I)

17.068min (-17.068) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022720\
Data File : BM025124.D
Acq On : 28 Feb 2020 03:39
Operator : CG/JU
Sample : SP5066
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP5066

Manual Integrations
APPROVED

mohammad
2/28/2020 2:41:15 PM

Quant Time: Feb 28 04:27:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

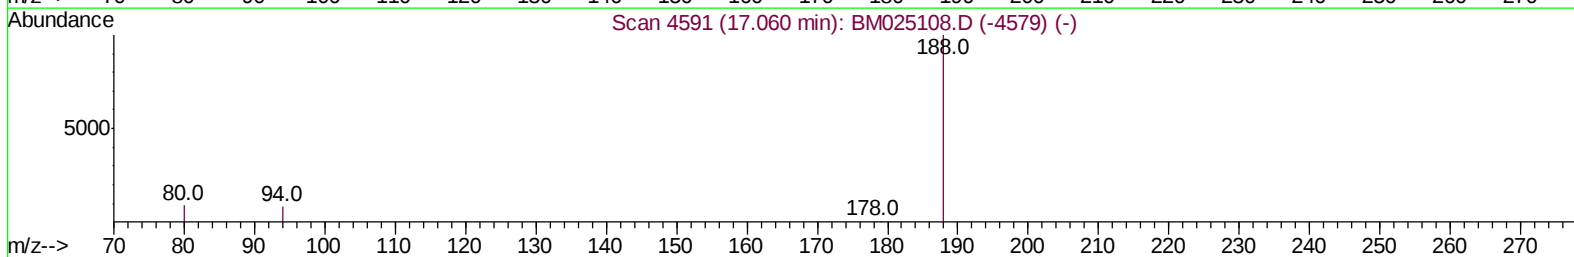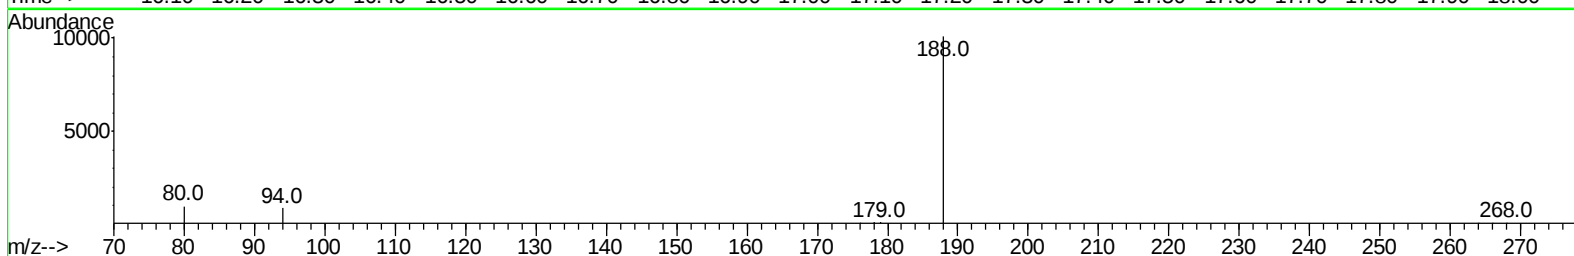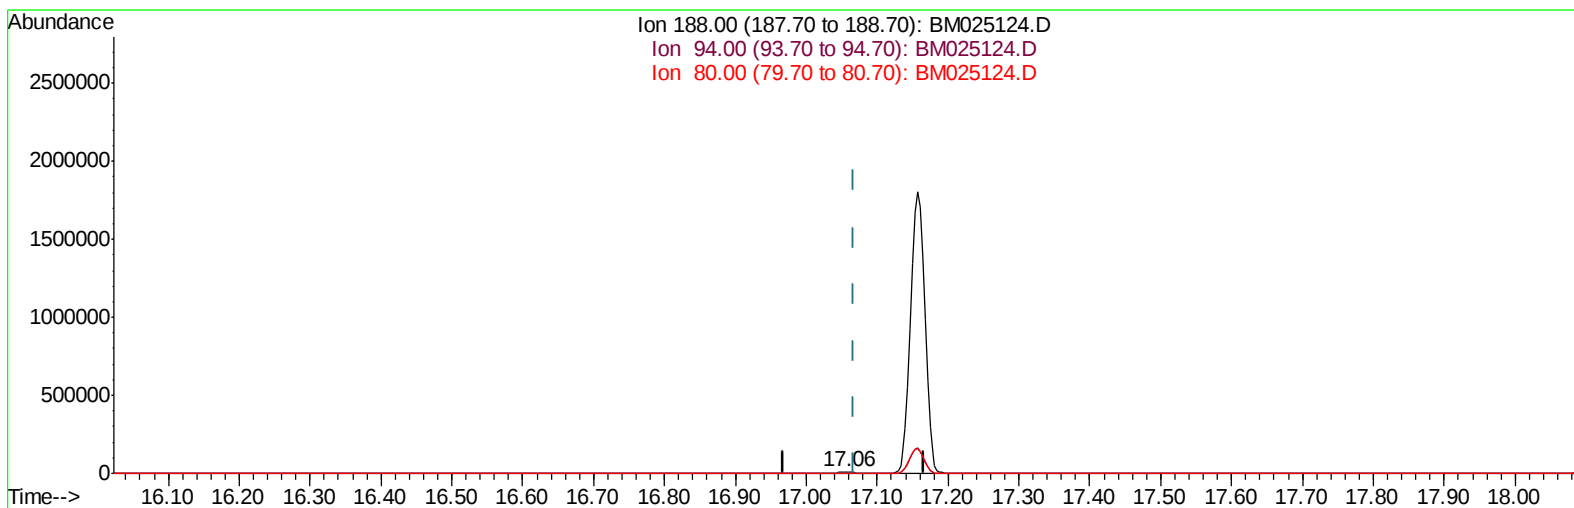

TIC: BM025124.D

(10) Phenanthrene-d10 (I)

17.056min (-0.012) 0.40ng/ul m

response 13485

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.64#
80.00	22.60	9.64#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022720\
 Data File : BM025124.D
 Acq On : 28 Feb 2020 03:39
 Operator : CG/JU
 Sample : SP5066
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SP5066

Manual Integrations
 APPROVED

mohammad
 2/28/2020 2:41:15 PM

Quant Time: Feb 28 06:21:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 25 11:03:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2349	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.46	136	9124	0.40	ng/ul	-0.02
6) Acenaphthene-d10	14.32	164	6266	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	13485m	0.40	ng/ul	-0.01
16) Chrysene-d12	21.24	240	13711	0.40	ng/ul	-0.01
20) Perylene-d12	23.44	264	16246	0.40	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.05	152	12527	0.73	ng/ul	-0.01
14) Fluoranthene-d10	19.09	212	31230	0.68	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022720\
Data File : BM025124.D
Acq On : 28 Feb 2020 03:39
Operator : CG/JU
Sample : SP5066
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SP5066

Manual Integrations
APPROVED

mohammad
2/28/2020 2:41:15 PM

Quant Time: Feb 28 06:21:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 25 11:03:43 2020
Response via : Initial Calibration

