
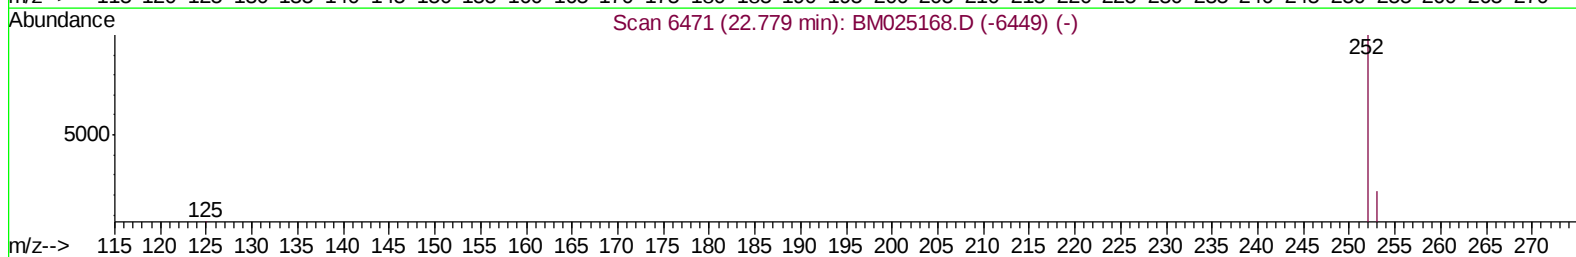
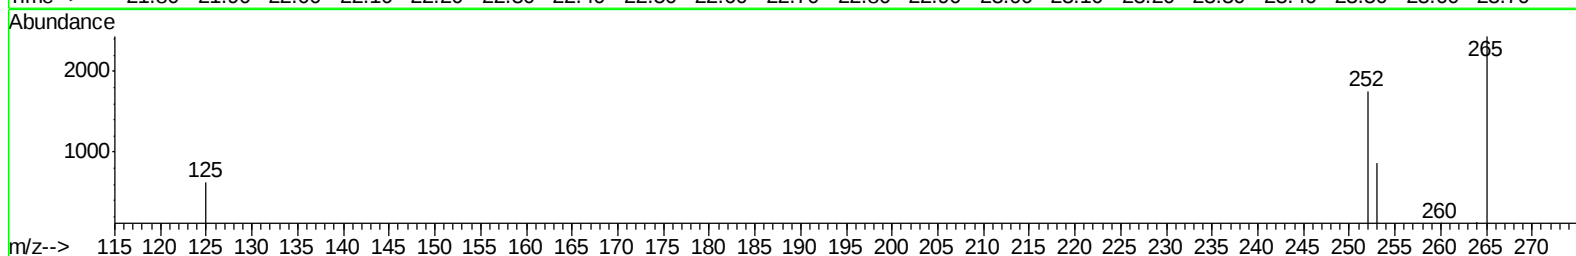


Data File : BM025169.D
Acq On : 29 Feb 2020 15:42
Operator : CG/JU
Sample : L1542-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Quant Time: Mar 02 02:41:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

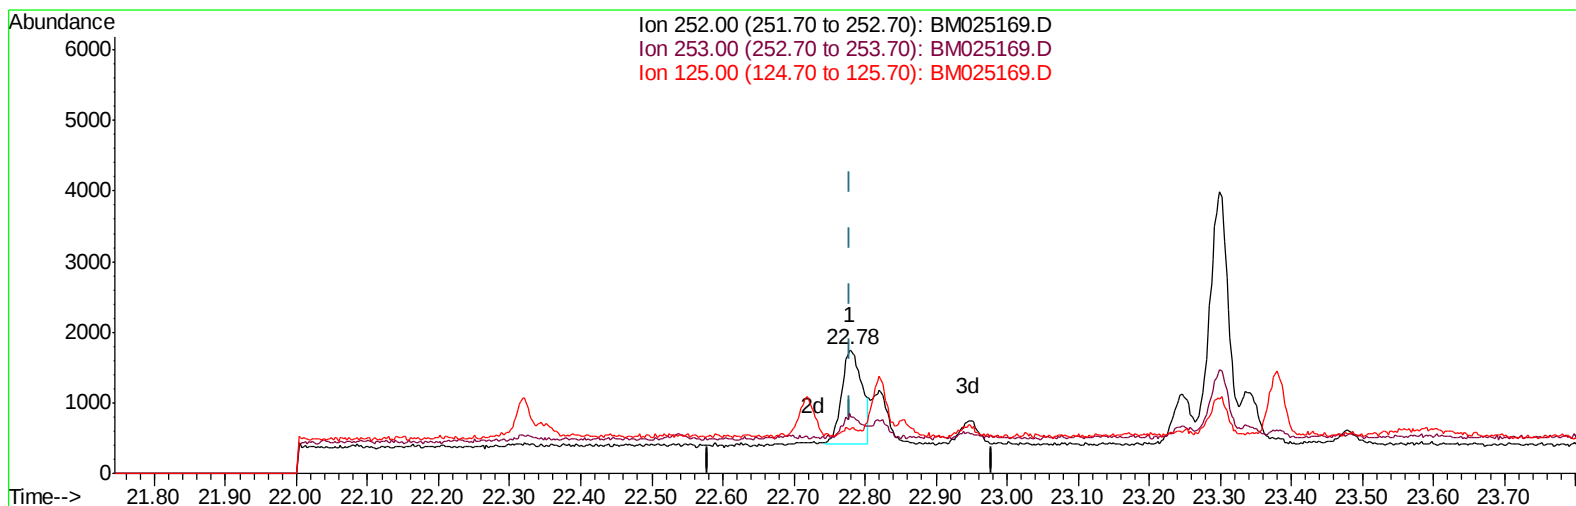

TIC: BM025169.D

(21) Benzo(b)fluoranthene

22.779min (-0.000) 0.04ng/ul m

response 2585

Ion	Exp%	Act%
252.00	100	100
253.00	24.90	49.17
125.00	14.30	35.64#
0.00	0.00	0.00