
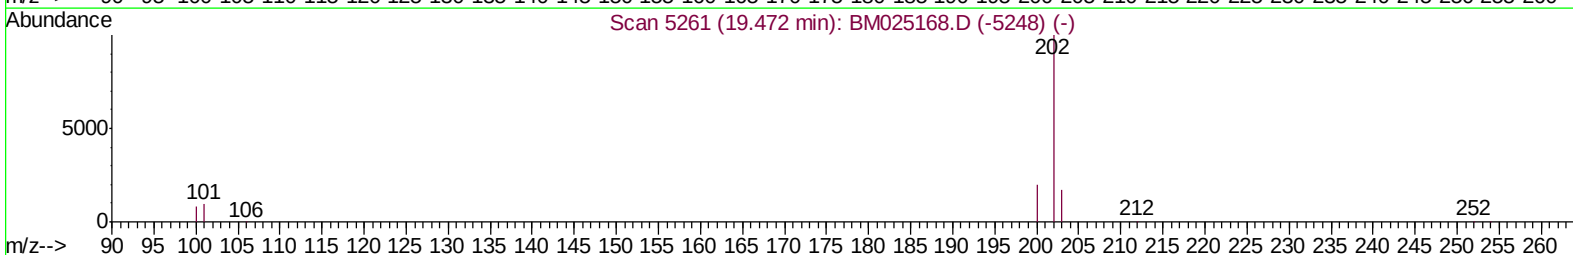
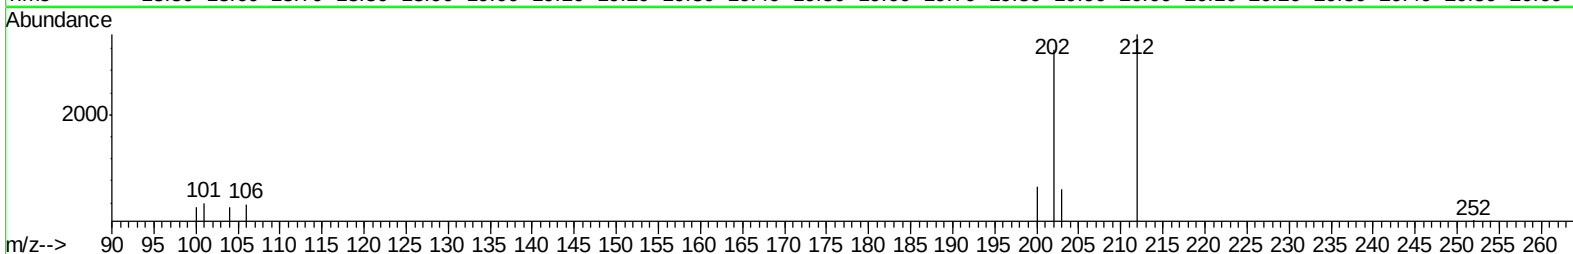


Data File : BM025177.D
Acq On : 29 Feb 2020 20:28
Operator : CG/JU
Sample : L1542-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Mar 02 02:11:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

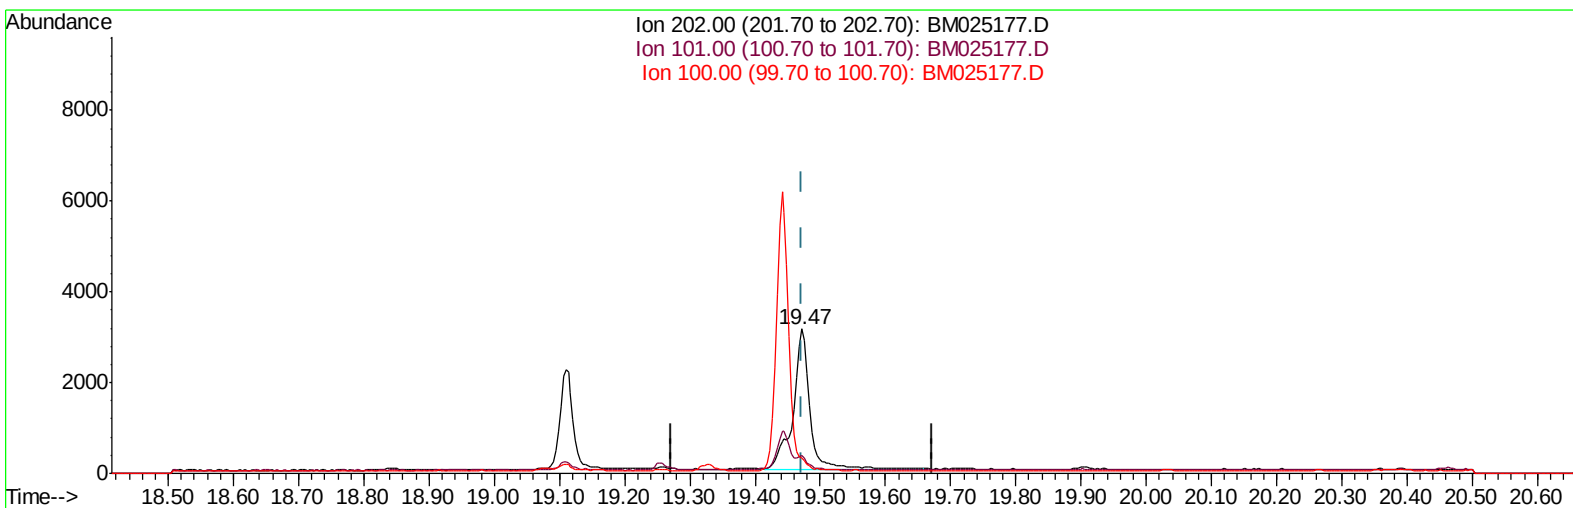

TIC: BM025177.D

(17) Pyrene

19.472min (-0.000) 0.07ng/ul

response 5437

Ion	Exp%	Act%
202.00	100	100
101.00	10.90	12.34
100.00	9.10	10.36
0.00	0.00	0.00