
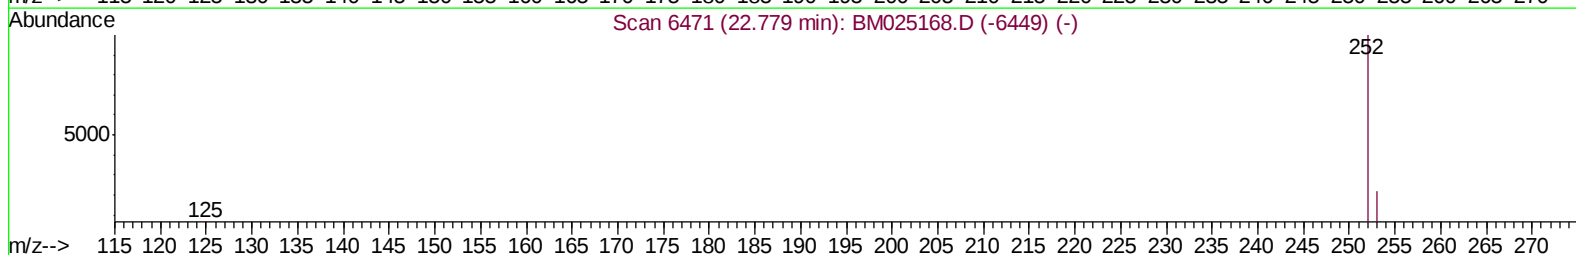
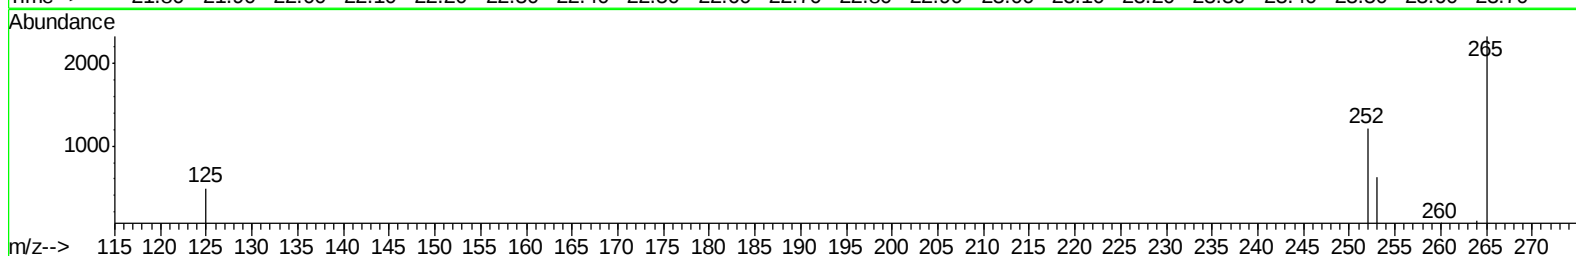


Data File : BM025177.D
Acq On : 29 Feb 2020 20:28
Operator : CG/JU
Sample : L1542-16
Misc :
ALS Vial : 50 Sample Multiplier: 1

Quant Time: Mar 02 02:11:05 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

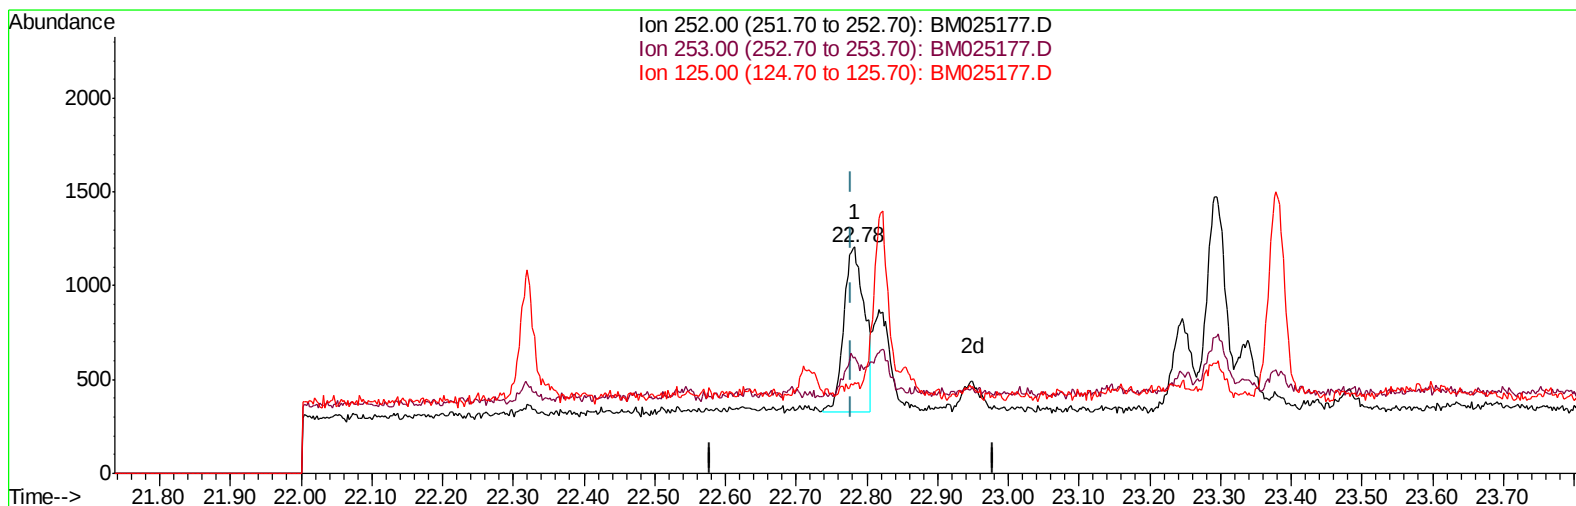

TIC: BM025177.D

(21) Benzo(b)fluoranthene

22.783min (+0.004) 0.02ng/ul m

response 1761

Ion	Exp%	Act%
252.00	100	100
253.00	24.90	51.33#
125.00	14.30	40.22#
0.00	0.00	0.00