

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Not Reviewed)

Data File : BM025136.D
Acq On : 28 Feb 2020 16:56
Operator : CG/JU
Sample : PB126835BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Quant Time: Feb 29 04:45:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2194	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	8316	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	5456	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.06
16) Chrysene-d12	21.24	240	12107	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	14339	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	5137	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	13175	0.00	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.30	252	4873	0.095	ng/ul#	Qvalue 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025136.D
Acq On : 28 Feb 2020 16:56
Operator : CG/JU
Sample : PB126835BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK36

Quant Time: Feb 29 04:45:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

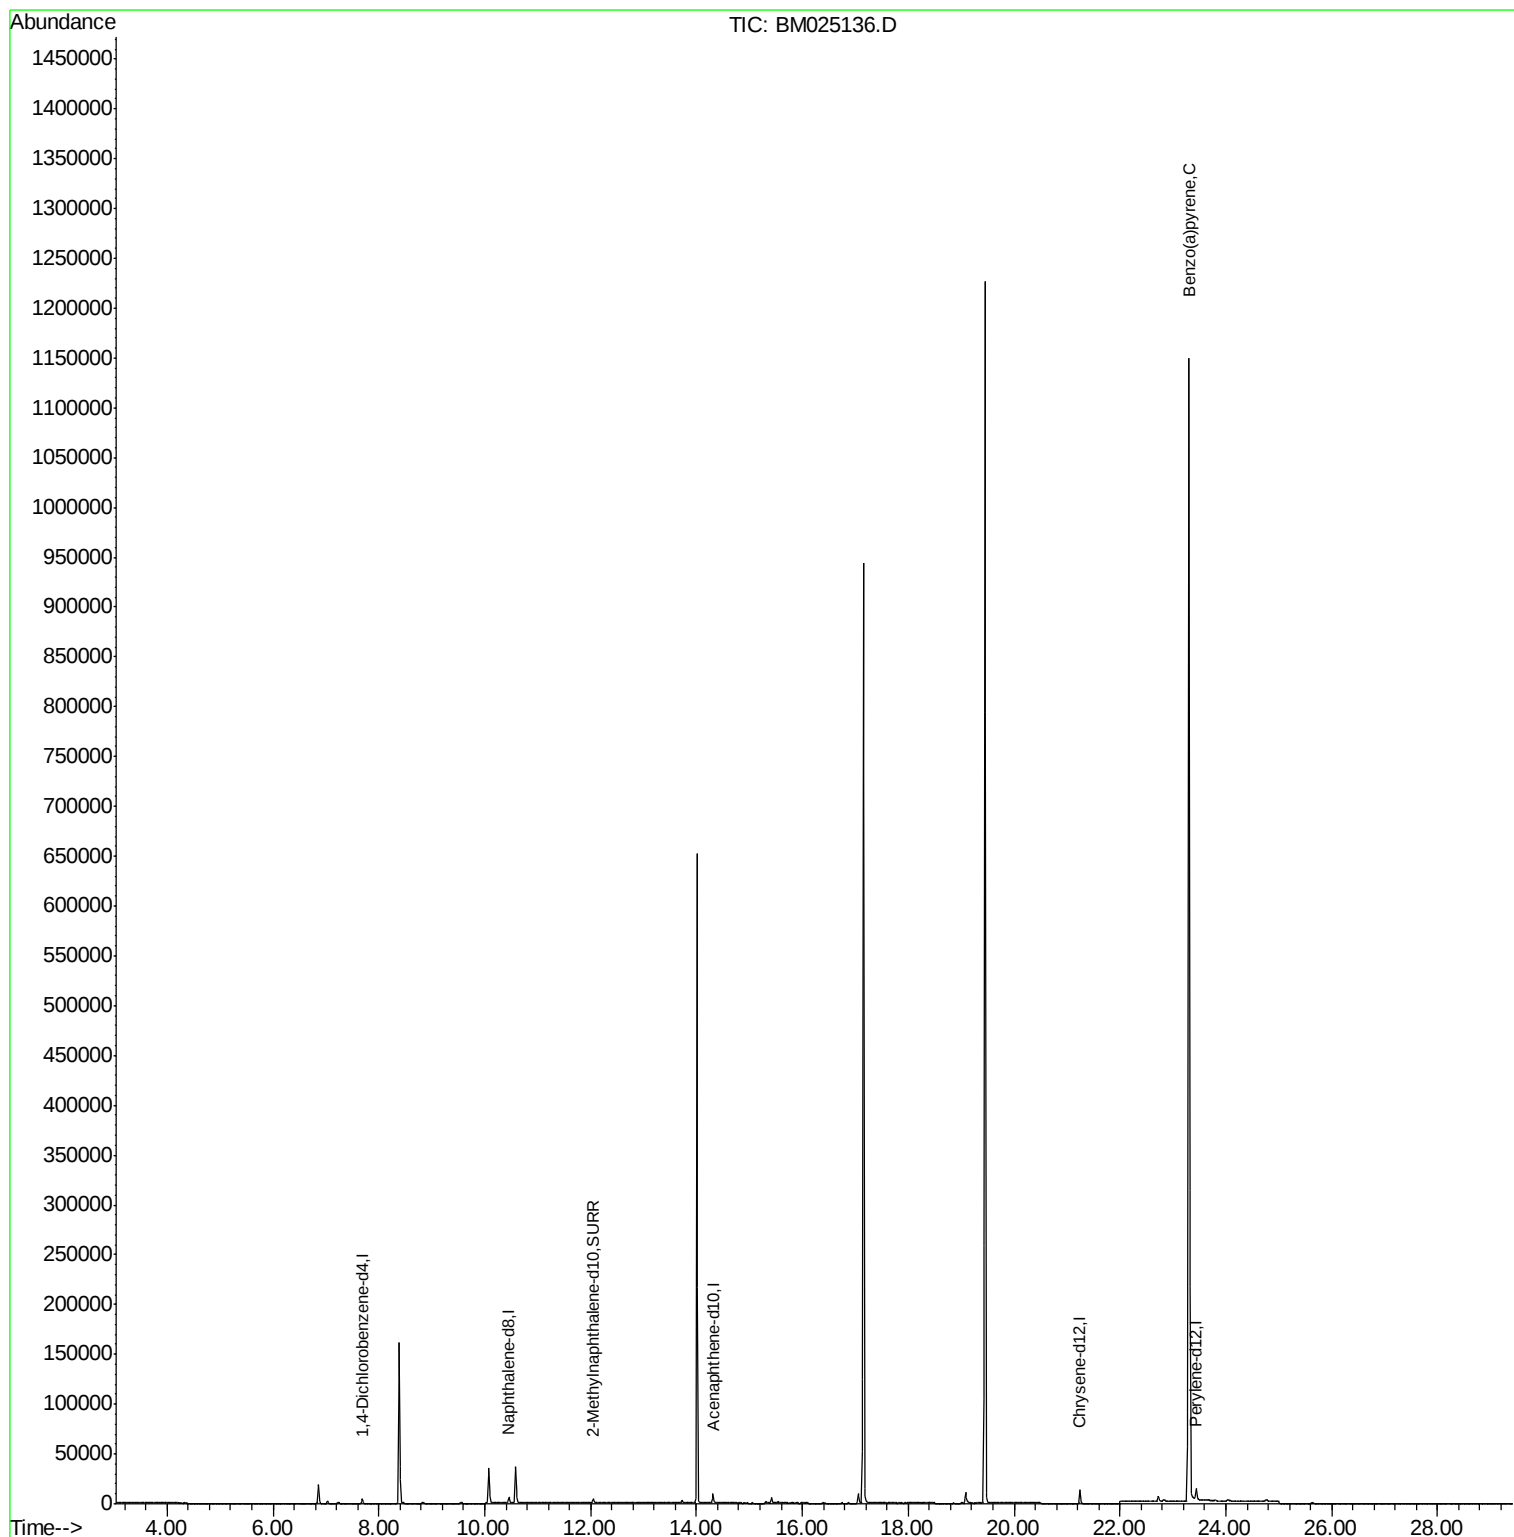

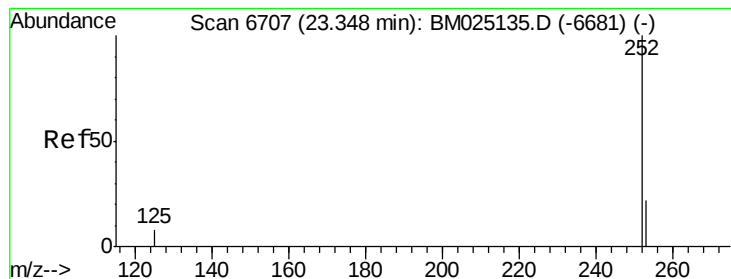

#23

Benzo(a)pyrene

Concen: 0.095 ng/ul

RT: 23.30 min Scan# 6687

Delta R.T. -0.05 min

Lab File: BM025136.D


Acq: 28 Feb 2020 16:56

Instrument :

BNA_M

ClientSampleId :

SBLK36

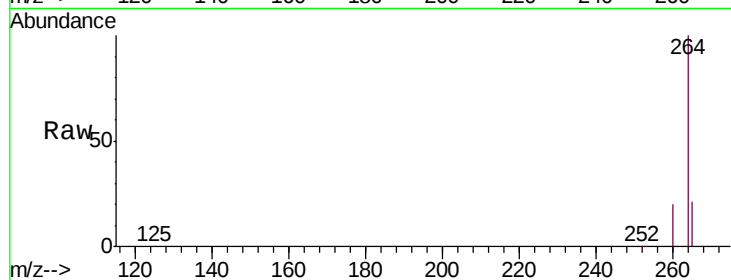


Tgt Ion: 252 Resp: 4873

Ion Ratio Lower Upper

252 100

253 35.7 20.3 30.5#

125 26.5 13.0 19.4#

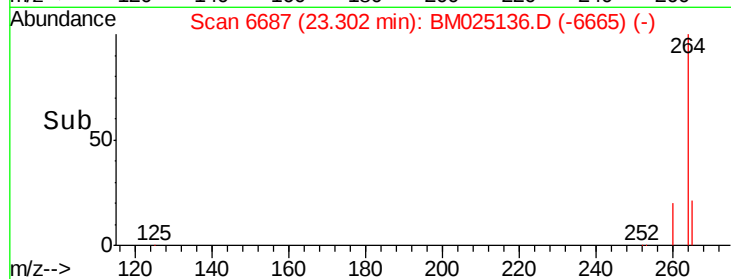

Abundance Ion 252.00 (251.70 to 252.70): E

4000 Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

