

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Not Reviewed)

Data File : BM025142.D
Acq On : 28 Feb 2020 20:33
Operator : CG/JU
Sample : L1507-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD06

Quant Time: Feb 29 04:46:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2649	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	9965	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	6508	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.06
16) Chrysene-d12	21.24	240	16243	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	19071	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	5624	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	15200	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.45	202	2689	0.037	ng/ul#	1
23) Benzo(a)pyrene	23.30	252	5423	0.079	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025142.D
Acq On : 28 Feb 2020 20:33
Operator : CG/JU
Sample : L1507-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD06

Quant Time: Feb 29 04:46:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

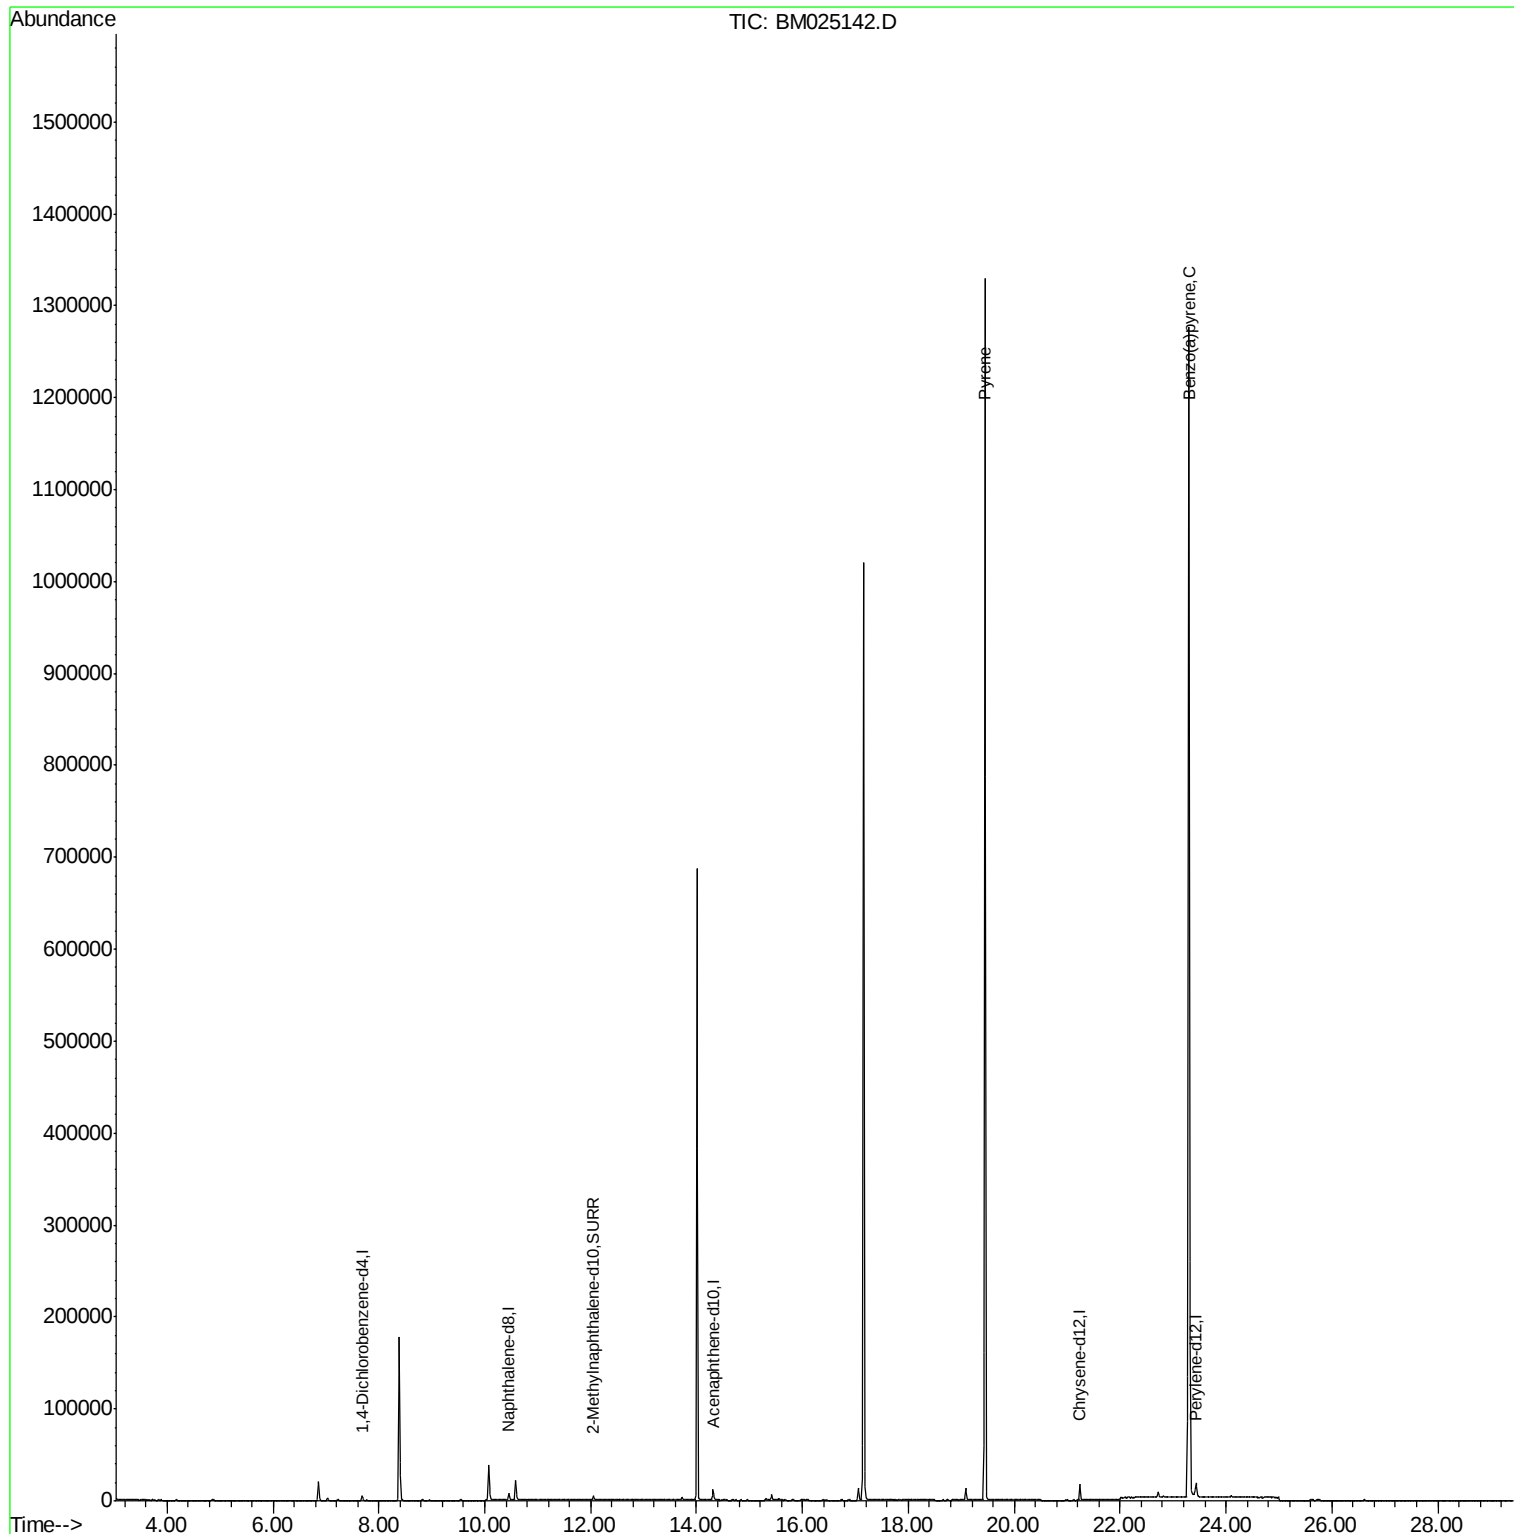

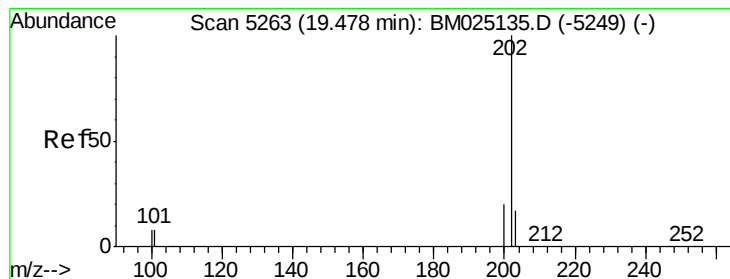

#17

Pyrene

Concen: 0.037 ng/ul

RT: 19.45 min Scan# 5255

Delta R.T. -0.03 min

Lab File: BM025142.D

Acq: 28 Feb 2020 20:33

Instrument :

BNA_M

ClientSampleId :

DBD06


Tgt Ion:202 Resp: 2689

Ion Ratio Lower Upper

202 100

101 139.4 8.7 13.1#




100 960.5 7.3 10.9#

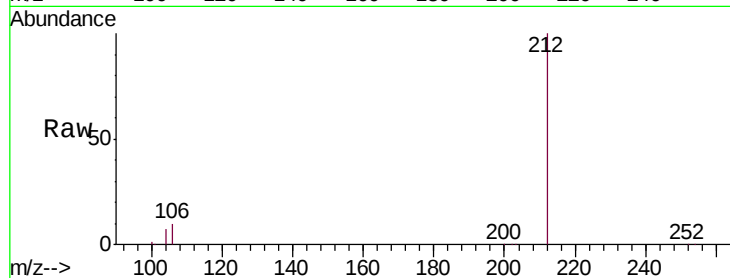

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

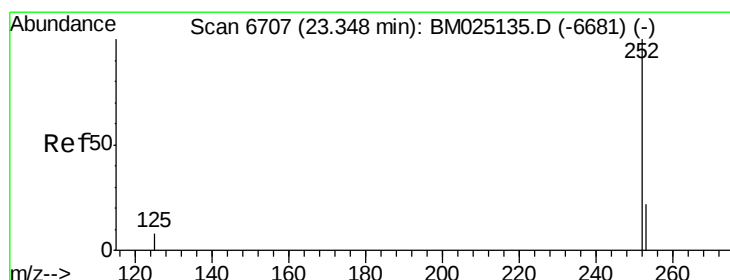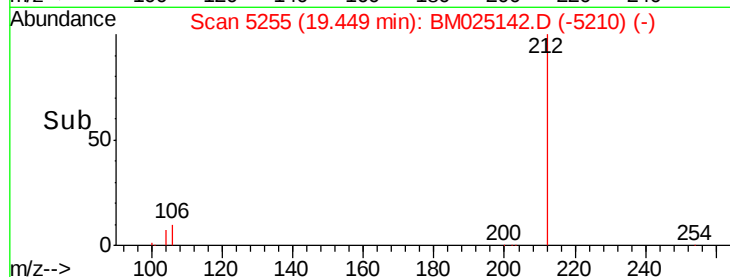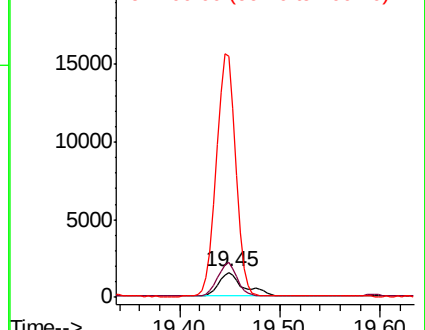

#23

Benzo(a)pyrene

Concen: 0.079 ng/ul

RT: 23.30 min Scan# 6686

Delta R.T. -0.05 min

Lab File: BM025142.D

Acq: 28 Feb 2020 20:33


Tgt Ion:252 Resp: 5423

Ion Ratio Lower Upper

252 100

253 38.6 20.3 30.5#

125 37.2 13.0 19.4#

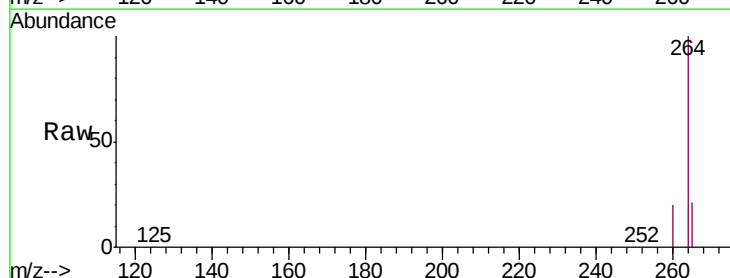

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

