

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Not Reviewed)

Data File : BM025148.D
Acq On : 29 Feb 2020 00:09
Operator : CG/JU
Sample : L1507-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD13

Quant Time: Feb 29 04:47:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2689	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	10378	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	6768	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.06
16) Chrysene-d12	21.24	240	15861	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	17856	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	6865	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	18951	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.47	202	1913	0.027	ng/ul#	79
23) Benzo(a)pyrene	23.30	252	6330	0.099	ng/ul#	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025148.D
Acq On : 29 Feb 2020 00:09
Operator : CG/JU
Sample : L1507-15
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD13

Quant Time: Feb 29 04:47:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration




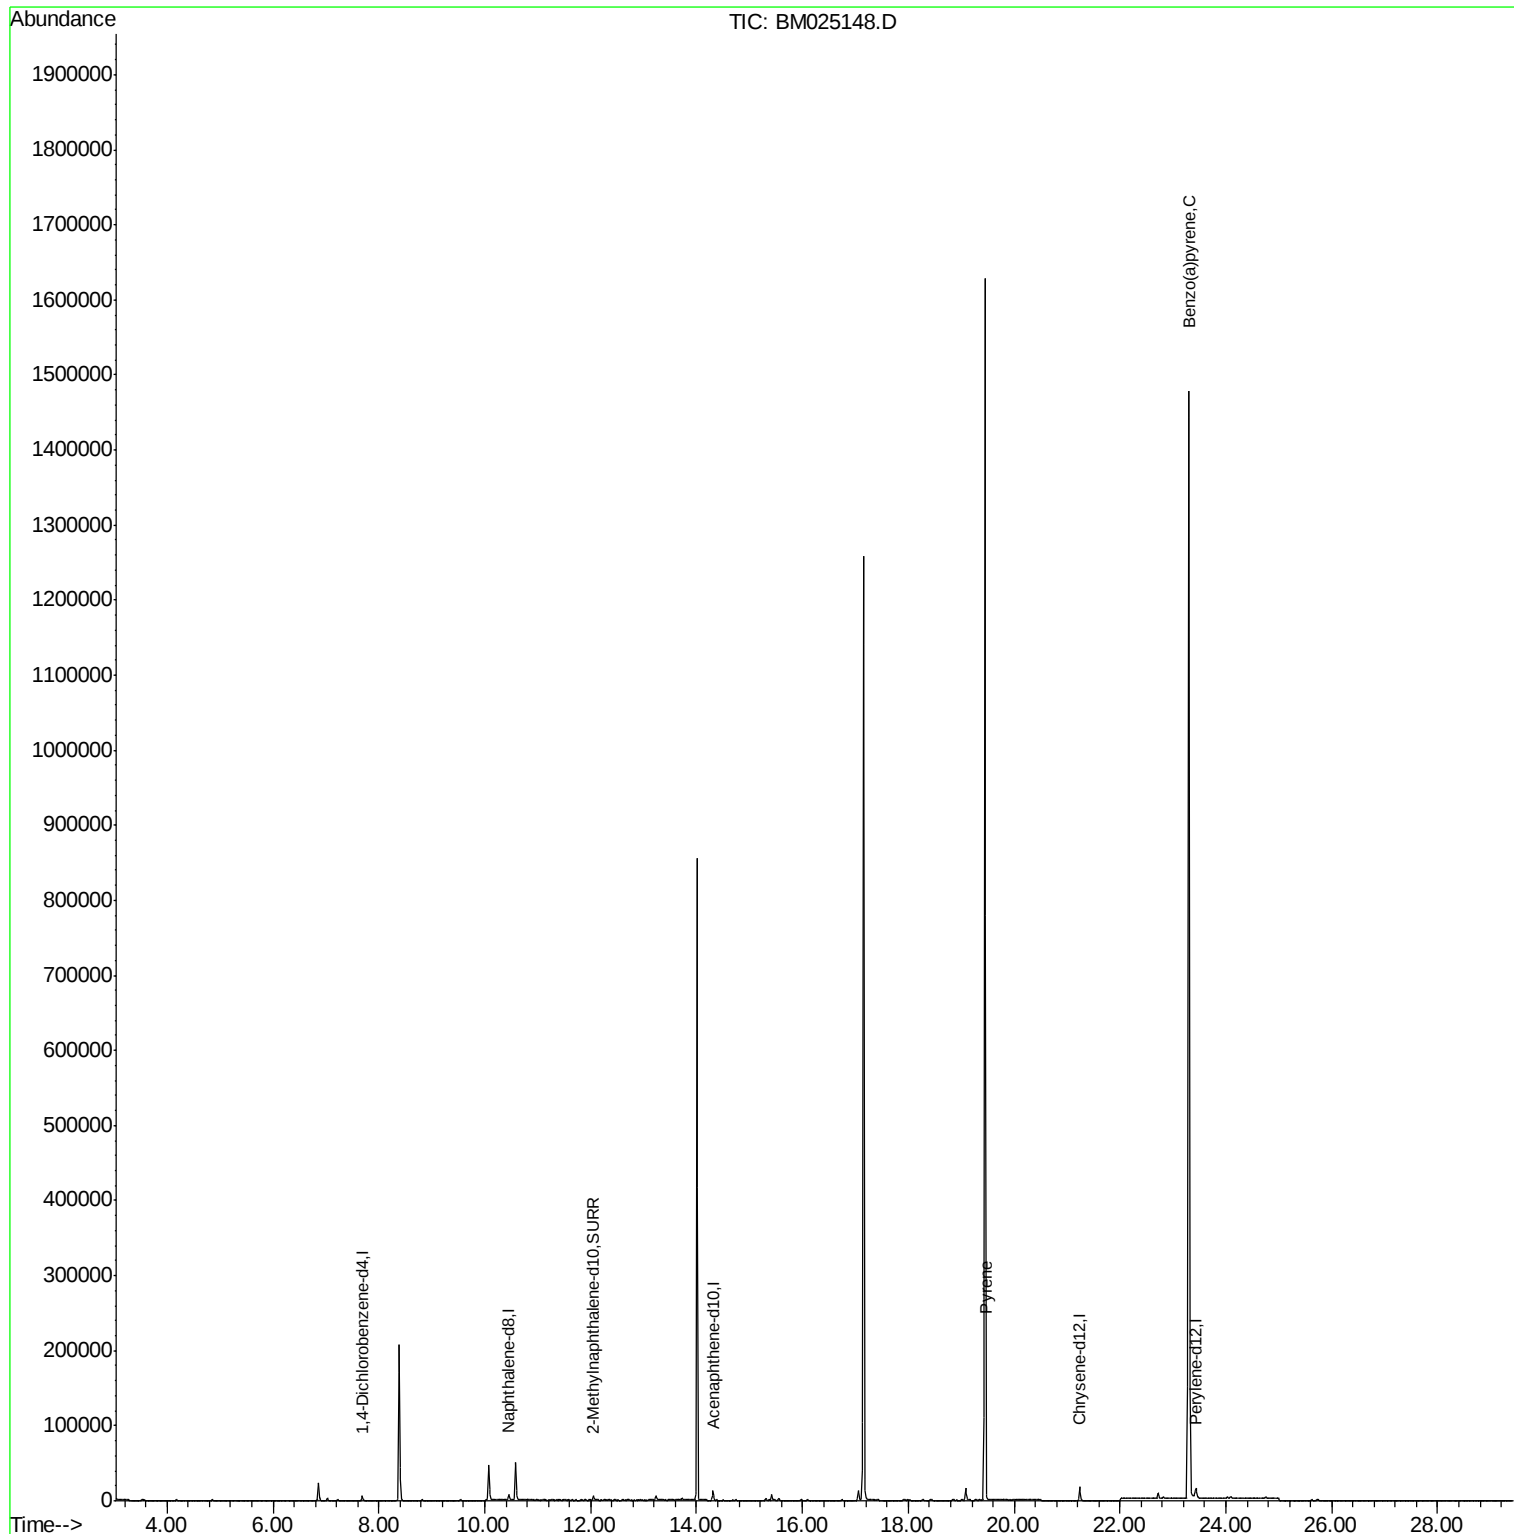


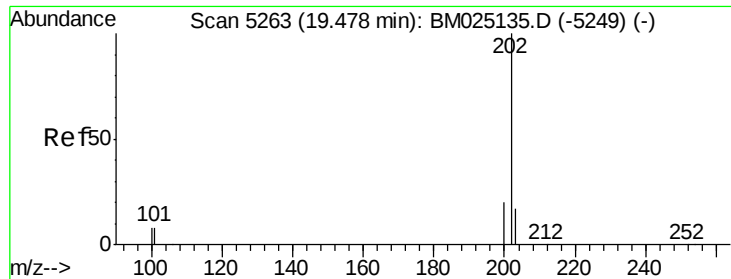

#17
 Pyrene
 Concen: 0.027 ng/ul
 RT: 19.47 min Scan# 5261
 Delta R.T. -0.01 min
 Lab File: BM025148.D
 Acq: 29 Feb 2020 00:09

Instrument :
 BNA_M
 ClientSampleId :
 DBD13

Tgt Ion:202 Resp: 1913
 Ion Ratio Lower Upper
 202 100
 101 16.8 8.7 13.1#
 100 19.3 7.3 10.9#

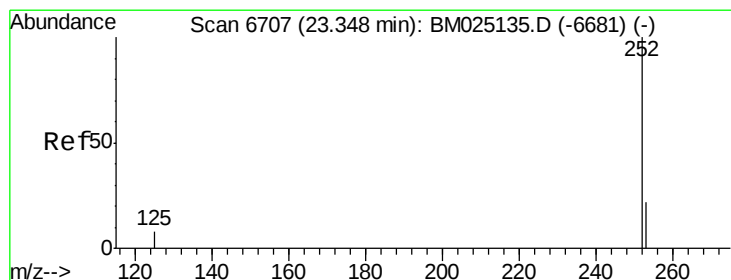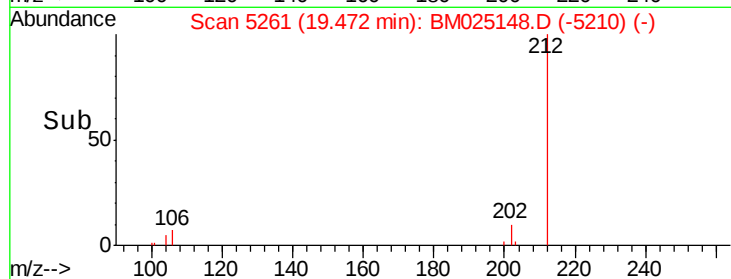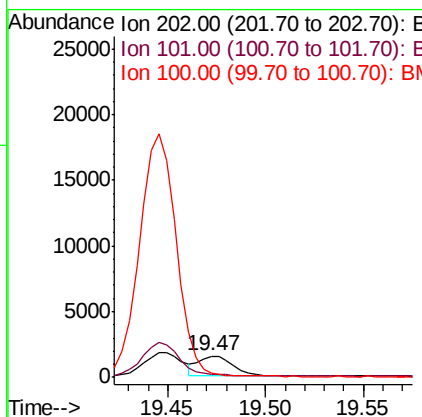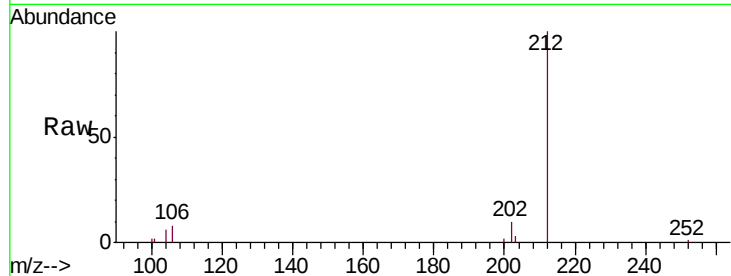

#23
 Benzo(a)pyrene
 Concen: 0.099 ng/ul
 RT: 23.30 min Scan# 6686
 Delta R.T. -0.05 min
 Lab File: BM025148.D
 Acq: 29 Feb 2020 00:09

Tgt Ion:252 Resp: 6330
 Ion Ratio Lower Upper
 252 100
 253 35.7 20.3 30.5#
 125 25.7 13.0 19.4#

