

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Not Reviewed)

Data File : BM025158.D
Acq On : 29 Feb 2020 09:07
Operator : CG/JU
Sample : PB126929BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK29

Quant Time: Mar 02 01:17:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 01:15:39 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	3353	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	12656	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	8074	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.24	240	18826	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	21475	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	7778	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	20491	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.47	202	12710	0.150	ng/ul#	95
23) Benzo(a)pyrene	23.30	252	7195	0.094	ng/ul#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025158.D
Acq On : 29 Feb 2020 09:07
Operator : CG/JU
Sample : PB126929BL
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK29

Quant Time: Mar 02 01:17:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 01:15:39 2020
Response via : Initial Calibration

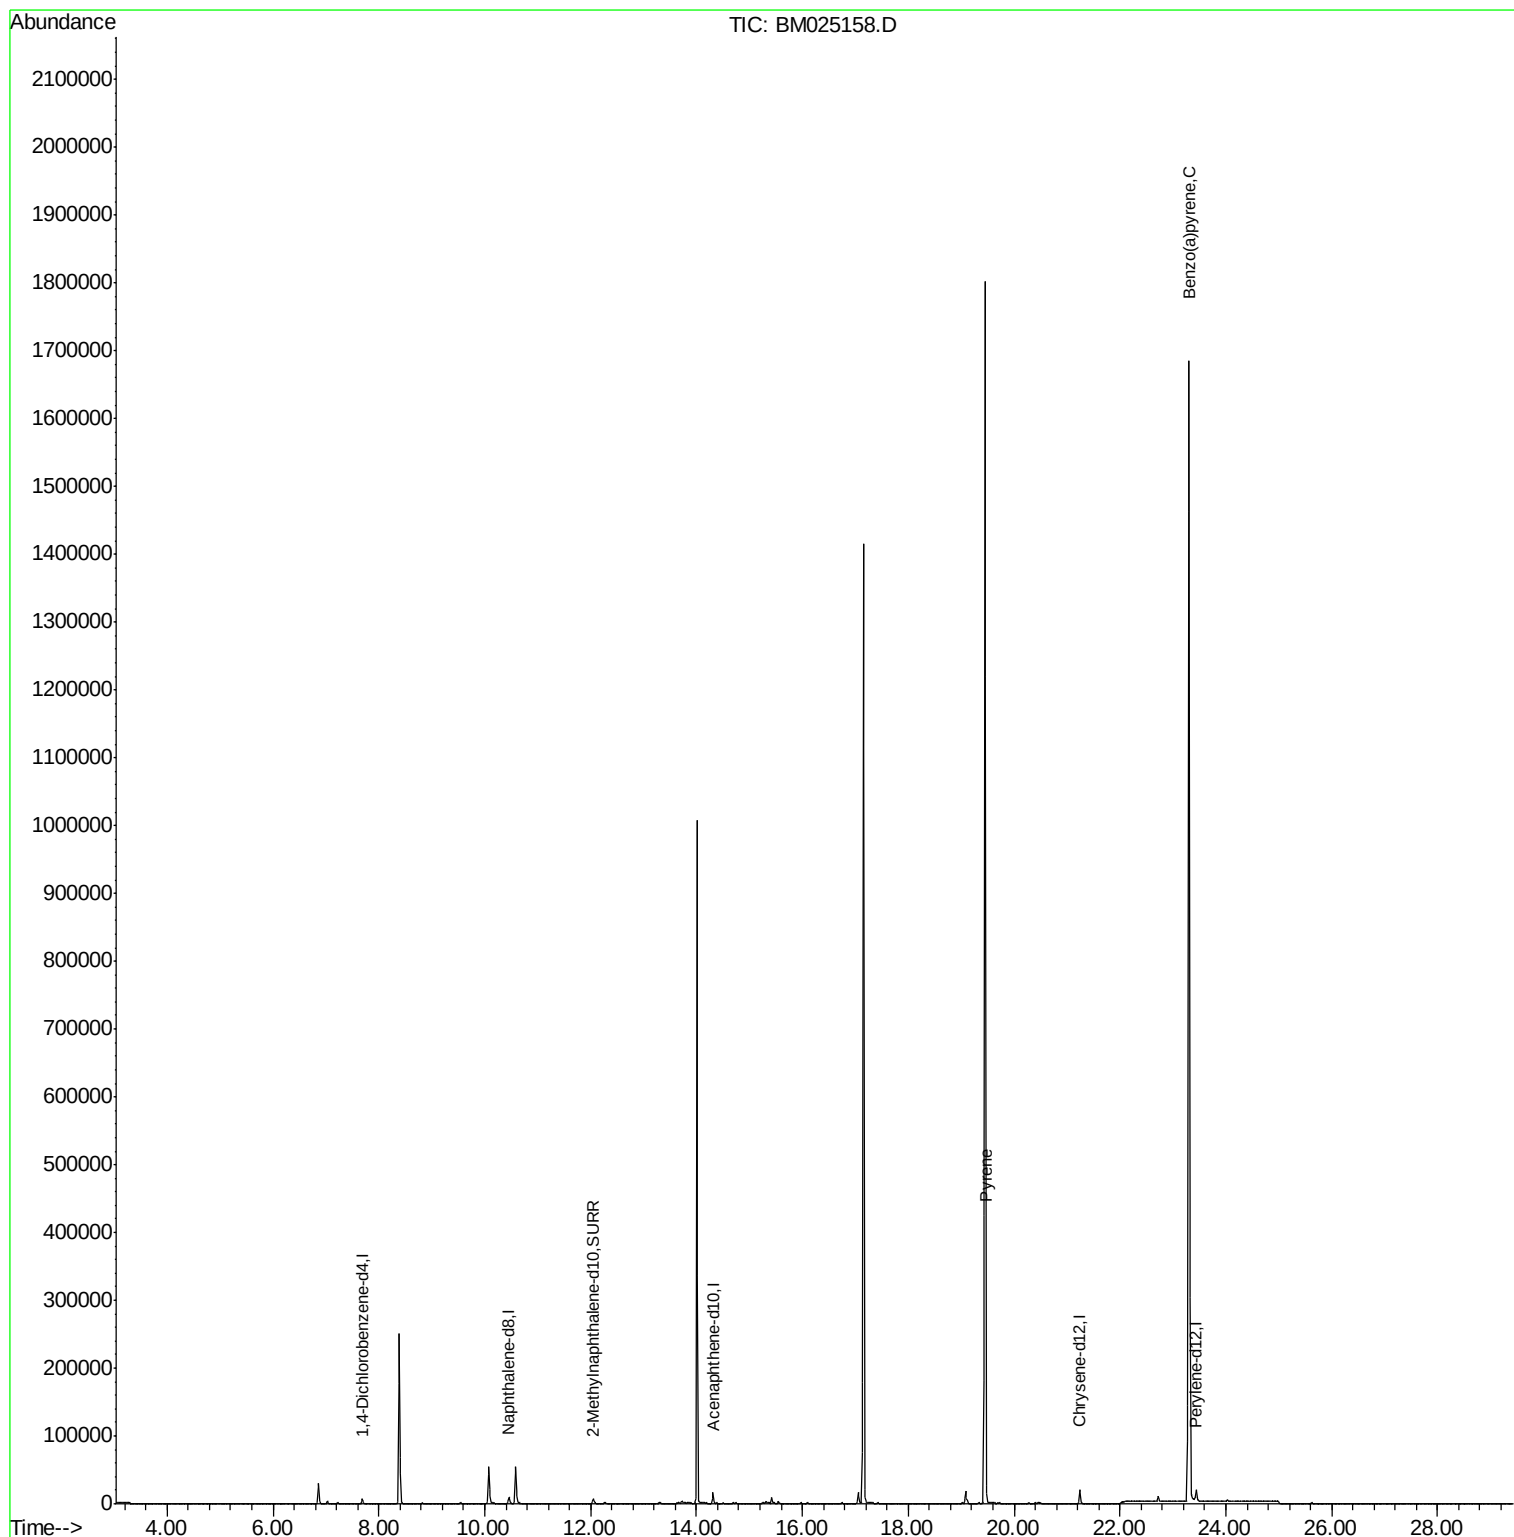

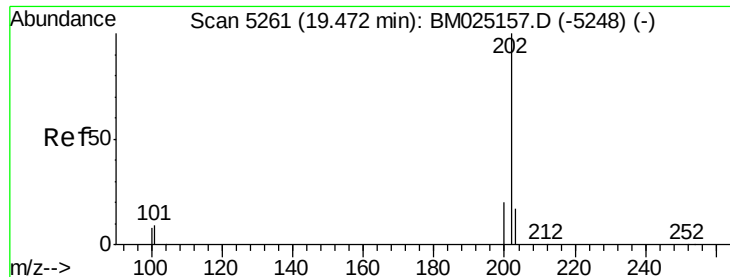

#17

Pyrene

Concen: 0.150 ng/ul

RT: 19.47 min Scan# 5261

Delta R.T. 0.00 min

Lab File: BM025158.D

Acq: 29 Feb 2020 09:07

Instrument :

BNA_M

ClientSampleId :

SBLK29


Tgt Ion:202 Resp: 12710

Ion Ratio Lower Upper

202 100

101 10.9 8.7 13.1




100 13.3 7.3 10.9#

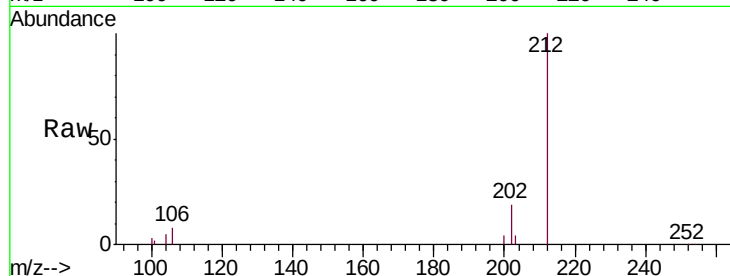

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

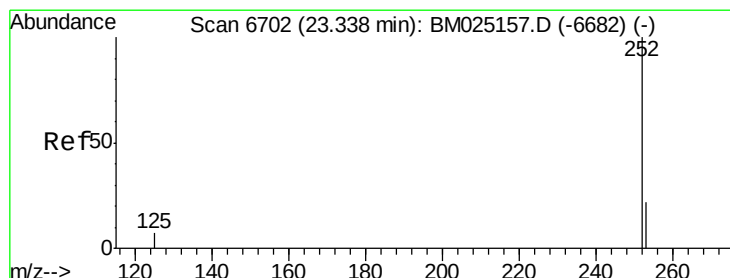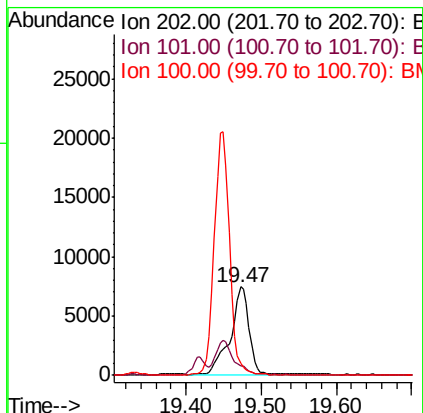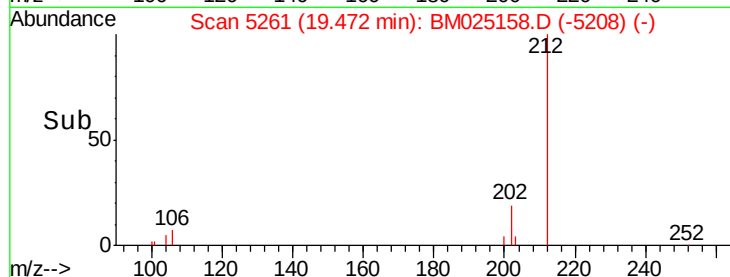

#23

Benzo(a)pyrene

Concen: 0.094 ng/ul

RT: 23.30 min Scan# 6688

Delta R.T. -0.03 min

Lab File: BM025158.D

Acq: 29 Feb 2020 09:07


Tgt Ion:252 Resp: 7195

Ion Ratio Lower Upper

252 100

253 34.4 20.3 30.5#

125 24.2 13.0 19.4#

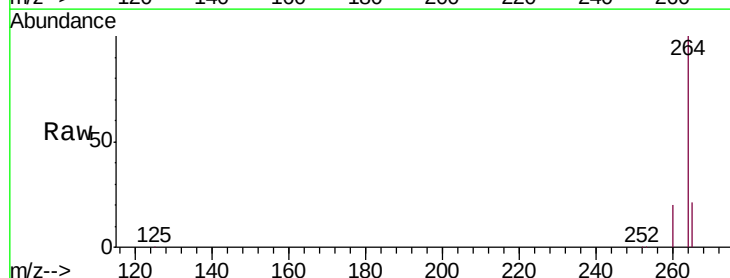

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

