

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Not Reviewed)

Data File : BM025178.D
Acq On : 29 Feb 2020 21:04
Operator : CG/JU
Sample : L1542-19
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD53

Quant Time: Mar 02 02:11:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	3068	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	11823	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	7300	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	16865	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	16204	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	18106	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.06	152	9	0.00	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	38	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.47	202	2853	0.039	ng/ul	Qvalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BM025178.D
Acq On : 29 Feb 2020 21:04
Operator : CG/JU
Sample : L1542-19
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD53

Quant Time: Mar 02 02:11:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

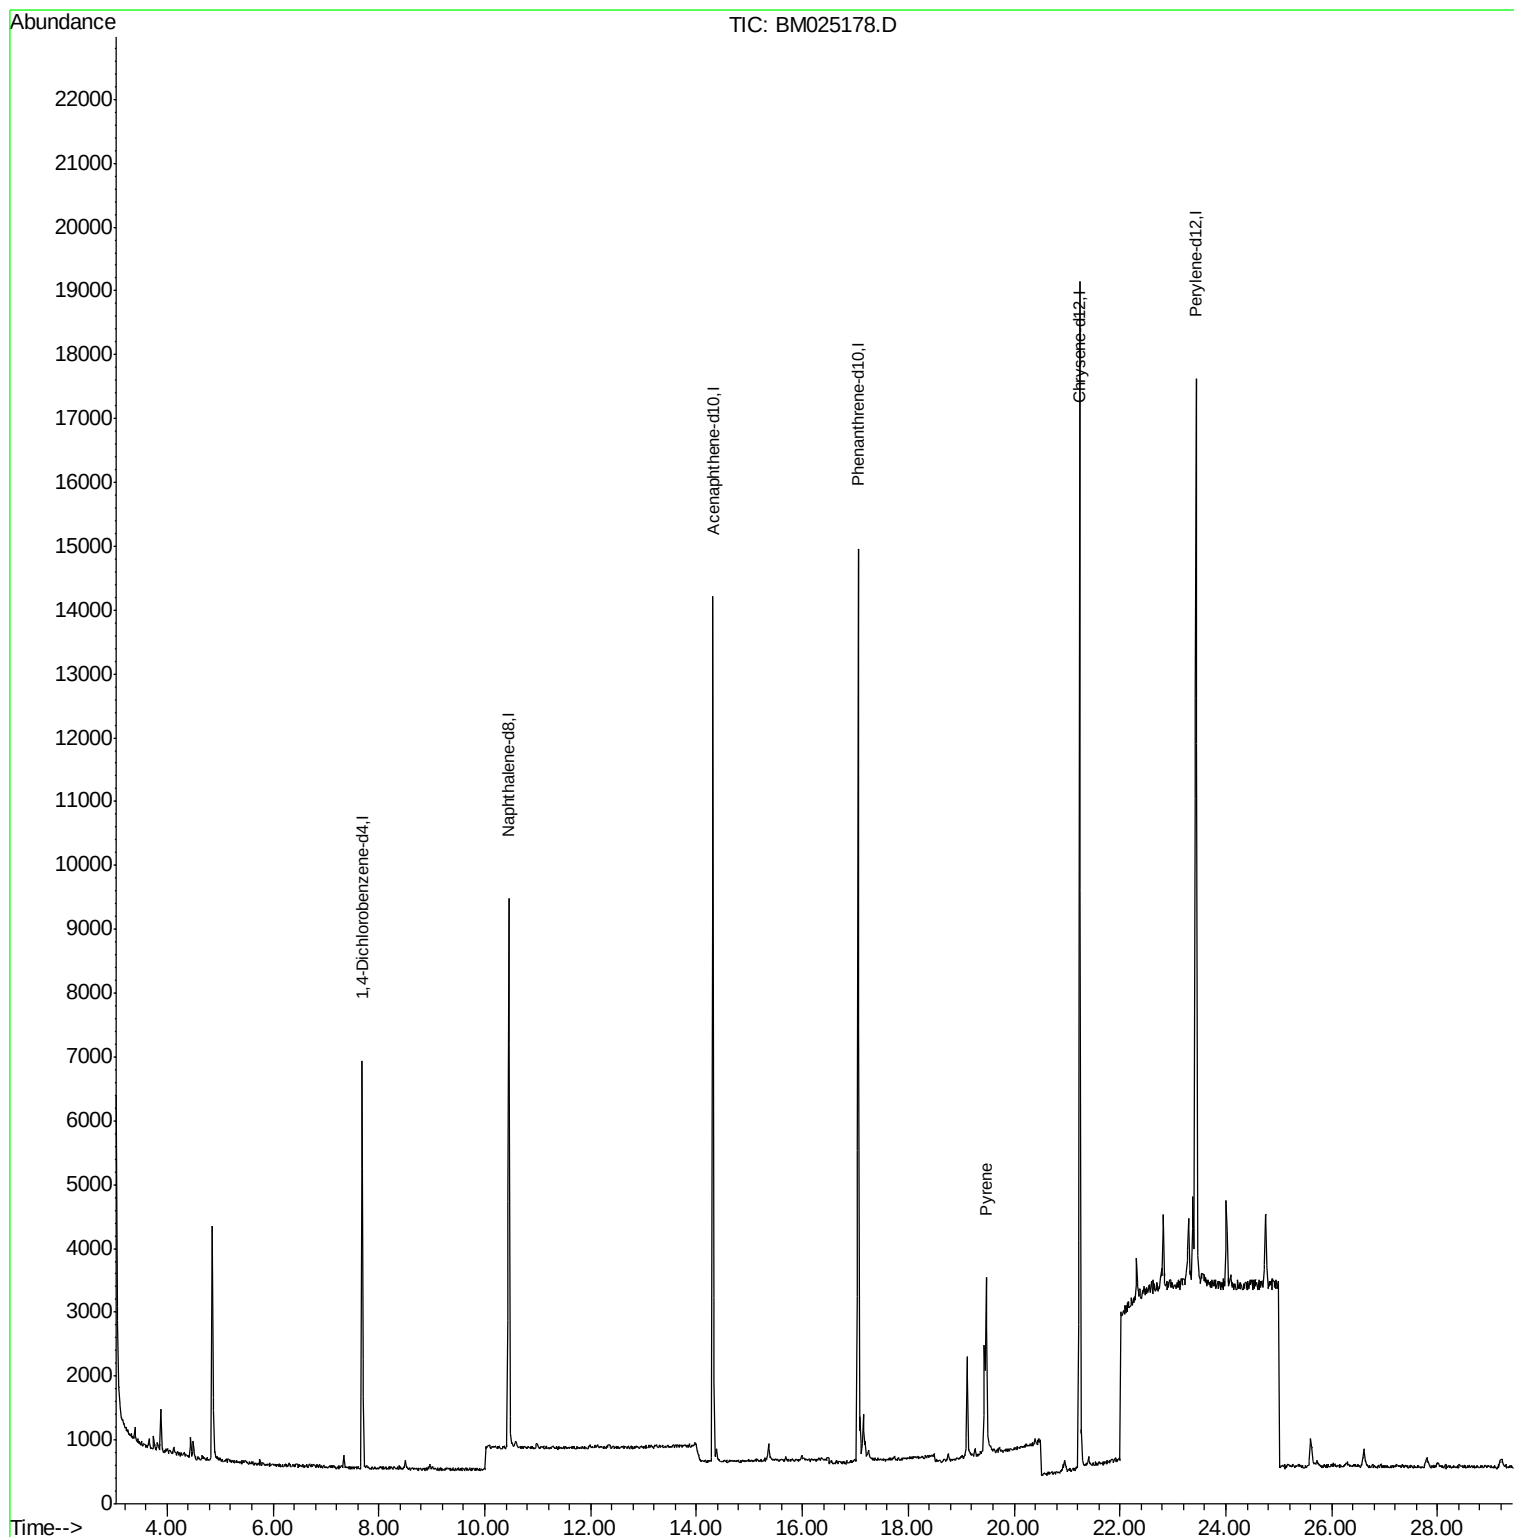

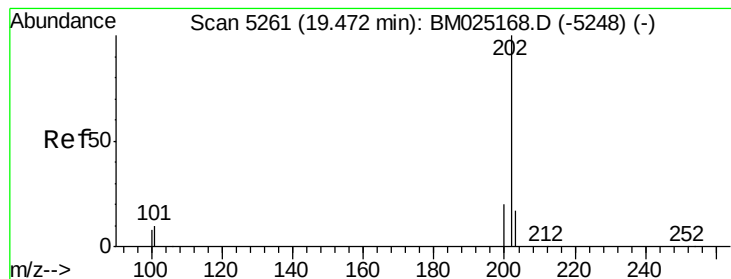

#17

Pyrene

Concen: 0.039 ng/ul

RT: 19.47 min Scan# 5261

Delta R.T. 0.00 min

Lab File: BM025178.D

Acq: 29 Feb 2020 21:04

Instrument :

BNA_M

ClientSampleId :

DBD53


Tgt Ion:202 Resp: 2853

Ion Ratio Lower Upper

202 100

101 12.6 8.7 13.1

100 10.6 7.3 10.9

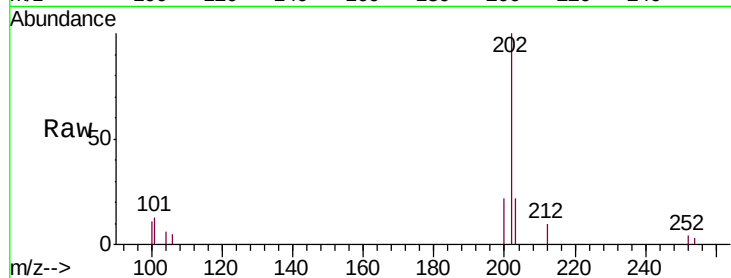

Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

