

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022820\
Data File : BM025136.D
Acq On : 28 Feb 2020 16:56
Operator : CG/JU
Sample : PB126836BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Mar 02 09:59:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

Instrument :

BNA_M


ClientSampleId :

SBLK36

Manual Integrations
APPROVED

Sohil

3/3/2020 8:38:34 AM

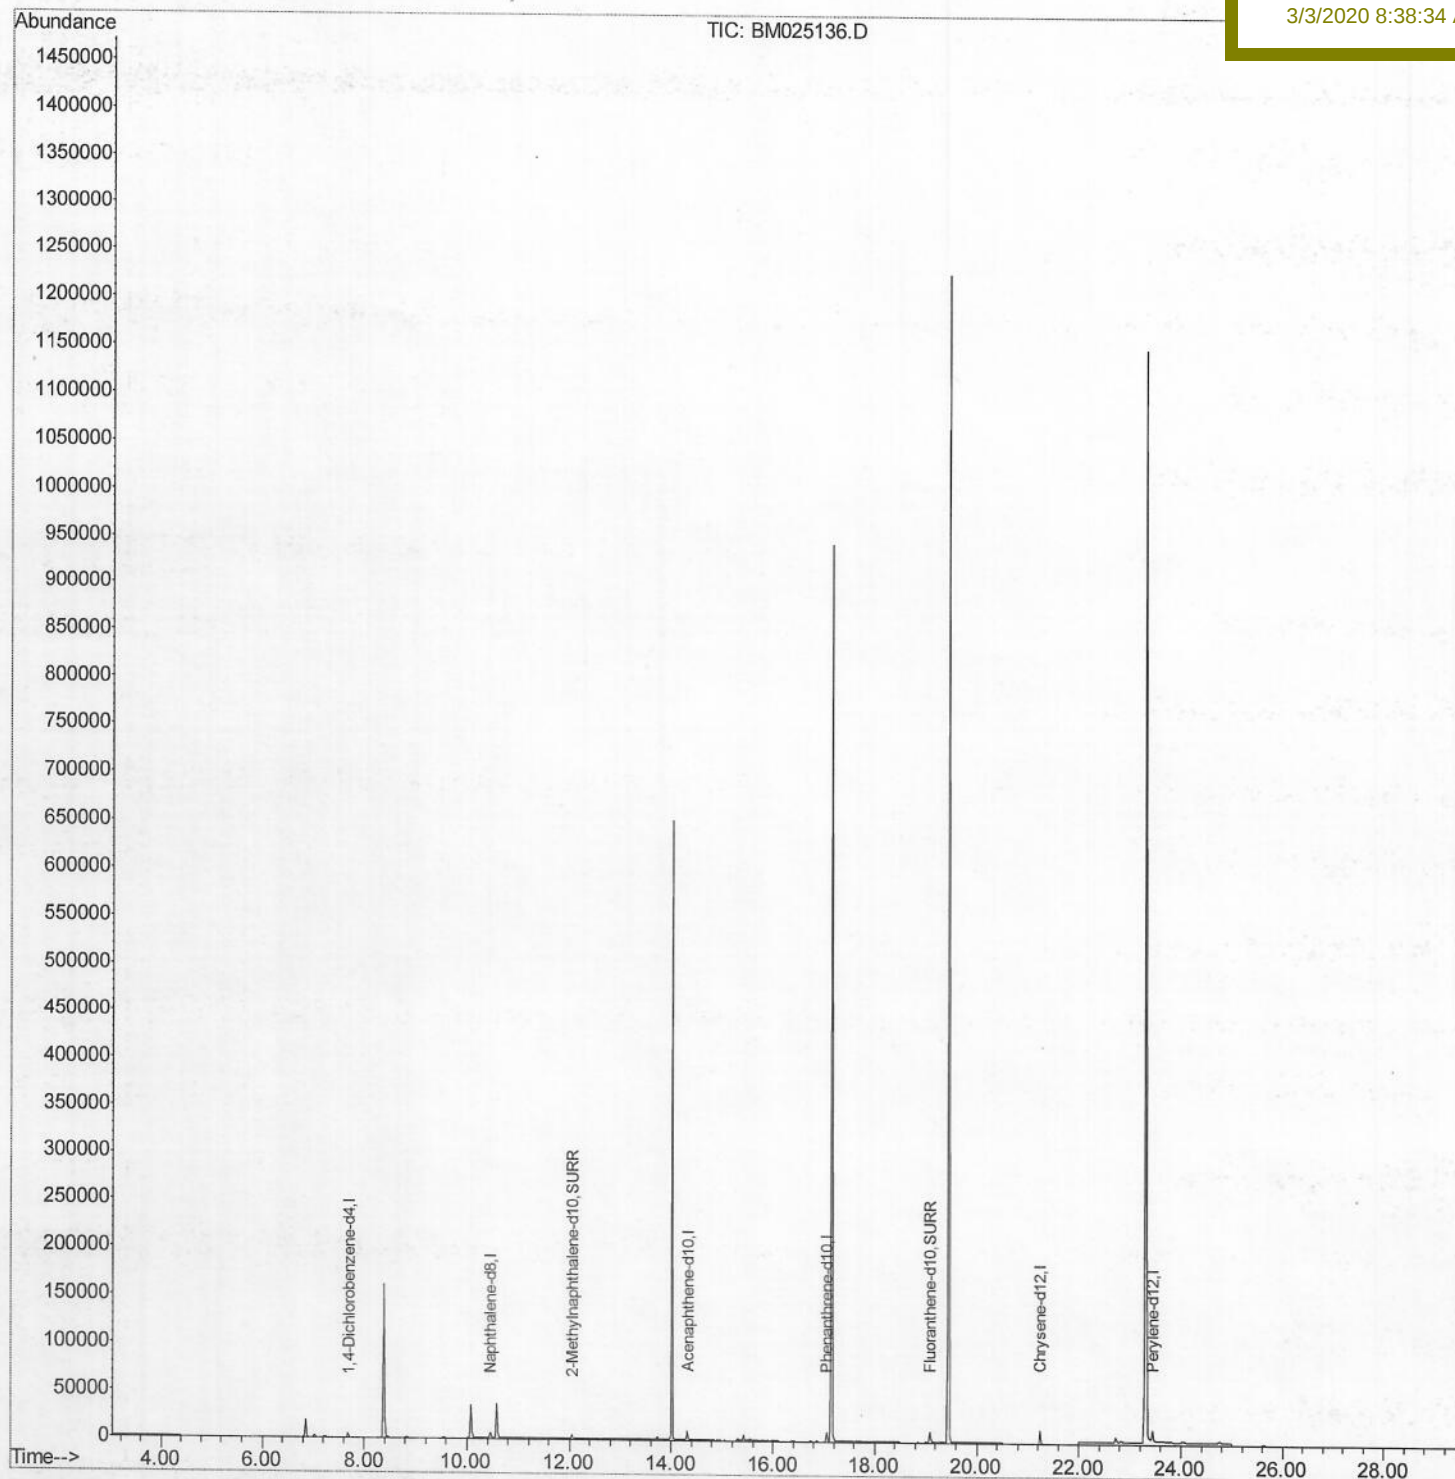

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Qedit)




Data File : BM025136.D
Acq On : 28 Feb 2020 16:56
Operator : CG/JU
Sample : PB126836BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 29 04:45:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK36

Manual Integrations
APPROVED

Sohil
3/3/2020 8:38:34 AM

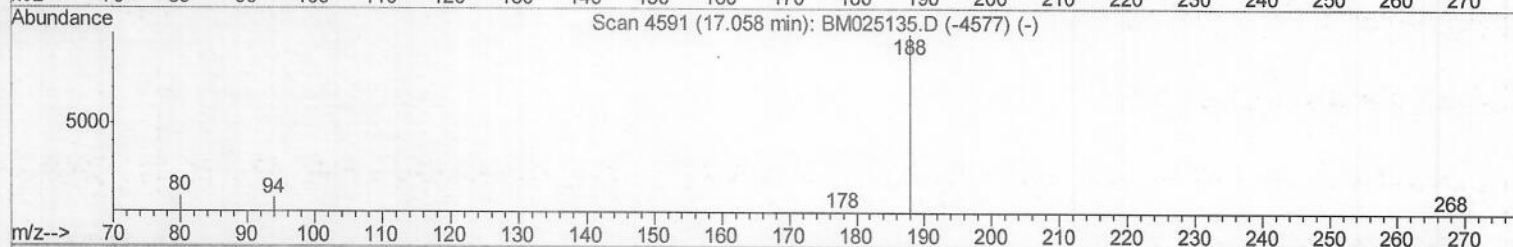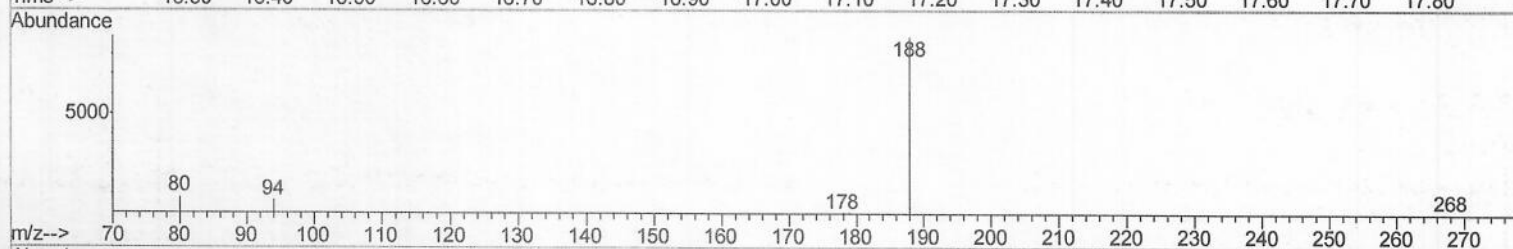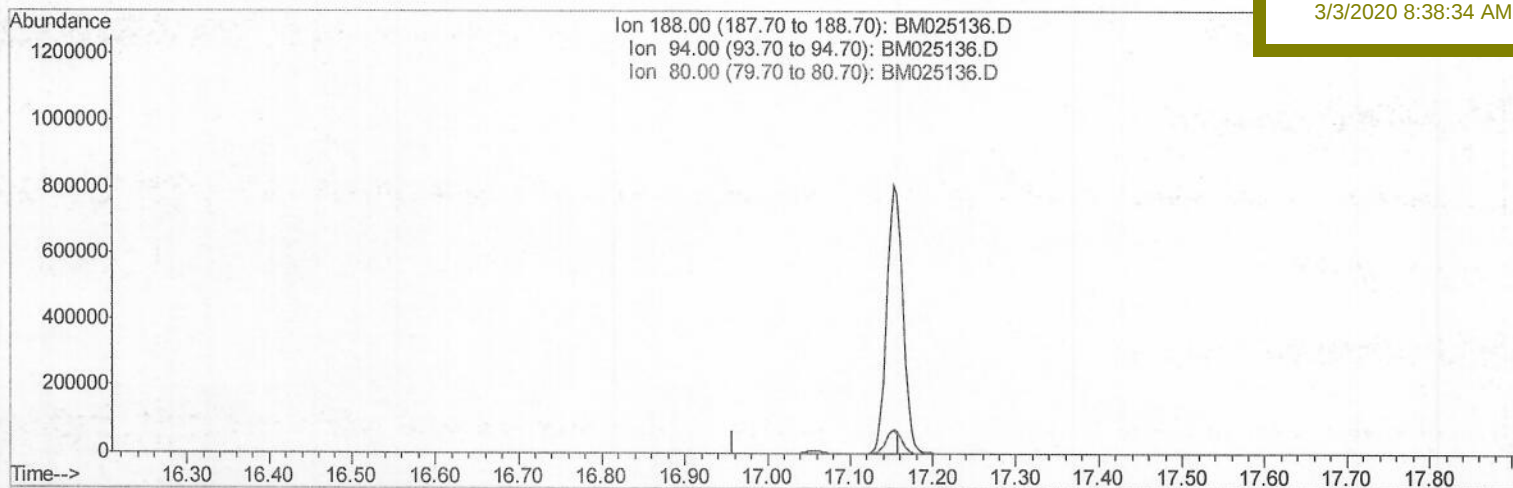

TIC: BM025136.D

(10) Phenanthrene-d10 (I)

17.058min (-17.058) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022820\

Data File : BM025136.D

Acq On : 28 Feb 2020 16:56

Operator : CG/JU

Sample : PB126836BL

Misc :

ALS Vial : 10 Sample Multiplier: 1

Quant Time: Mar 02 09:59:18 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Mar 02 02:08:15 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




SBLK36

Manual Integrations

APPROVED

Sohil

3/3/2020 8:38:34 AM

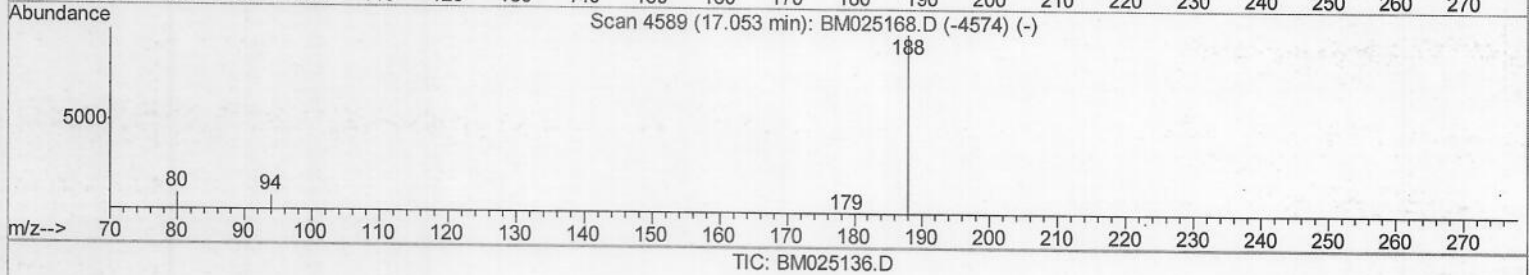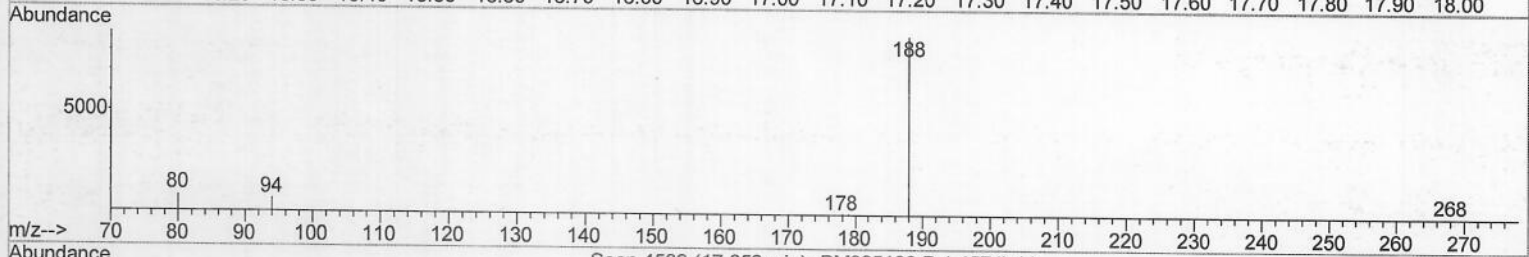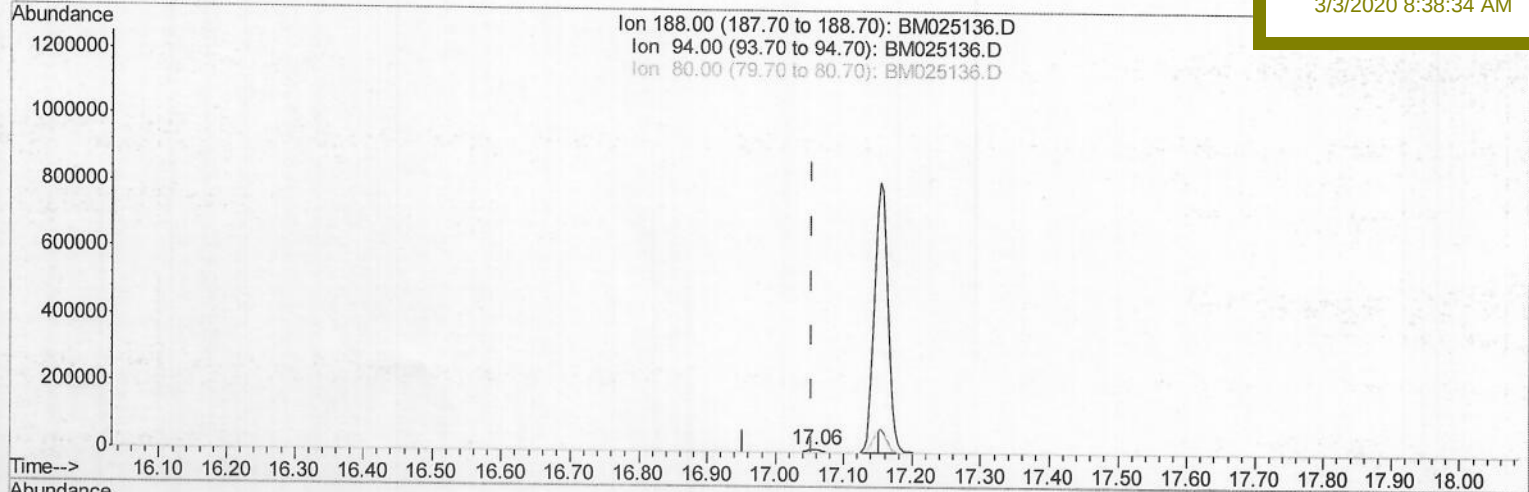

(10) Phenanthrene-d10 (I)

17.057min (+0.003) 0.40ng/ul m > JV 03/04/20

response 12164

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.02#
80.00	22.60	9.64#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022820\
Data File : BM025136.D
Acq On : 28 Feb 2020 16:56
Operator : CG/JU
Sample : PB126836BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Mar 02 09:59:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sample ID :
SBLK36

Manual Integrations
APPROVED

Sohil
3/3/2020 8:38:34 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev (Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2194	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	8316	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	5456	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	12164m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	12107	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	14339	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	5137	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.09	212	13171	0.32	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed