

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (QT Reviewed)


Data File : BM025137.D
Acq On : 28 Feb 2020 17:32
Operator : CG/JU
Sample : L1507-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DBD01

Manual Integrations
APPROVED

Sohil
3/3/2020 8:38:35 AM

Quant Time: Feb 29 05:01:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

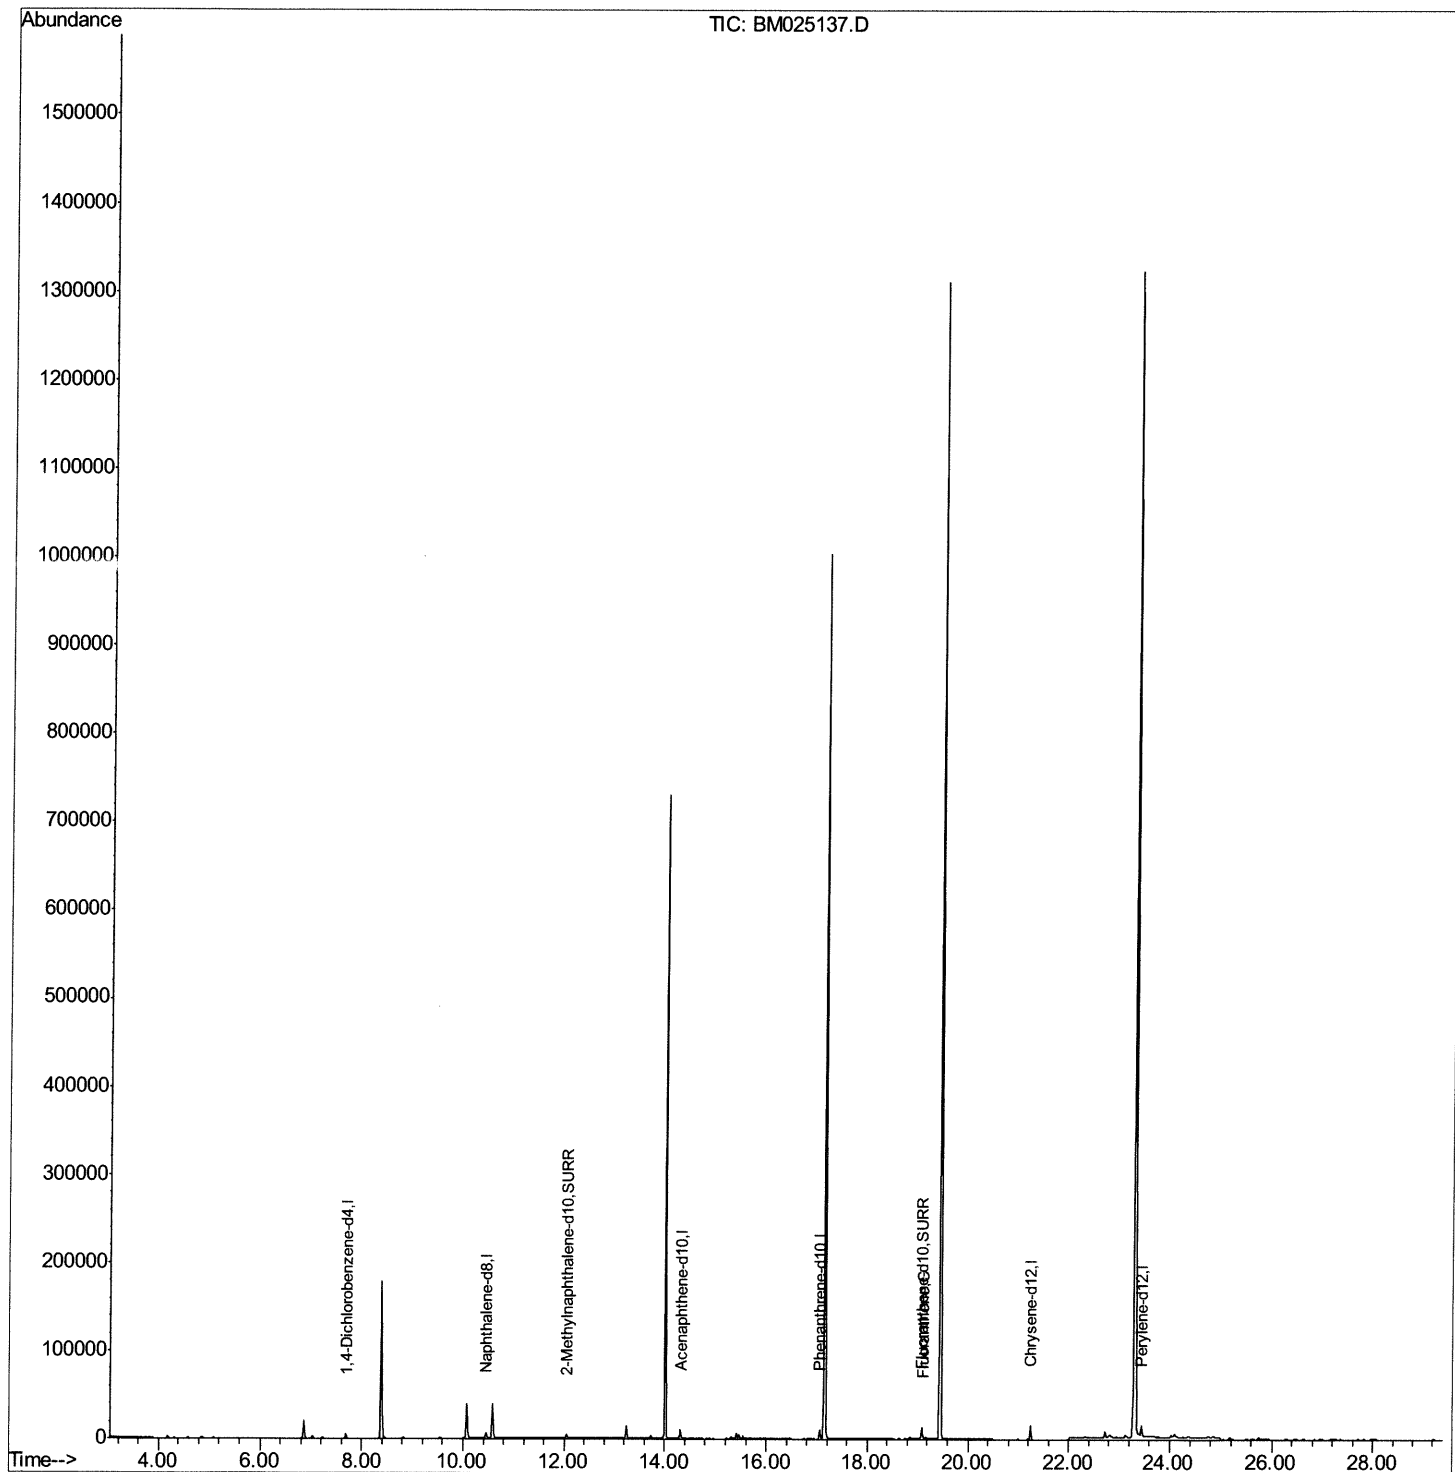

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Qedit)




Data File : BM025137.D
Acq On : 28 Feb 2020 17:32
Operator : CG/JU
Sample : L1507-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
DBD01

Manual Integrations
APPROVED

Sohil
3/3/2020 8:38:35 AM

Quant Time: Feb 29 04:46:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

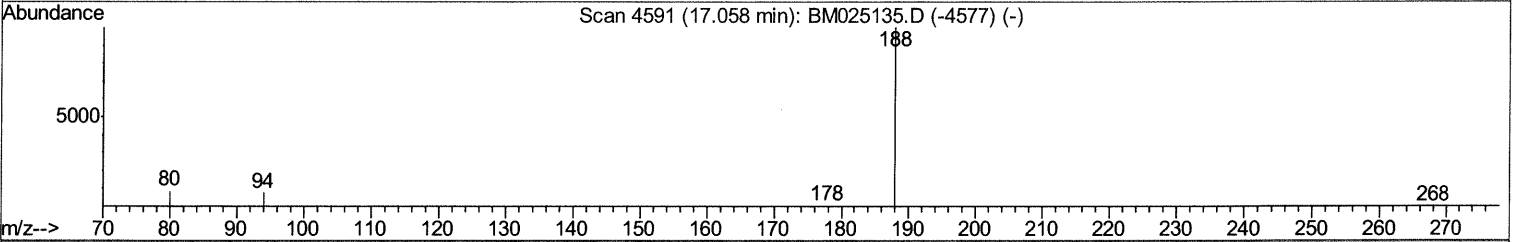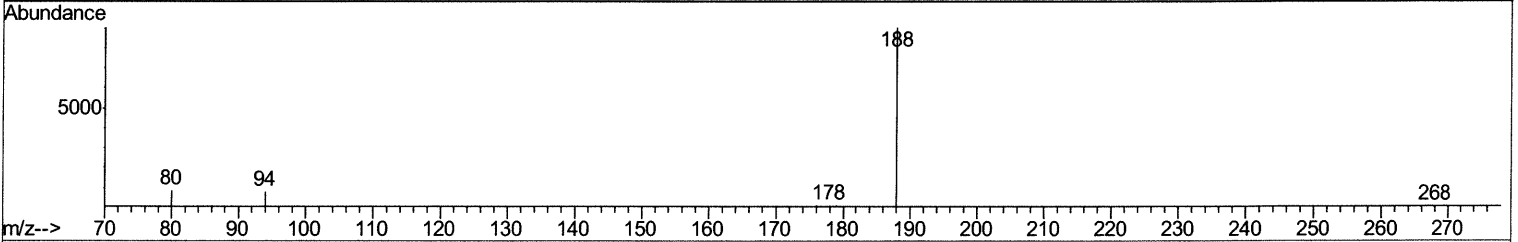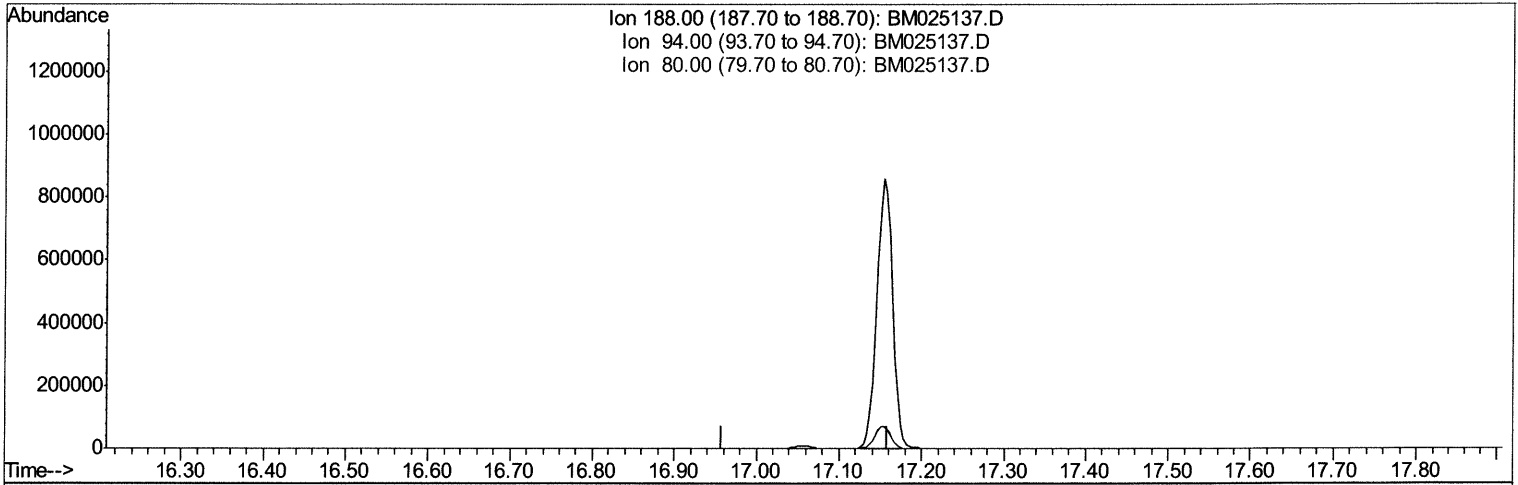

TIC: BM025137.D

(10) Phenanthrene-d10 (I)
17.058min (-17.058) 0.00ng/ul
response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Qedit)




Data File : BM025137.D
Acq On : 28 Feb 2020 17:32
Operator : CG/JU
Sample : L1507-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD01

Manual Integrations
APPROVED

Sohil
3/3/2020 8:38:35 AM

Quant Time: Feb 29 04:46:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

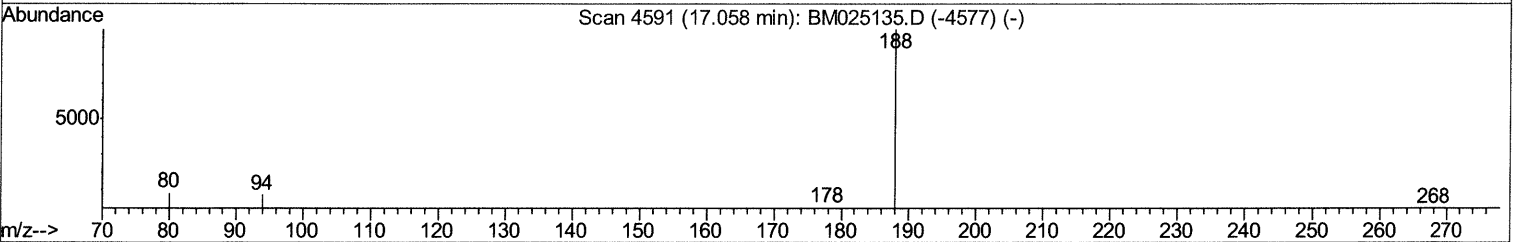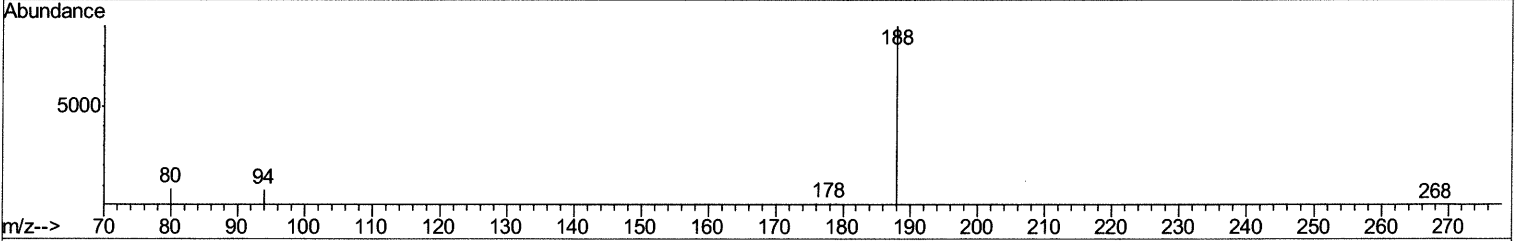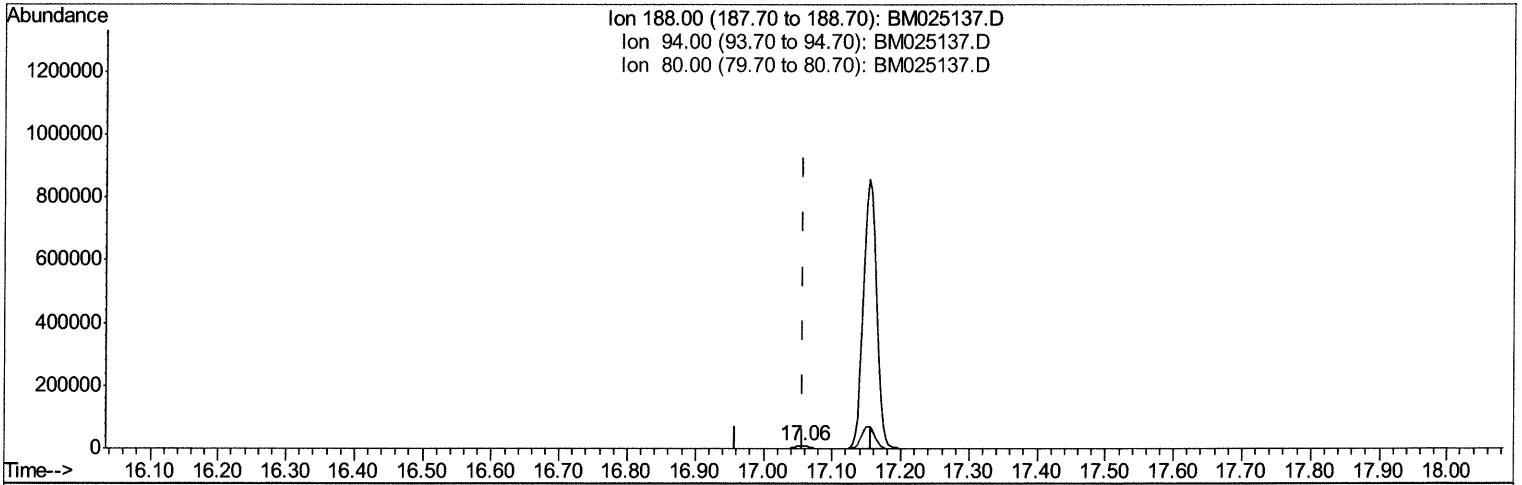

TIC: BM025137.D

(10) Phenanthrene-d10 (I)

17.057min (-0.002) 0.40ng/ul m *JU 03/02/20*

response 12340

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.75#
80.00	22.60	9.45#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (QT Reviewed)

Data File : BM025137.D
Acq On : 28 Feb 2020 17:32
Operator : CG/JU
Sample : L1507-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD01

Manual Integrations
APPROVED

Sohil
3/3/2020 8:38:35 AM

Quant Time: Feb 29 05:01:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2277	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	8623	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.32	164	5601	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.06	188	12340m >	0.40	ng/ul >	0.00
16) Chrysene-d12	21.24	240	13709	0.40	ng/ul	0.00
20) Perylene-d12	23.44	264	16410	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	5715	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	15042	0.36	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.11	202	1302	0.021	ng/ul	Qvalue 86

su 03/02/20

(#) = qualifier out of range (m) = manual integration (+) = signals summed