

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (QT Reviewed)


Data File : BM025180.D
Acq On : 29 Feb 2020 22:16
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:52 AM

Quant Time: Mar 02 03:10:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

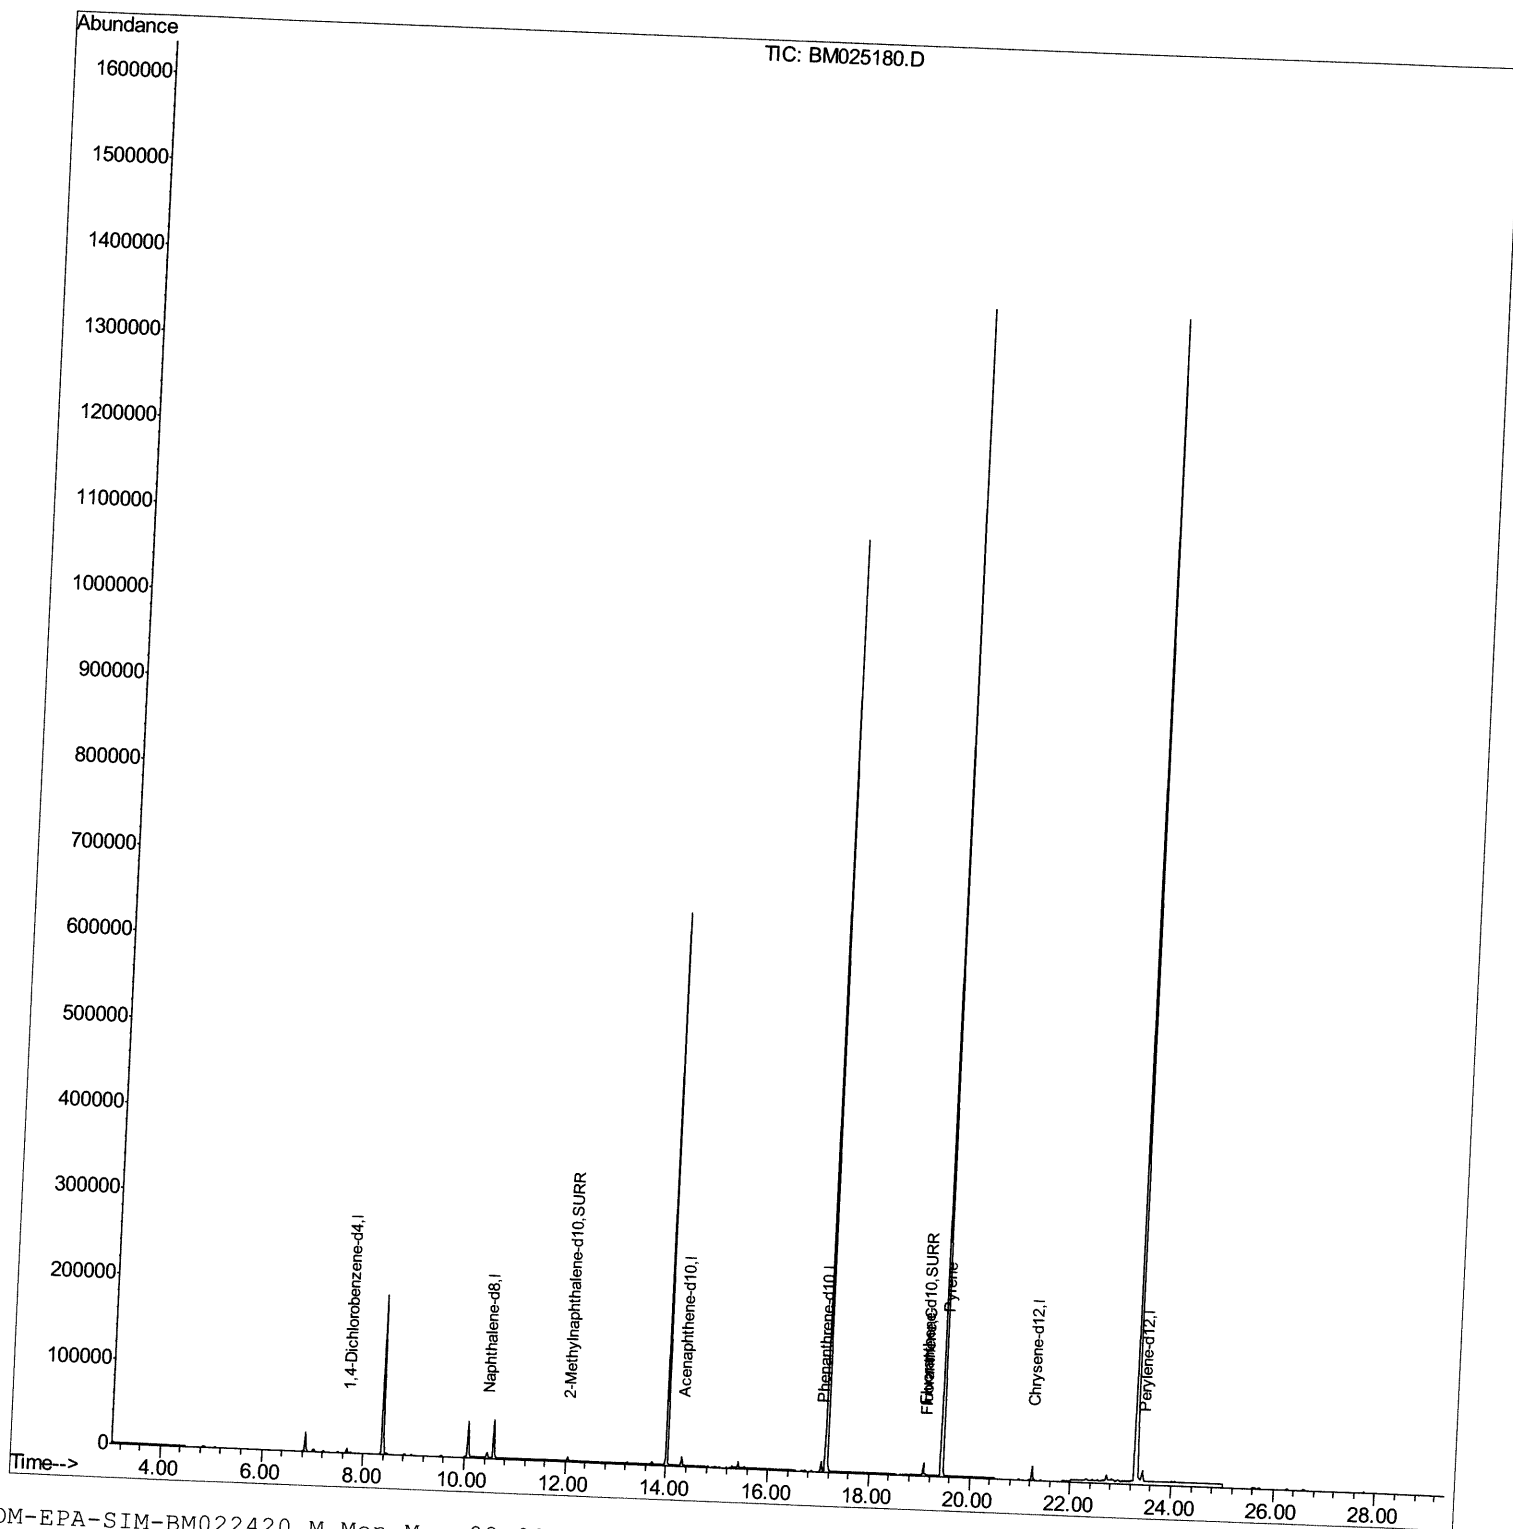

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Qedit)




Data File : BM025180.D
Acq On : 29 Feb 2020 22:16
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:52 AM

Quant Time: Mar 02 02:11:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

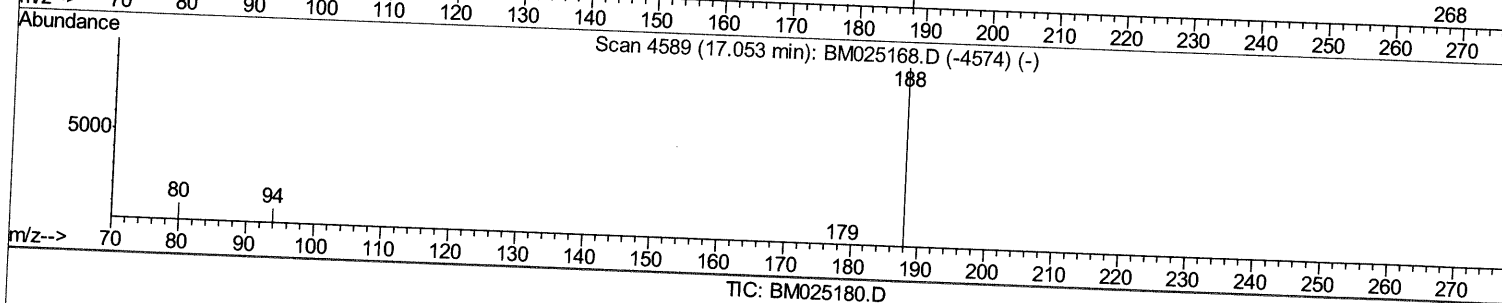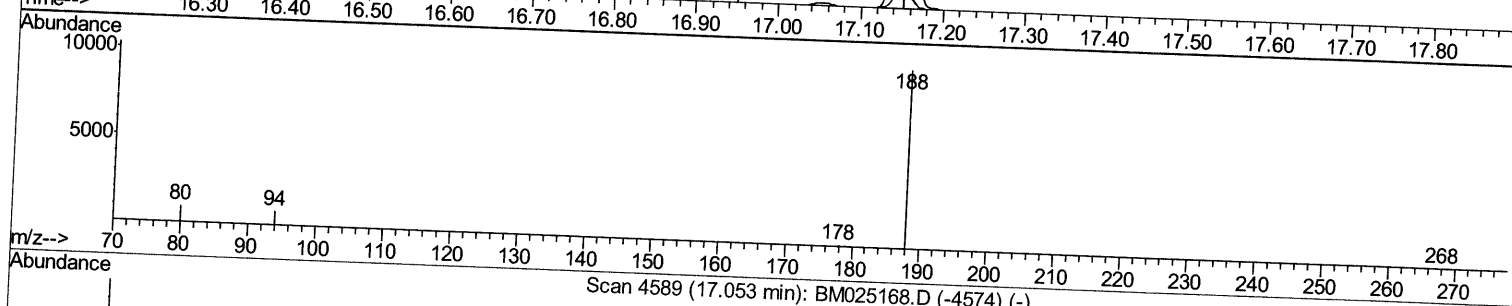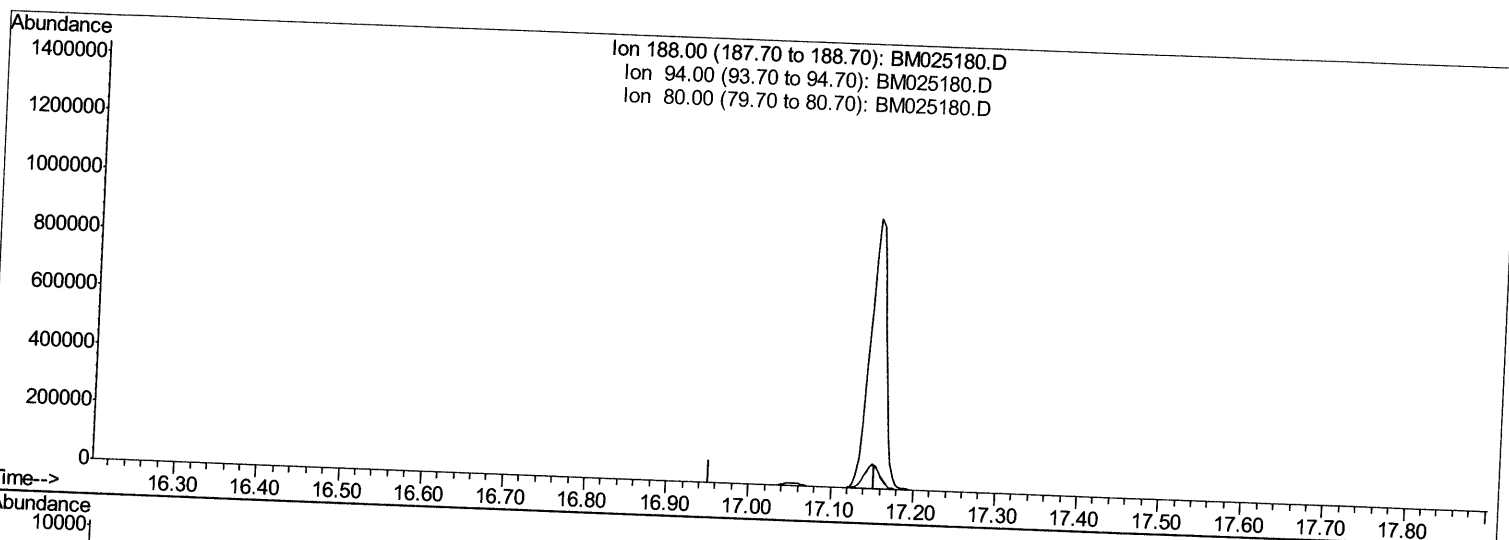

(10) Phenanthrene-d10 (I)

17.053min (-17.053) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (Qedit)




Data File : BM025180.D
Acq On : 29 Feb 2020 22:16
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:52 AM

Quant Time: Mar 02 02:11:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

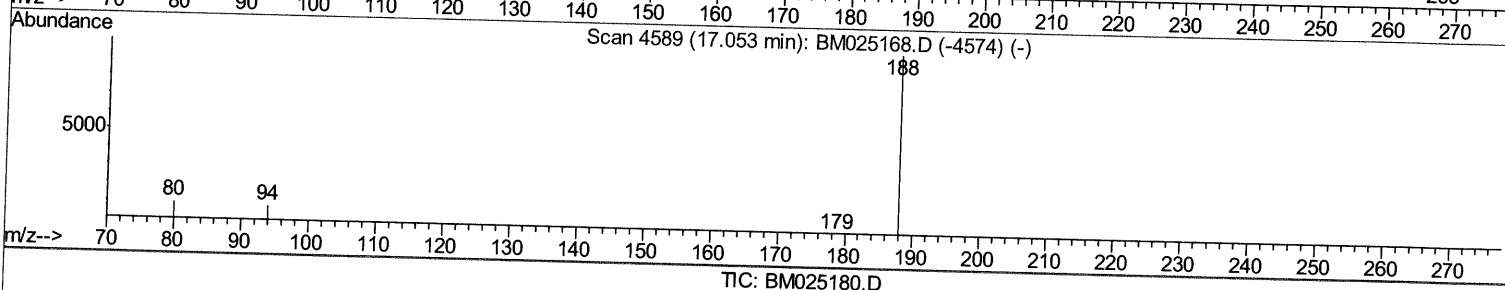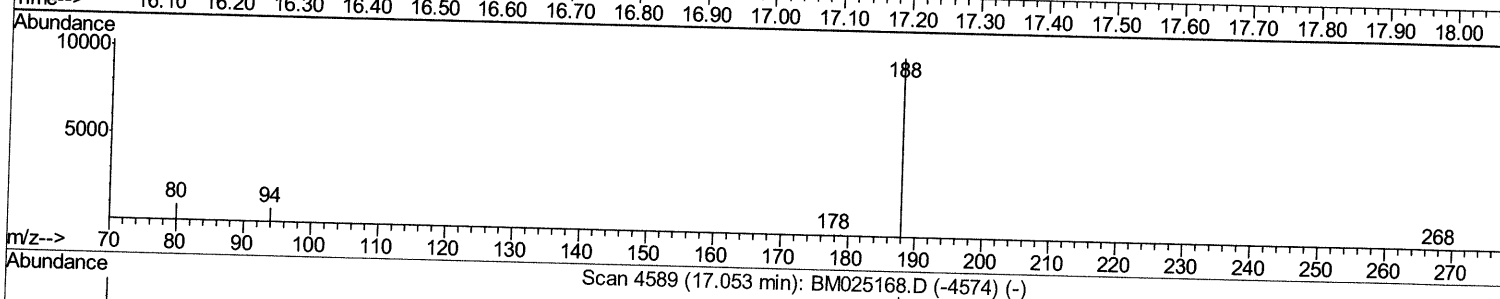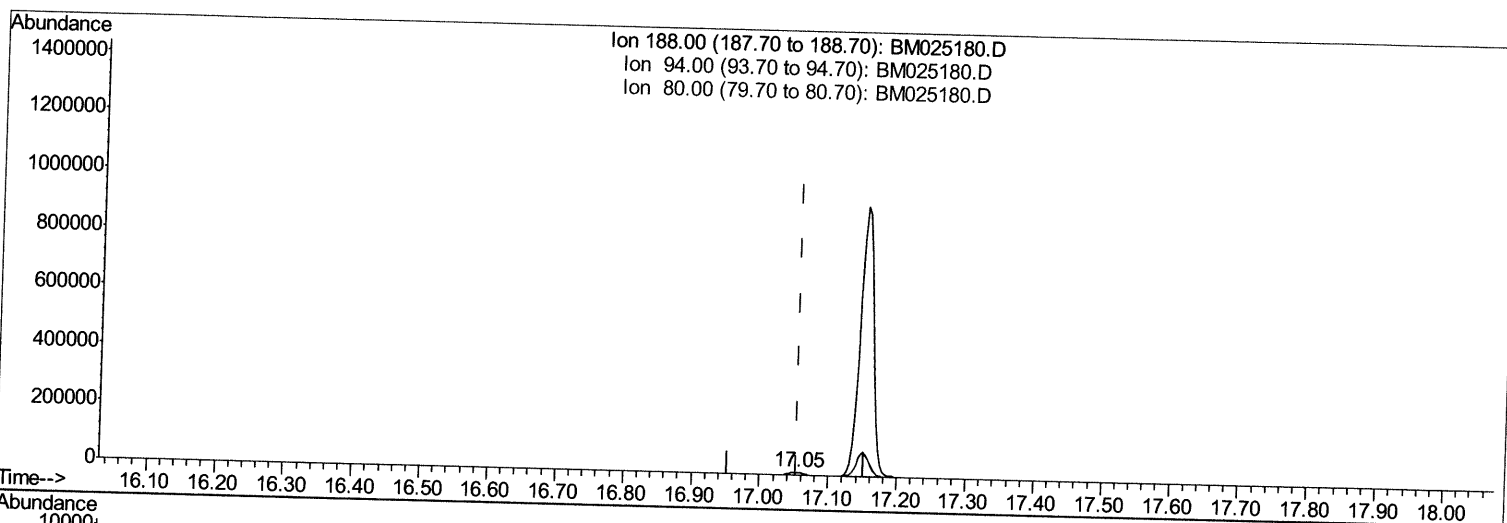

(10) Phenanthrene-d10 (I)

17.053min (+0.000) 0.40ng/ul m *Ju 03/02/20*

response 13619

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.34#
80.00	22.60	9.67#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022820\
Quantitation Report (QT Reviewed)

Data File : BM025180.D
Acq On : 29 Feb 2020 22:16
Operator : CG/JU
Sample : L1542-21
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD55

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:52 AM

Quant Time: Mar 02 03:10:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 02:08:15 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.68	152	2412	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	9387	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	6092	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	13619m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	14665	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	16871	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	6156	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	16272	0.35	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.11	202	1831	0.026	ng/ul	87
17) Pyrene	19.47	202	2831	0.043	ng/ul#	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed