

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022820\
 Data File : BM025148.D
 Acq On : 29 Feb 2020 00:09
 Operator : CG/JU
 Sample : L1507-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD13

Manual Integrations
 APPROVED

Sohil
 3/3/2020 8:39:21 AM

Quant Time: Feb 29 05:50:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Feb 29 04:43:59 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2689	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	10378	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	6768	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	15260m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	15861	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	17856	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	6865	0.35	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	18951	0.36	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.11	202	1713	0.022	ng/ul	91
17) Pyrene	19.47	202	1913	0.027	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022820\
Data File : BM025148.D
Acq On : 29 Feb 2020 00:09
Operator : CG/JU
Sample : L1507-15
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBD13

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:21 AM

Quant Time: Feb 29 05:50:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Feb 29 04:43:59 2020
Response via : Initial Calibration

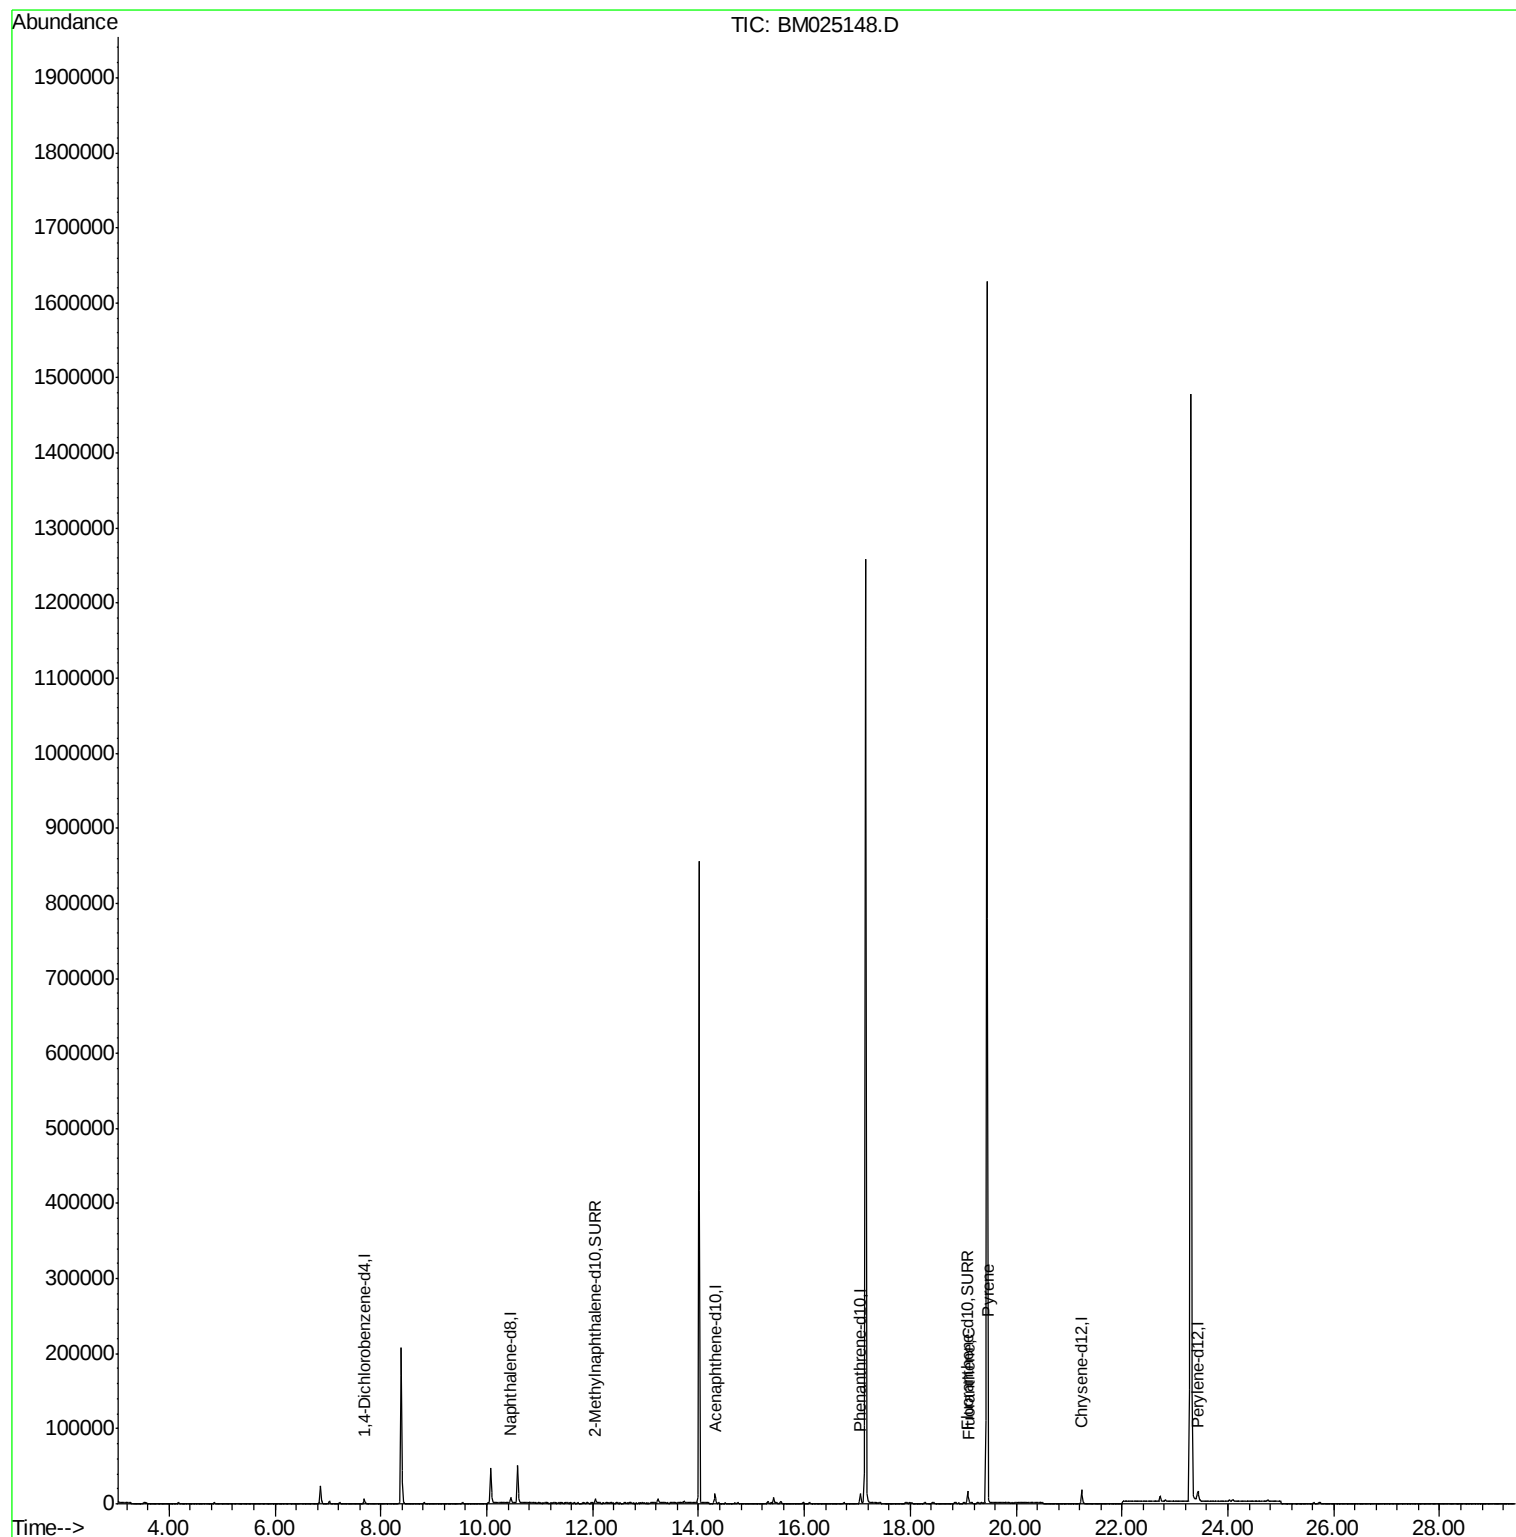

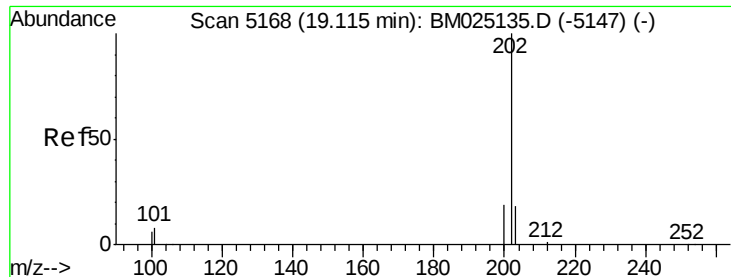





#15
Fluoranthene
Concen: 0.022 ng/ul
RT: 19.11 min Scan# 5167
Delta R.T. -0.00 min
Lab File: BM025148.D
Acq: 29 Feb 2020 00:09

Instrument :
BNA_M
ClientSampleId :
DBD13

Tot Ion	Ratio	Resp	Lower	Upper
202	100	1713		
101	13.9		0.0	29.4
100	10.0		0.0	28.0

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:21 AM

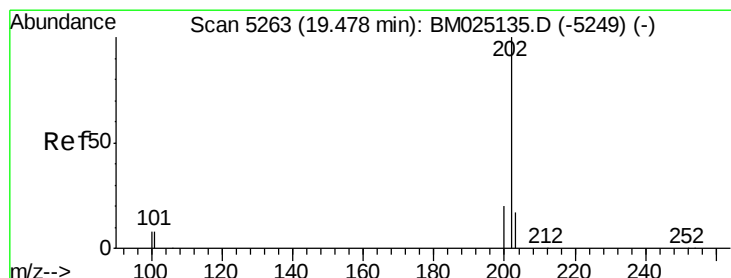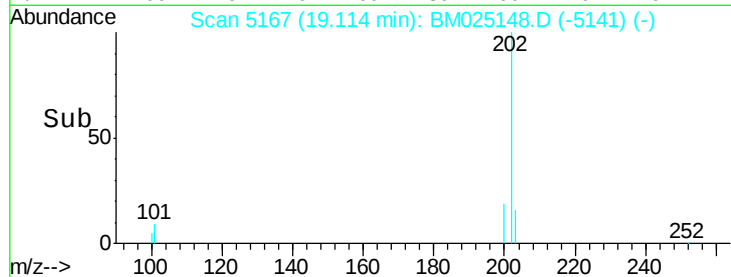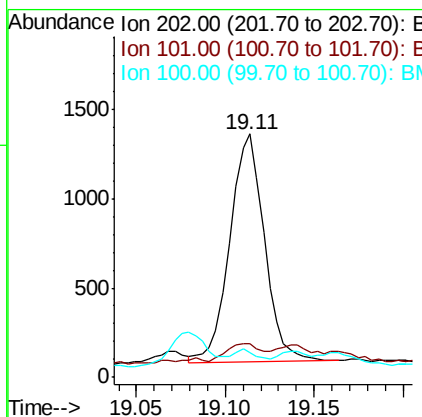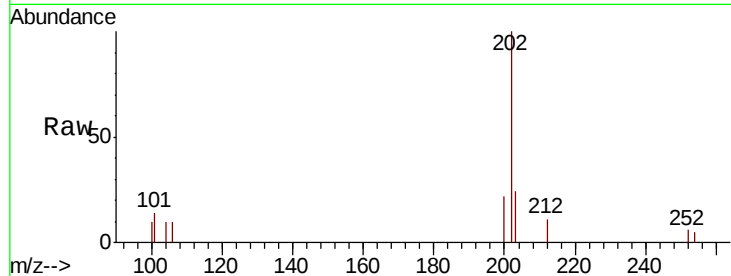

#17
Pyrene
Concen: 0.027 ng/ul
RT: 19.47 min Scan# 5261
Delta R.T. -0.01 min
Lab File: BM025148.D
Acq: 29 Feb 2020 00:09

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	1913		
101	16.8		8.7	13.1#
100	19.3		7.3	10.9#

