

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022820\
 Data File : BM025156.D
 Acq On : 29 Feb 2020 05:32
 Operator : CG/JU
 Sample : L1506-07DL 5X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBCY5DL

Manual Integrations
 APPROVED

Sohil
 3/3/2020 8:39:29 AM

Quant Time: Mar 02 01:00:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 02 00:36:45 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	3097	0.40	ng/ul	0.00
2) Naphthalene-d8	10.46	136	12047	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	7336	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	17179	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	17775	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	18865	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	362	0.02	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	1008	0.02	ng/ul	0.00
Target Compounds				Ovalue		
12) Phenanthrene	17.09	178	26275	0.435	ng/ul	96
13) Anthracene	17.18	178	13115	0.224	ng/ul	96
15) Fluoranthene	19.11	202	87011	0.991	ng/ul	94
17) Pyrene	19.47	202	73087	0.913	ng/ul	96
18) Benzo(a)anthracene	21.22	228	32918	0.429	ng/ul	99
19) Chrysene	21.27	228	30279	0.396	ng/ul	98
21) Benzo(b)fluoranthene	22.78	252	26275m	0.355	ng/ul	
22) Benzo(k)fluoranthene	22.82	252	9602m	0.131	ng/ul	
23) Benzo(a)pyrene	23.34	252	14598	0.216	ng/ul#	94
24) Indeno(1,2,3-cd)pyrene	25.62	276	6127	0.072	ng/ul#	100
25) Dibenzo(a,h)anthracene	25.63	278	1833	0.026	ng/ul#	59
26) Benzo(g,h,i)perylene	26.29	276	3898	0.055	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022820\
Data File : BM025156.D
Acq On : 29 Feb 2020 05:32
Operator : CG/JU
Sample : L1506-07DL 5X
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBCY5DL

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:29 AM

Quant Time: Mar 02 01:00:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 00:36:45 2020
Response via : Initial Calibration

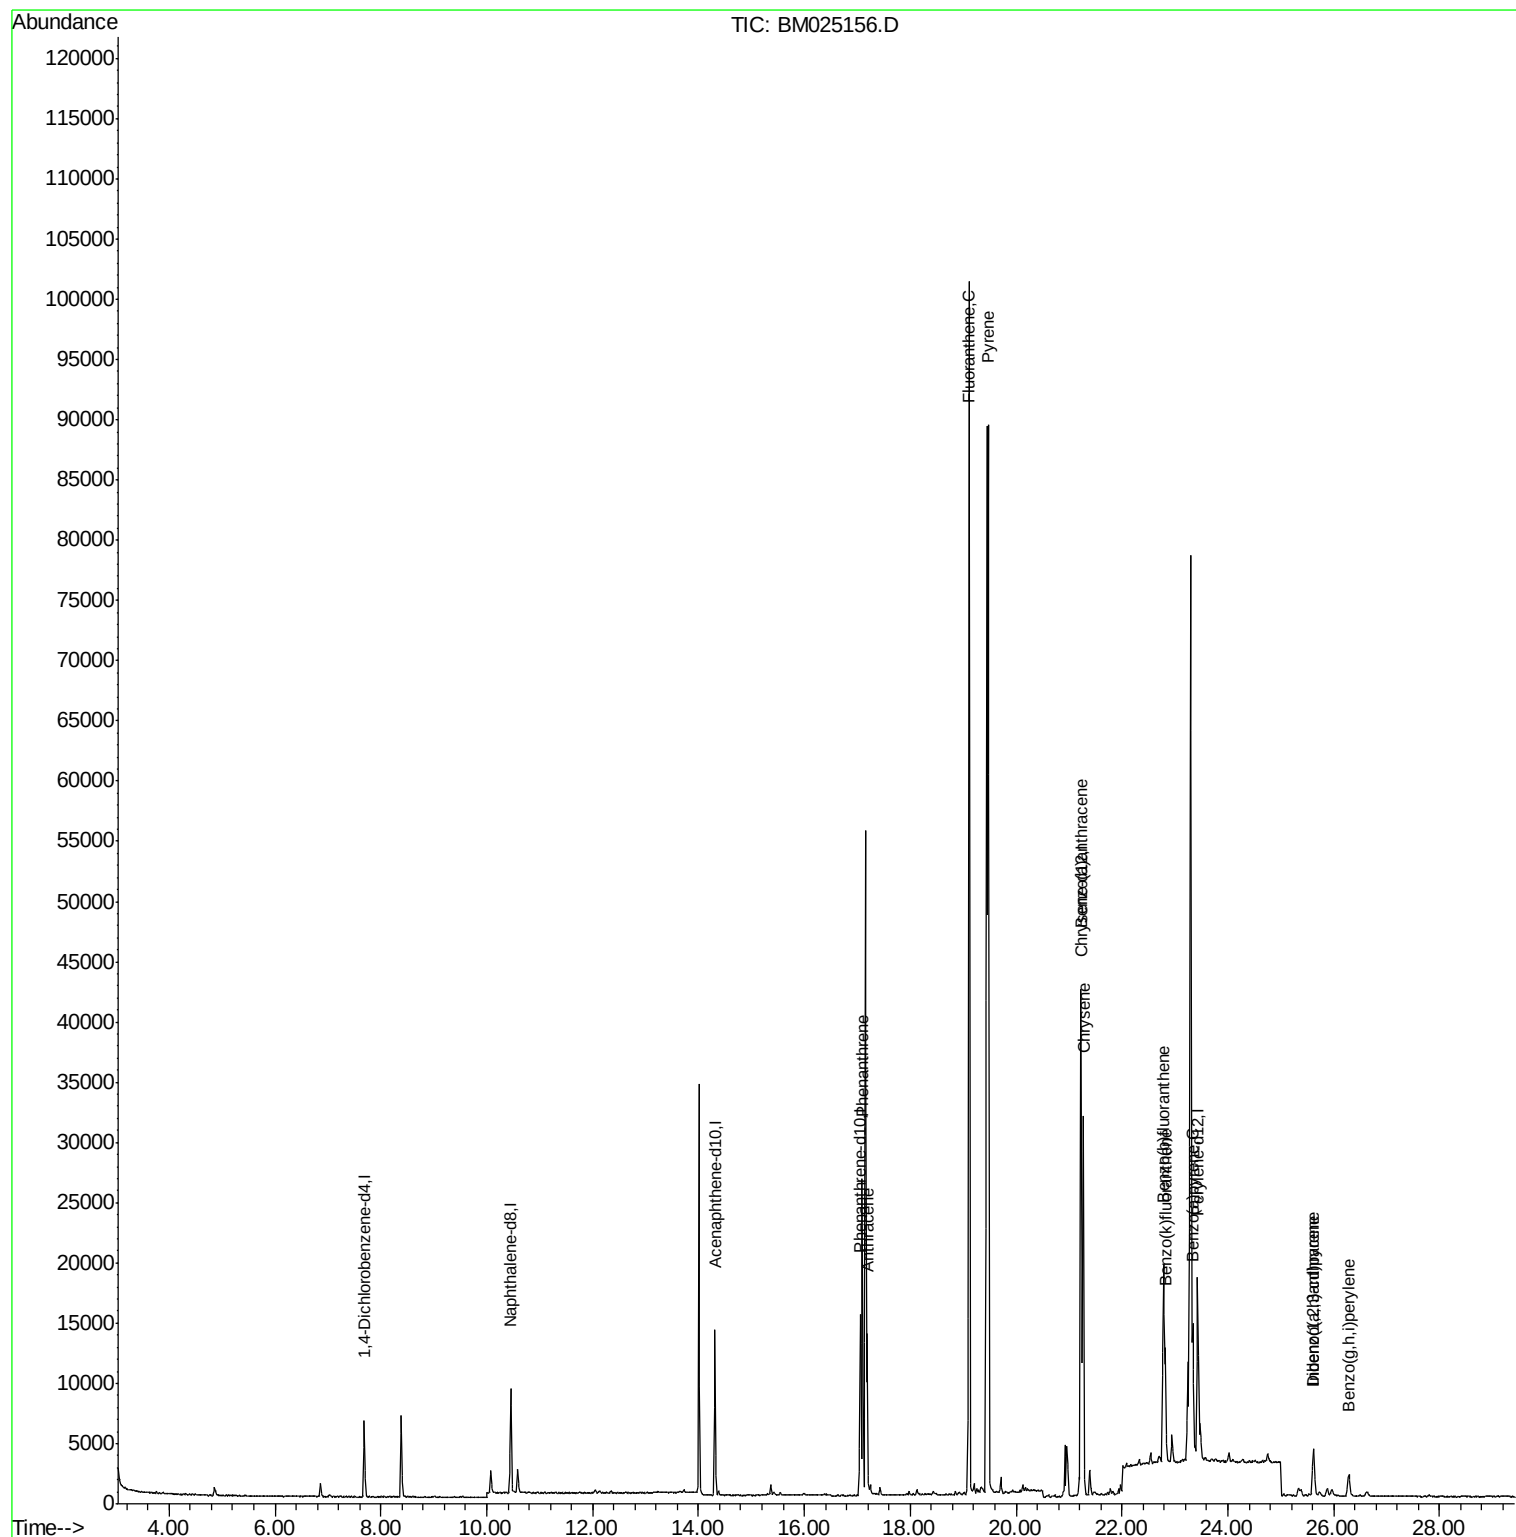

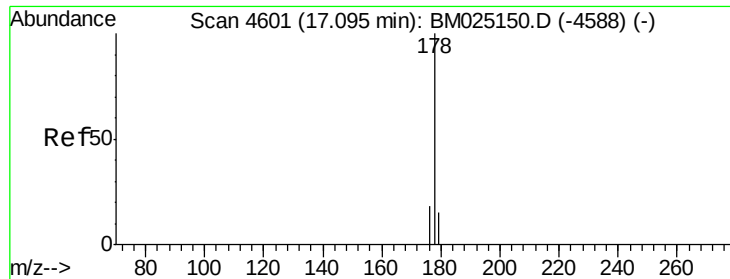

#12

Phenanthrene

Concen: 0.435 ng/ul

RT: 17.09 min Scan# 4601

Delta R.T. 0.00 min

Lab File: BM025156.D

Acq: 29 Feb 2020 05:32

Instrument :

BNA_M





ClientSampled :

DBCY5DL

Tot Ion:178	Resp:	26275
Ion Ratio	Lower	Upper
178	100	
179	16.1	14.0 21.0
176	18.4	16.6 24.8

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:29 AM

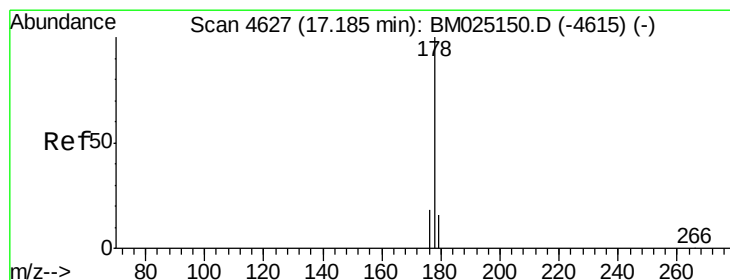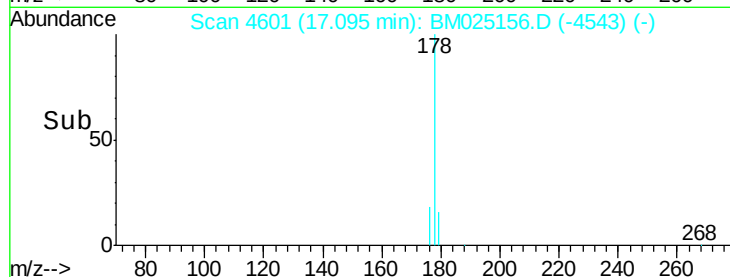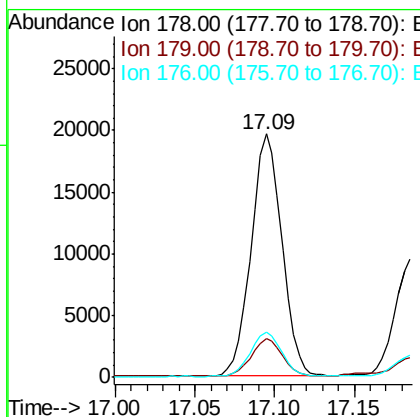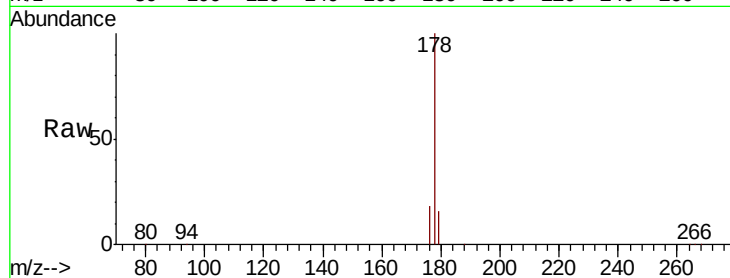

#13

Anthracene

Concen: 0.224 ng/ul




RT: 17.18 min Scan# 4627


Delta R.T. 0.00 min

Lab File: BM025156.D

Acq: 29 Feb 2020 05:32

Tgt Ion:178	Resp:	13115
Ion Ratio	Lower	Upper
178	100	
179	16.2	14.1 21.1
176	18.3	16.2 24.4

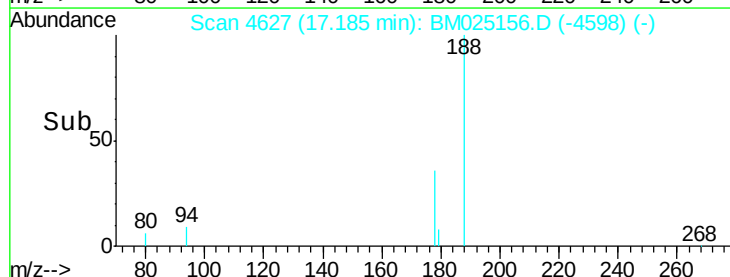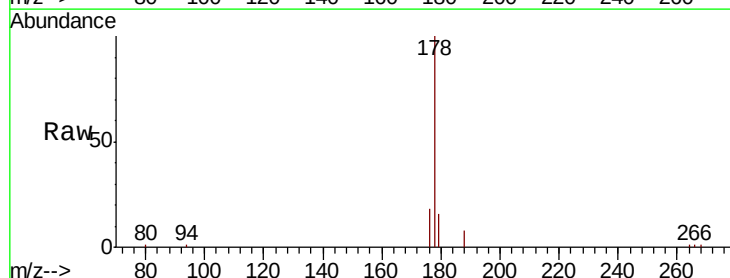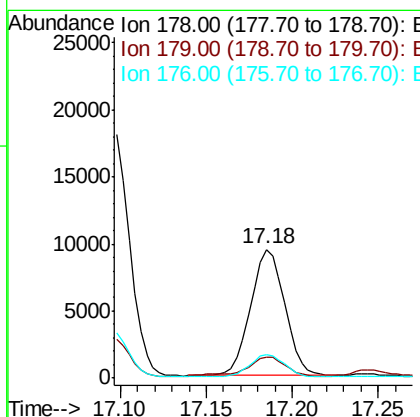

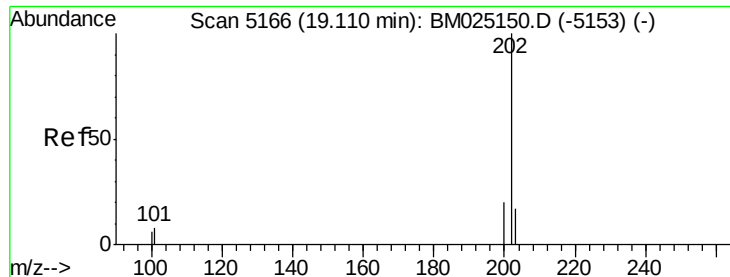





#15
Fluoranthene
 Concen: 0.991 ng/ul
 RT: 19.11 min Scan# 5167
 Delta R.T. 0.00 min
 Lab File: BM025156.D
 Acq: 29 Feb 2020 05:32

Instrument :
 BNA_M
 ClientSampleId :
 DBCY5DL

Tot Ion:	202	Resp:	87011
Ion Ratio	Lower	Upper	
202	100		
101	7.6	0.0	29.4
100	5.7	0.0	28.0




Manual Integrations
 APPROVED


Sohil
 3/3/2020 8:39:29 AM

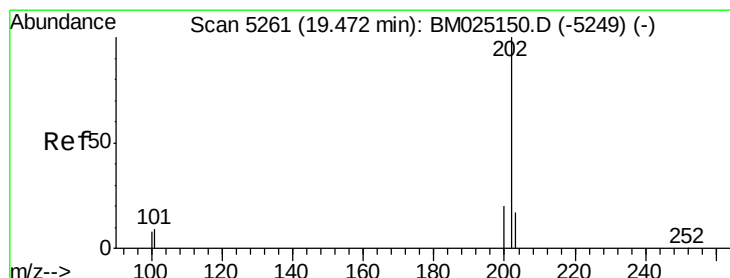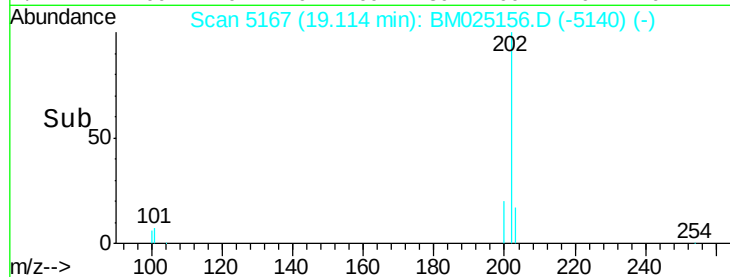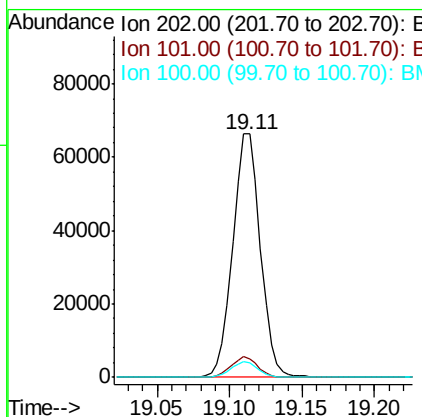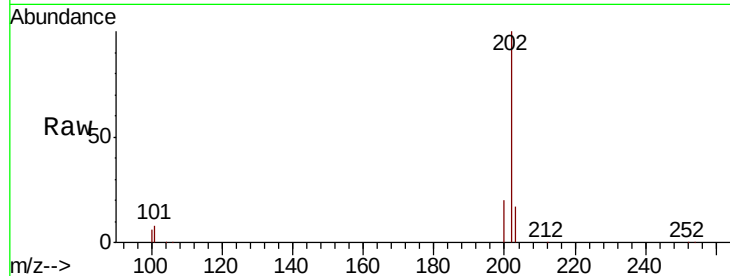

#17
Pyrene
 Concen: 0.913 ng/ul
 RT: 19.47 min Scan# 5261
 Delta R.T. 0.00 min
 Lab File: BM025156.D
 Acq: 29 Feb 2020 05:32

Tgt Ion:	202	Resp:	73087
Ion Ratio	Lower	Upper	
202	100		
101	9.4	8.7	13.1
100	7.7	7.3	10.9

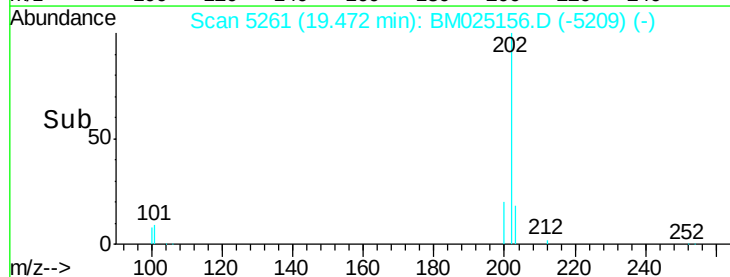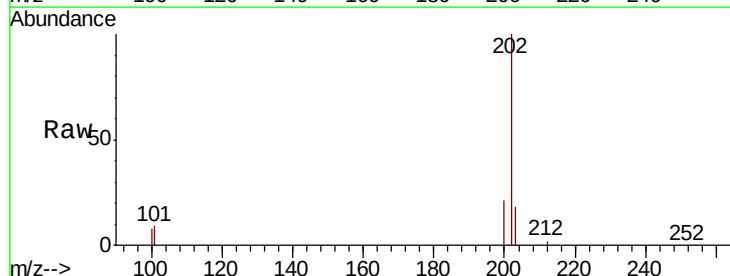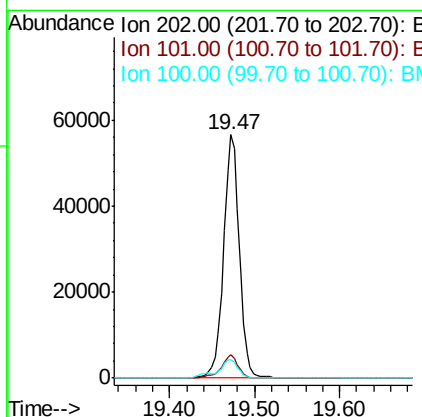

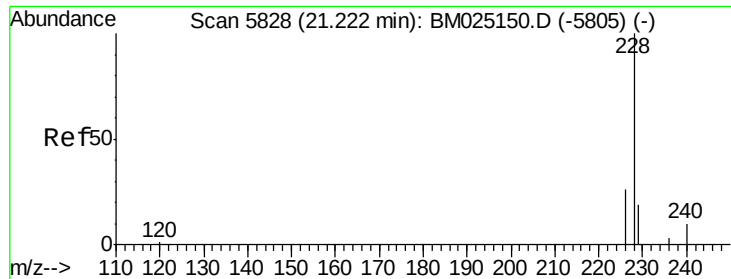





#18
Benzo(a)anthracene
Concen: 0.429 ng/ul
RT: 21.22 min Scan# 5828
Delta R.T. 0.00 min
Lab File: BM025156.D
Acq: 29 Feb 2020 05:32

Instrument :
BNA_M
ClientSampleId :
DBCY5DL

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.6	16.6	25.0
226	26.8	21.9	32.9




Manual Integrations
APPROVED


Sohil
3/3/2020 8:39:29 AM

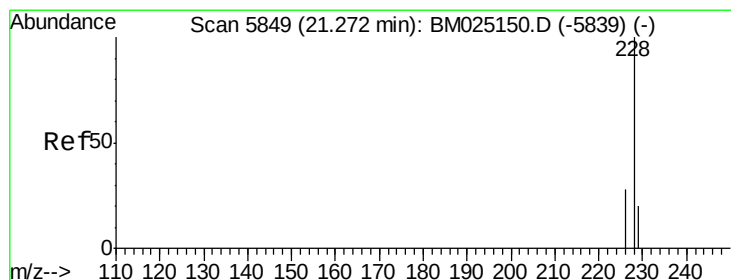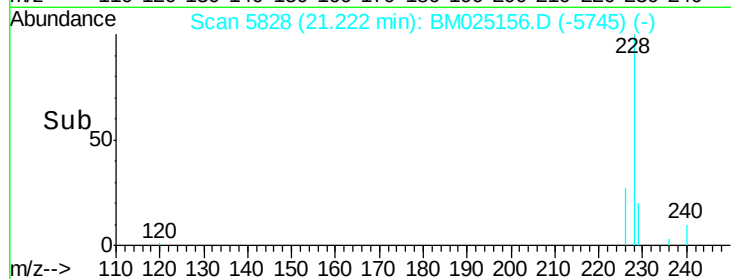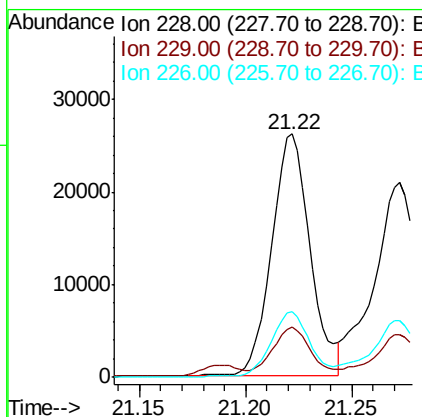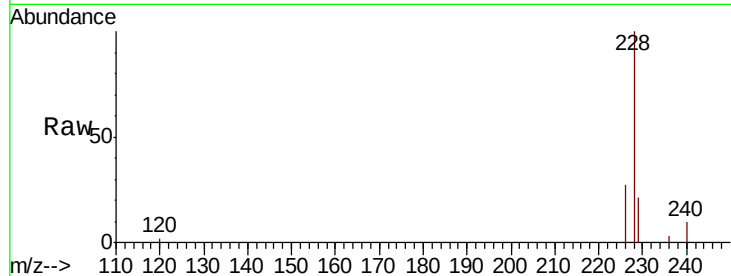

#19
Chrysene
Concen: 0.396 ng/ul
RT: 21.27 min Scan# 5849
Delta R.T. 0.00 min
Lab File: BM025156.D
Acq: 29 Feb 2020 05:32

Tgt Ion	Ratio	Lower	Upper
228	100		
226	28.9	23.8	35.8
229	22.2	16.9	25.3

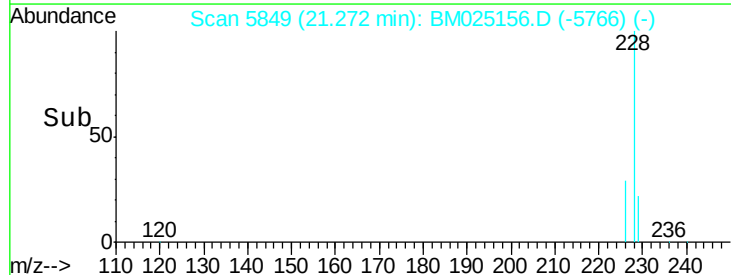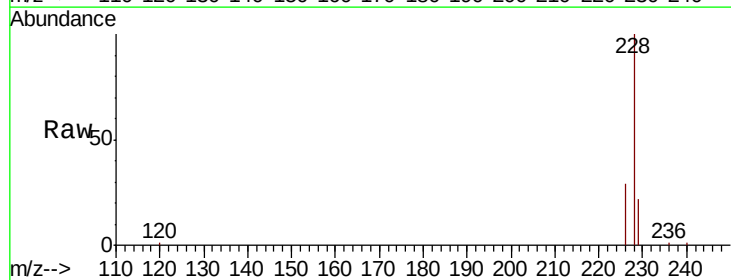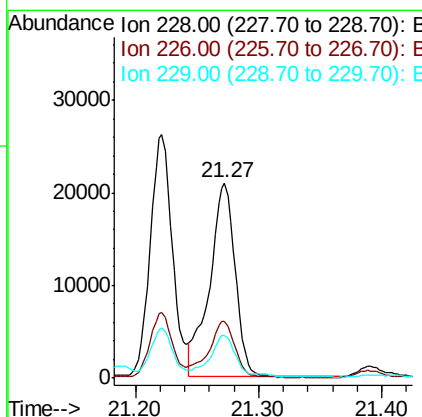

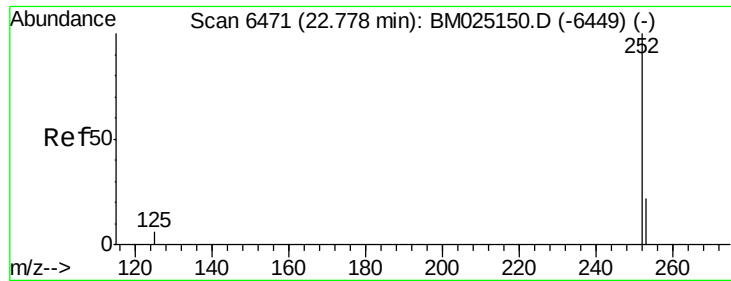





#21
Benzo(b)fluoranthene
Concen: 0.355 ng/ul m
RT: 22.78 min Scan# 6472
Delta R.T. 0.00 min
Lab File: BM025156.D
Acq: 29 Feb 2020 05:32

Instrument :
BNA_M
ClientSampleId :
DBCY5DL

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.7	0.0	49.8
125	9.9	0.0	28.6




Manual Integrations
APPROVED


Sohil
3/3/2020 8:39:29 AM

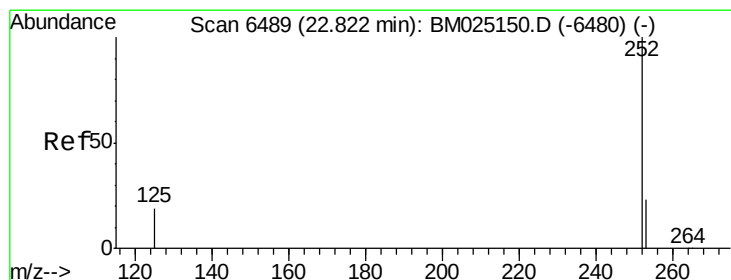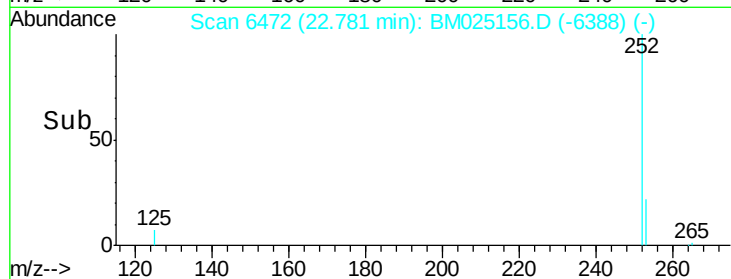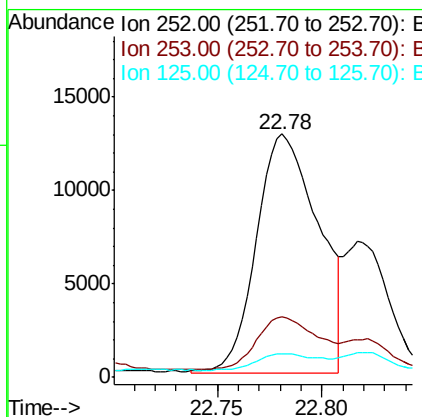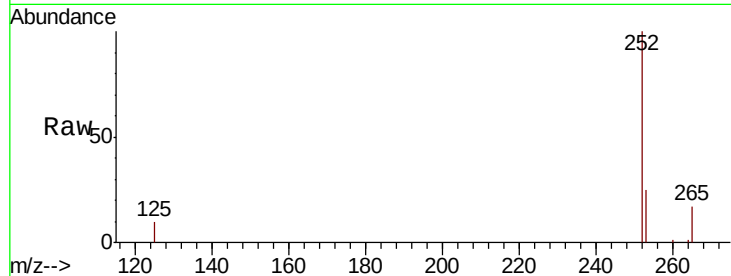

#22
Benzo(k)fluoranthene
Concen: 0.131 ng/ul m
RT: 22.82 min Scan# 6487
Delta R.T. -0.00 min
Lab File: BM025156.D
Acq: 29 Feb 2020 05:32

Tgt Ion	Ratio	Lower	Upper
252	100		
253	27.7	19.4	29.0
125	18.1	10.7	16.1

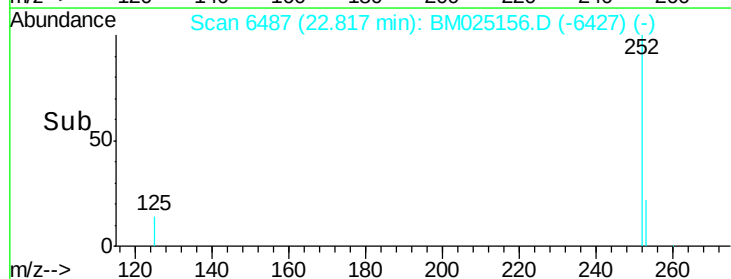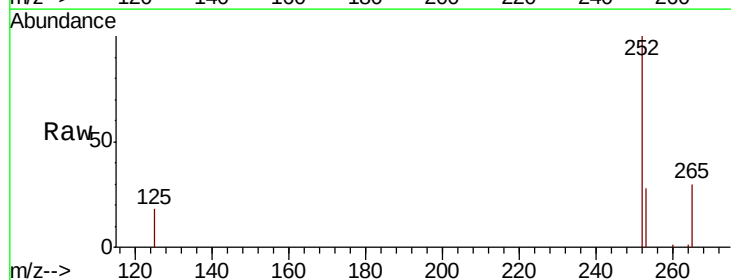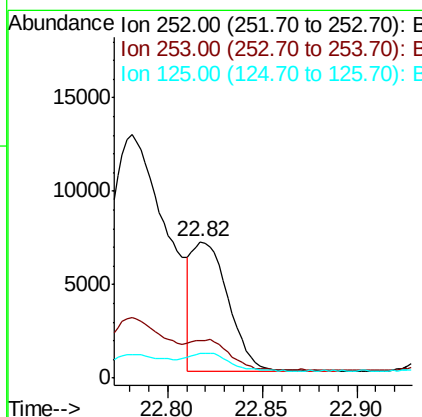

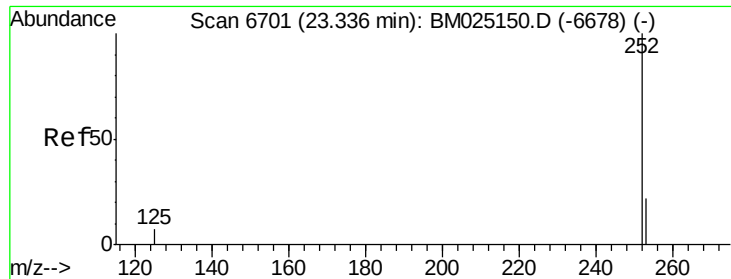

#23

Benzo(a)pyrene

Concen: 0.216 ng/ul

RT: 23.34 min Scan# 6702

Delta R.T. 0.00 min

Lab File: BM025156.D

Acq: 29 Feb 2020 05:32

Instrument :

BNA_M





ClientSampleId :

DBCY5DL

Tot Ion:	252	Resp:	14598
Ion Ratio	Lower	Upper	
252	100		
253	26.6	20.3	30.5
125	11.4	13.0	19.4#

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:29 AM

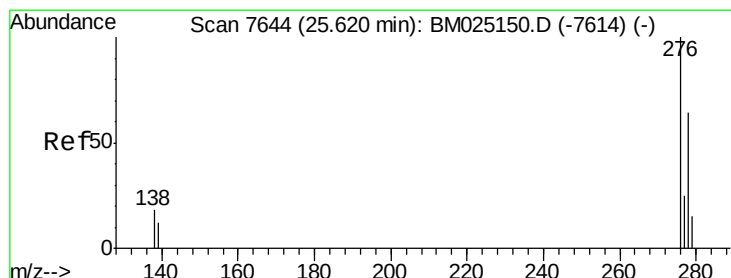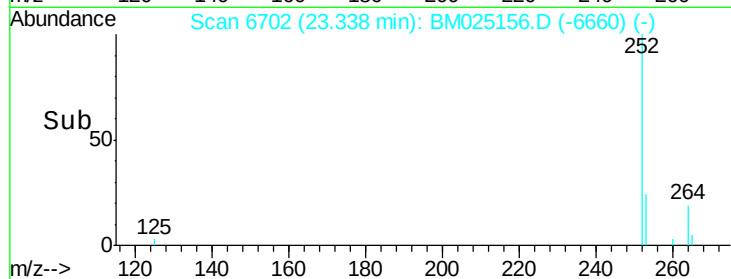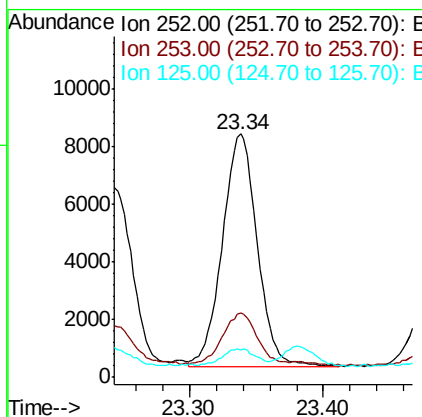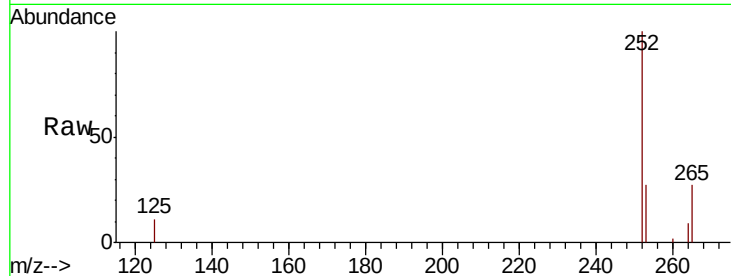

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.072 ng/ul




RT: 25.62 min Scan# 7642


Delta R.T. -0.00 min

Lab File: BM025156.D

Acq: 29 Feb 2020 05:32

Tgt Ion:	276	Resp:	6127
Ion Ratio	Lower	Upper	
276	100		
138	16.5	0.0	0.0#
227	0.0	0.0	0.0

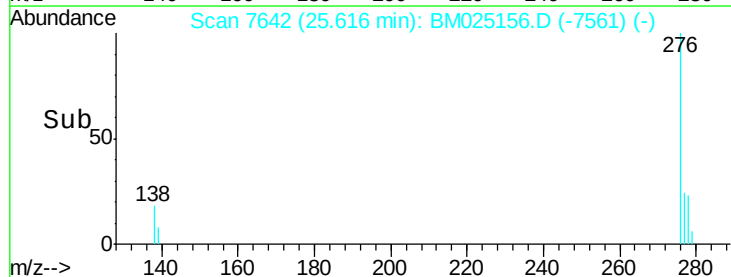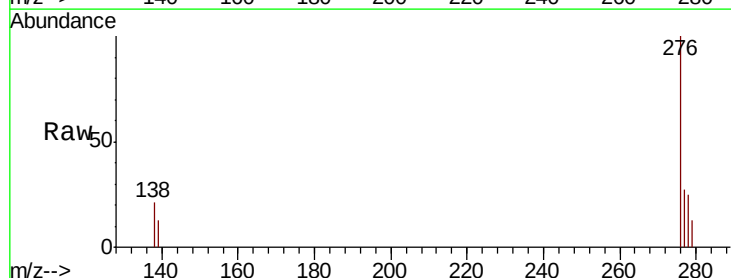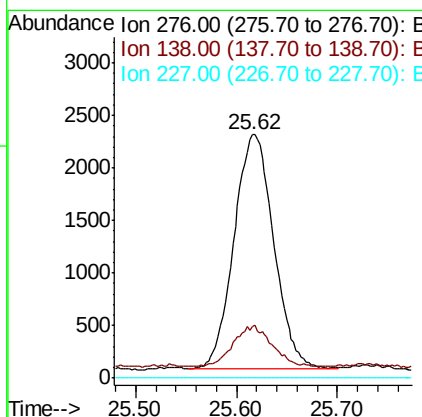

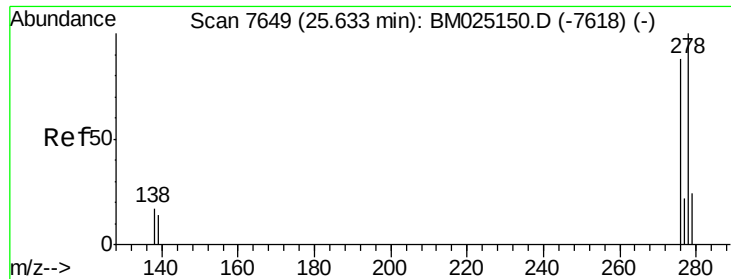





#25
Dibenzo(a,h)anthracene
Concen: 0.026 ng/ul
RT: 25.63 min Scan# 7648
Delta R.T. -0.00 min
Lab File: BM025156.D
Acq: 29 Feb 2020 05:32

Instrument :
BNA_M
ClientSampleId :
DBCY5DL

Tot Ion	Ratio	Lower	Upper
278	100		
139	35.9	13.2	19.8#
279	45.9	21.0	31.4#

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:29 AM

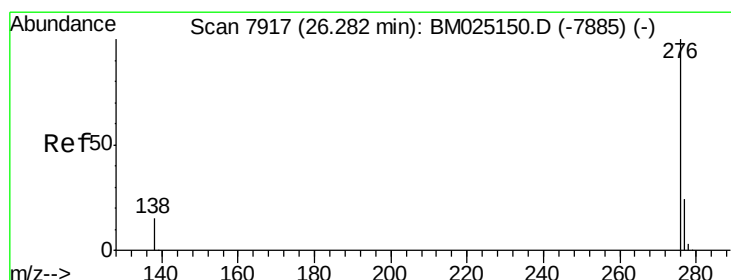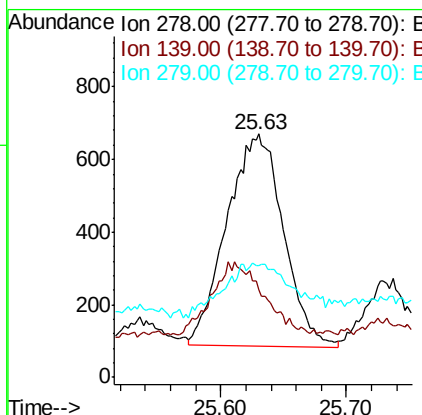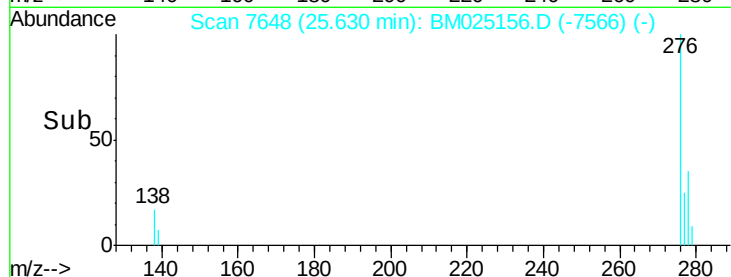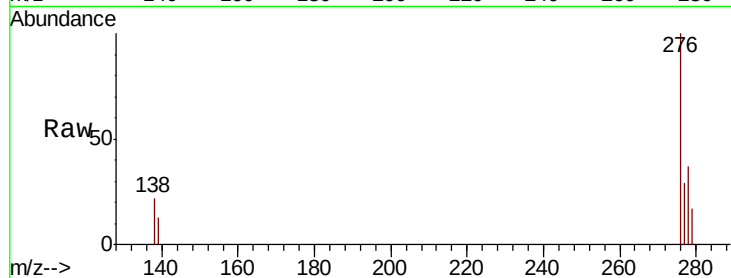

#26
Benzo(g,h,i)perylene
Concen: 0.055 ng/ul
RT: 26.29 min Scan# 7919
Delta R.T. 0.00 min
Lab File: BM025156.D
Acq: 29 Feb 2020 05:32

Tgt Ion	Ratio	Lower	Upper
276	100		
138	19.8	17.9	26.9
277	28.7	20.5	30.7

