

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022820\
 Data File : BM025162.D
 Acq On : 29 Feb 2020 11:30
 Operator : CG/JU
 Sample : L1542-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD40

Manual Integrations
 APPROVED

Sohil
 3/3/2020 8:39:35 AM

Quant Time: Mar 02 01:45:25 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 02 01:15:39 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	2348	0.40	ng/ul	0.00
2) Naphthalene-d8	10.45	136	9191	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.31	164	6036	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.05	188	13615m	0.40	ng/ul	0.00
16) Chrysene-d12	21.24	240	13974	0.40	ng/ul	0.00
20) Perylene-d12	23.43	264	15979	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.05	152	6943	0.40	ng/ul	0.00
14) Fluoranthene-d10	19.08	212	17981	0.39	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.09	178	2256	0.047	ng/ul#	92
15) Fluoranthene	19.11	202	2170	0.031	ng/ul	90
17) Pyrene	19.47	202	2302	0.037	ng/ul#	83

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022820\
Data File : BM025162.D
Acq On : 29 Feb 2020 11:30
Operator : CG/JU
Sample : L1542-04
Misc :
ALS Vial : 35 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
DBD40

Manual Integrations
APPROVED

Sohil
3/3/2020 8:39:35 AM

Quant Time: Mar 02 01:45:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 02 01:15:39 2020
Response via : Initial Calibration

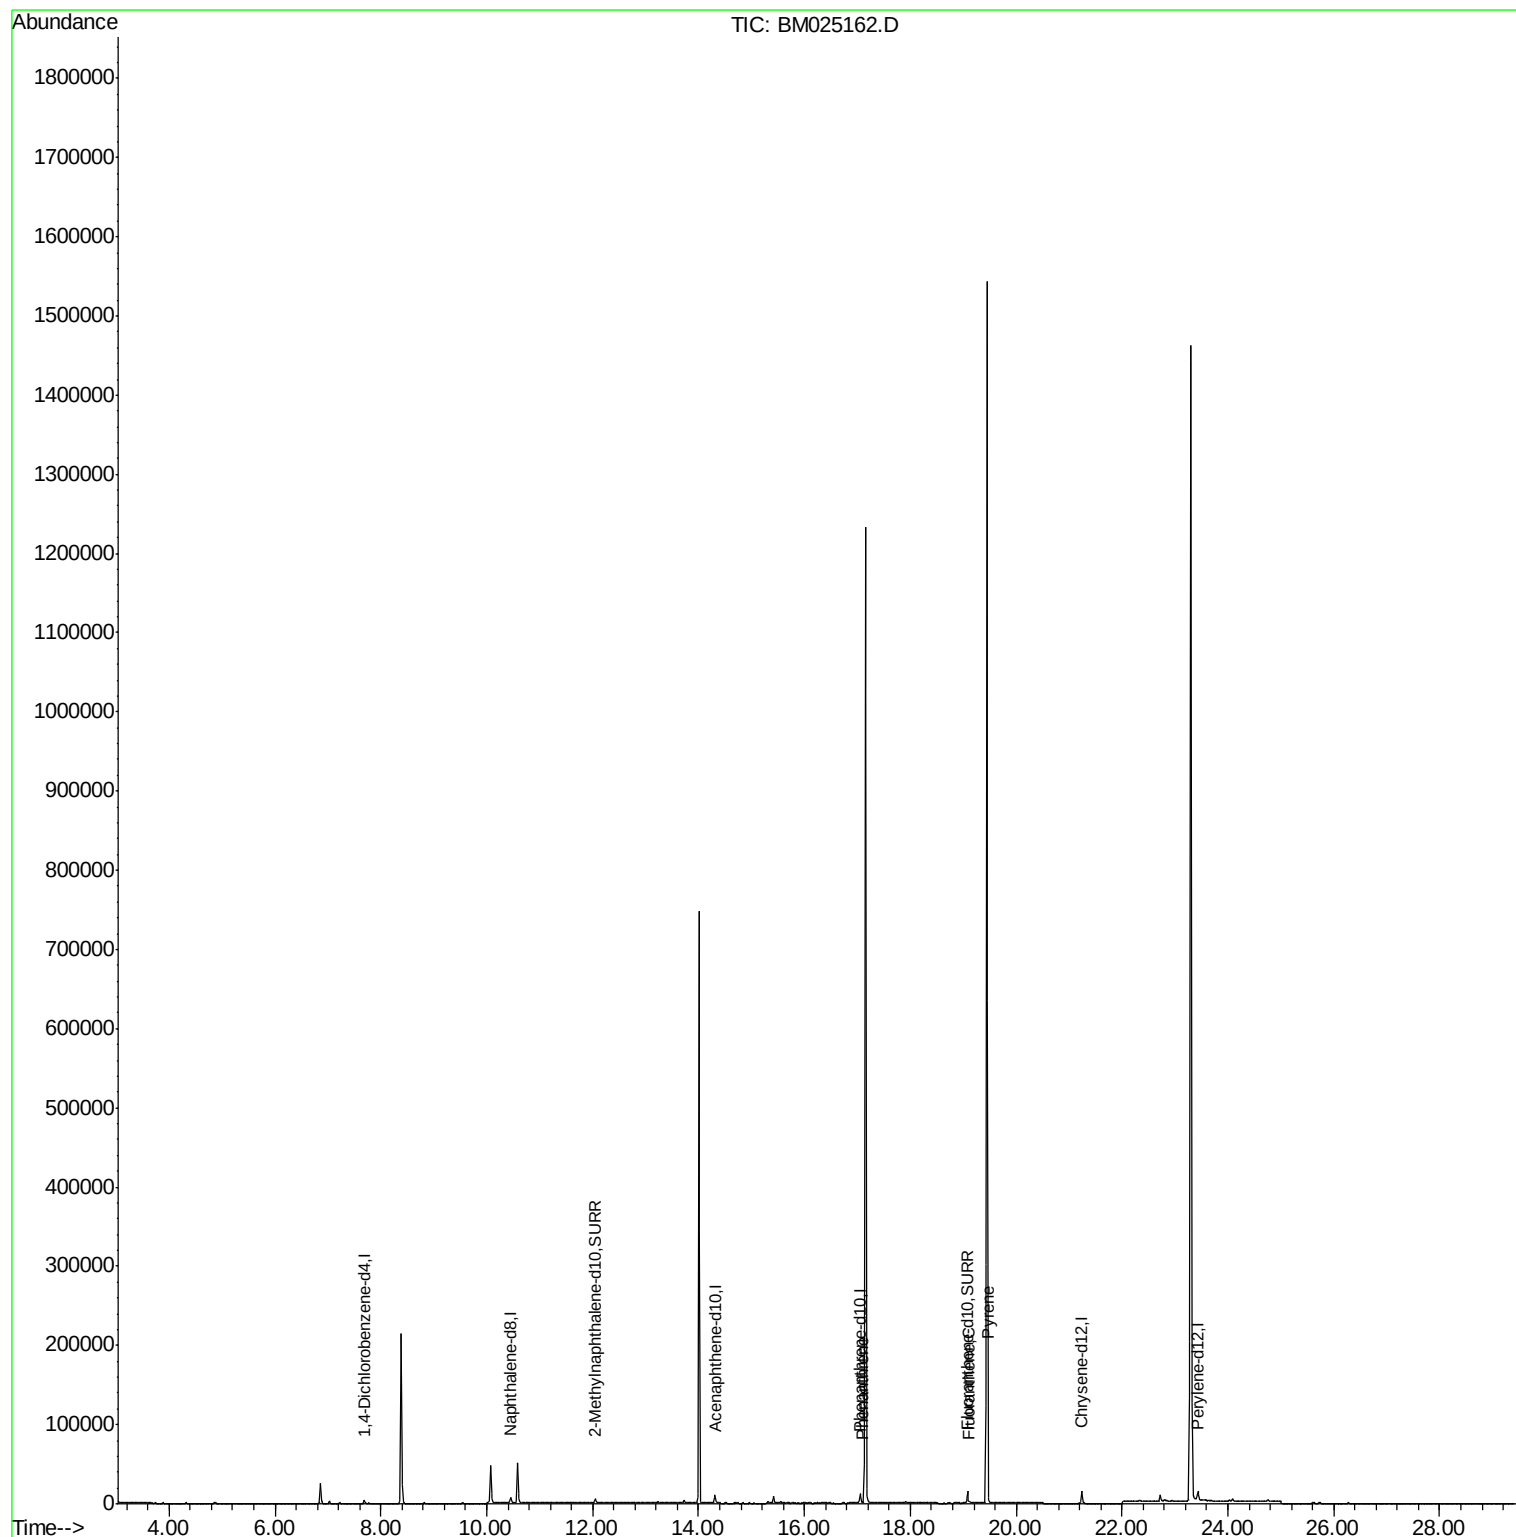

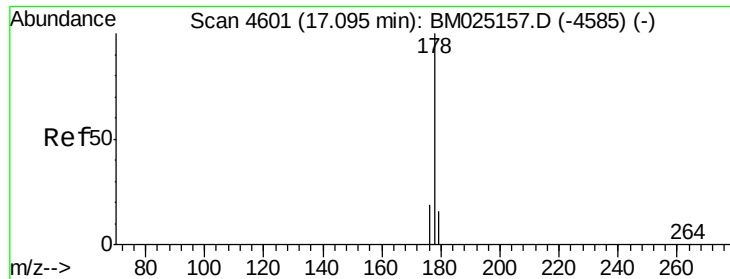





#12
Phenanthrene
Concen: 0.047 ng/ul
RT: 17.09 min Scan# 4601
Delta R.T. 0.00 min
Lab File: BM025162.D
Acq: 29 Feb 2020 11:30

Instrument :
BNA_M
ClientSampleId :
DBD40

Tot Ion	Ratio	Lower	Upper
178	100		
179	23.2	14.0	21.0#
176	22.4	16.6	24.8




Manual Integrations
APPROVED




Sohil
3/3/2020 8:39:35 AM

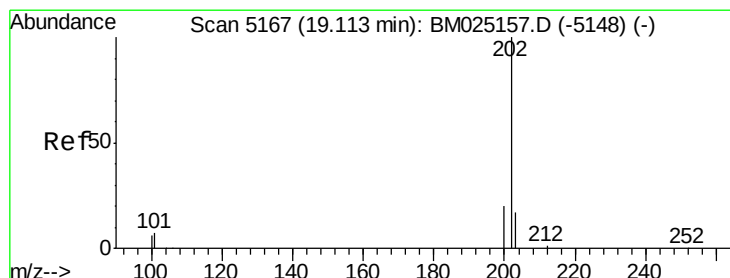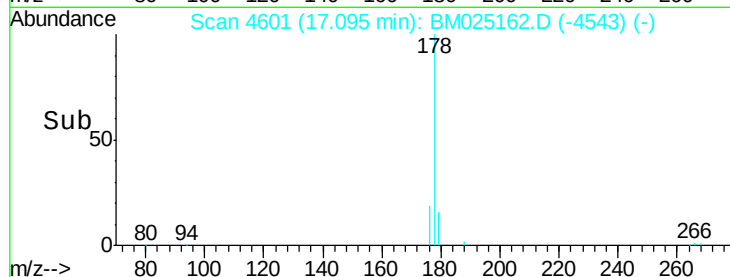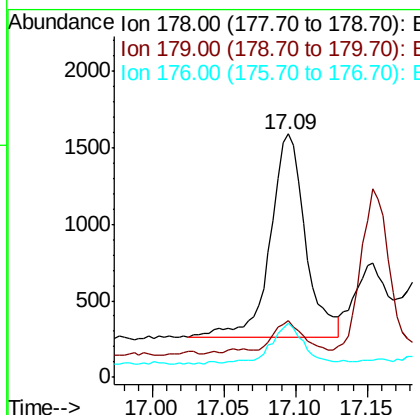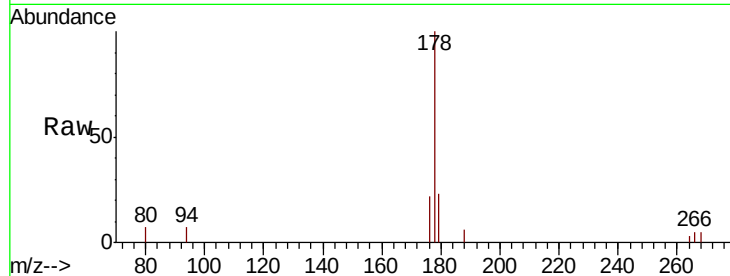

#15
Fluoranthene
Concen: 0.031 ng/ul
RT: 19.11 min Scan# 5166
Delta R.T. -0.00 min
Lab File: BM025162.D
Acq: 29 Feb 2020 11:30

Tgt Ion	Ratio	Lower	Upper
202	100		
101	13.8	0.0	29.4
100	10.7	0.0	28.0

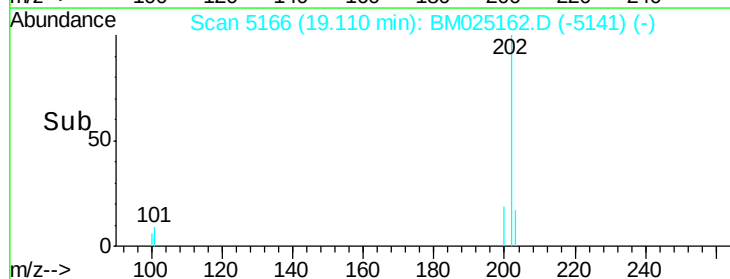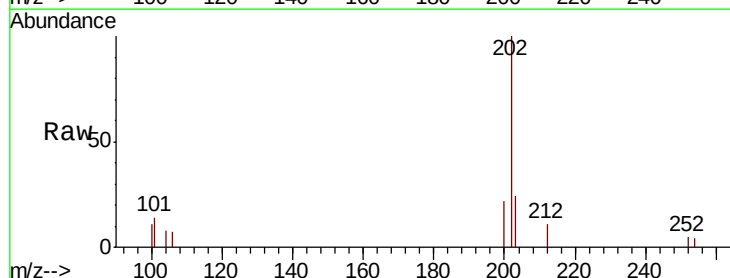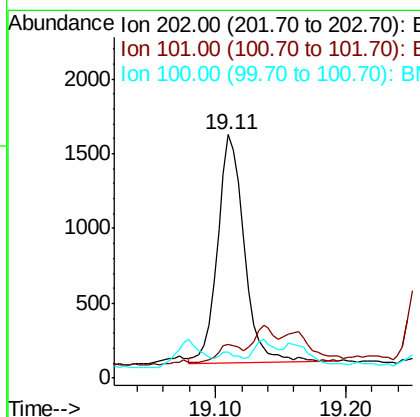

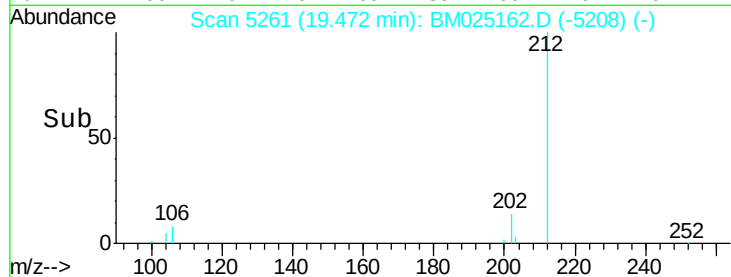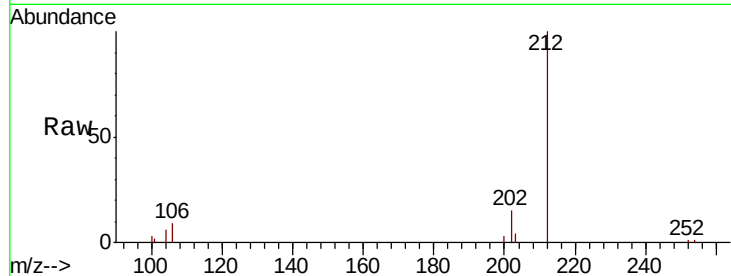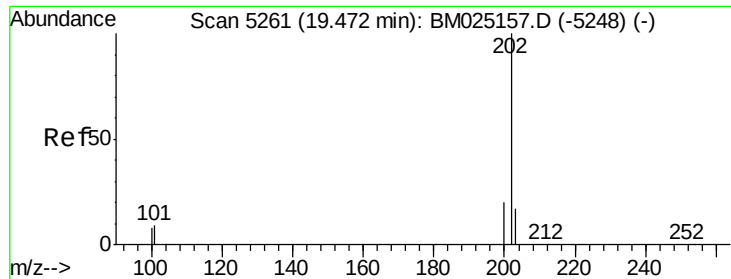

#17
 Pvrene
 Concen: 0.037 ng/ul
 RT: 19.47 min Scan# 5261
 Delta R.T. 0.00 min
 Lab File: BM025162.D
 Acq: 29 Feb 2020 11:30

Instrument :
 BNA_M
 ClientSampleId :
 DBD40

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	15.9	8.7	13.1#
100	16.8	7.3	10.9#

Manual Integrations
 APPROVED

Sohil
 3/3/2020 8:39:35 AM

