
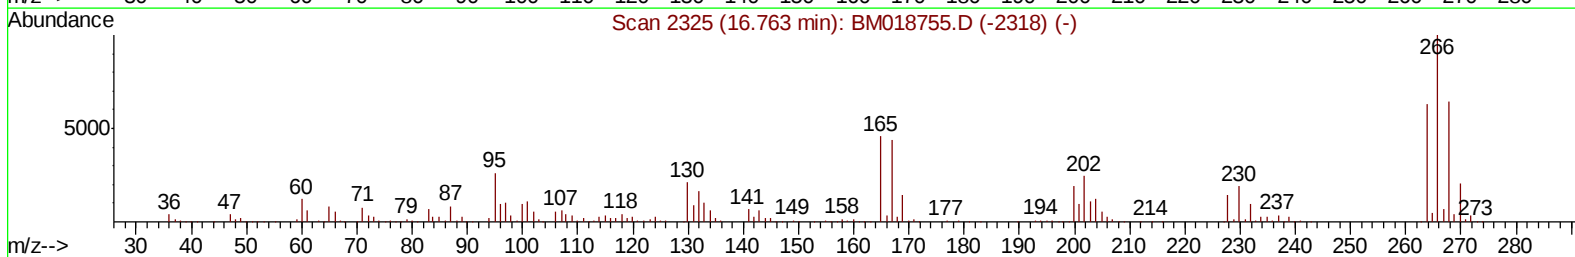
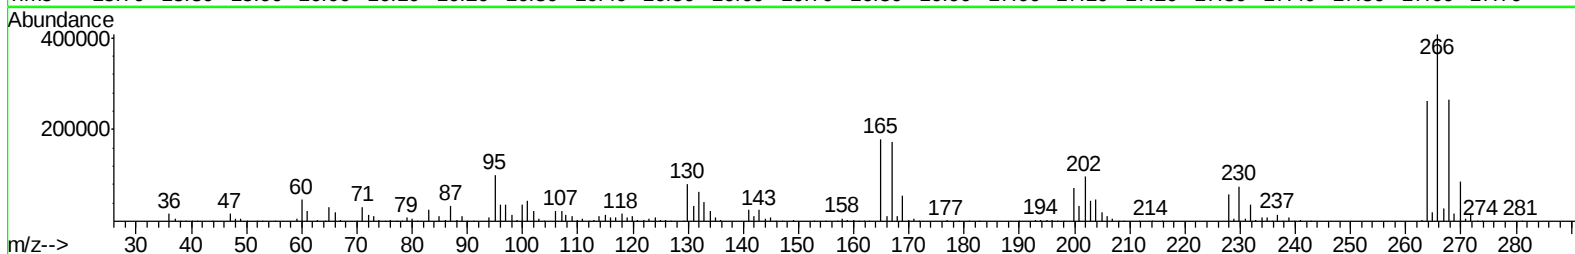


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030119\
Data File : BM018985.D
Acq On : 01 Mar 2019 12:56
Operator : JU/SJ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 01 14:18:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 01 14:12:30 2019
Response via : Initial Calibration

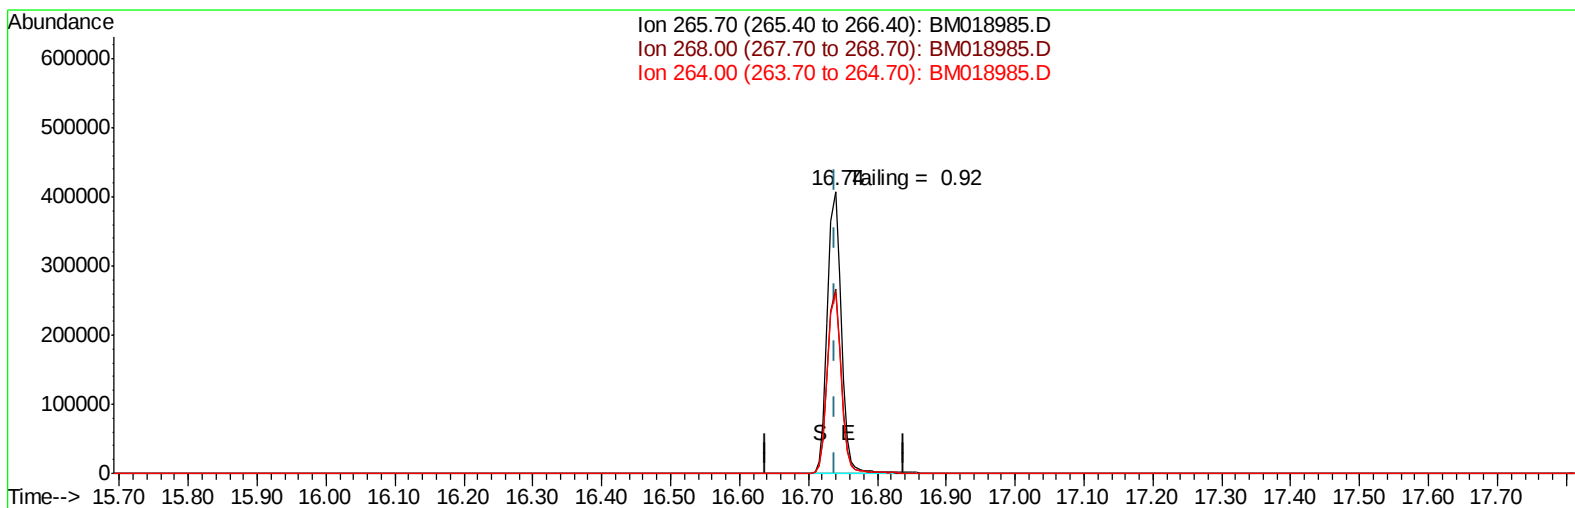

TIC: BM018985.D

(70) Pentachlorophenol (C)




16.739min (0.000) 42.84ng

response 567332

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	65.43
264.00	63.20	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030119\
 Data File : BM018985.D
 Acq On : 01 Mar 2019 12:56
 Operator : JU/SJ
 Sample : SSTDCCC040
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 01 14:18:55 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 01 14:12:30 2019
 Response via : Initial Calibration

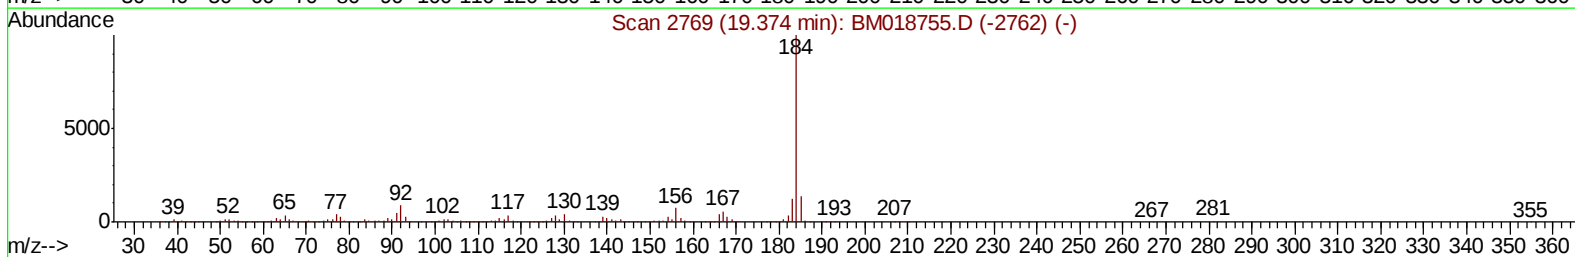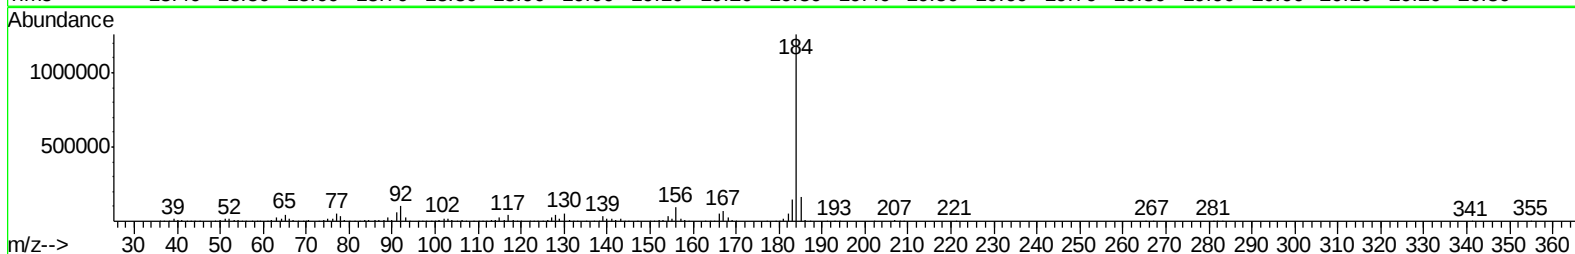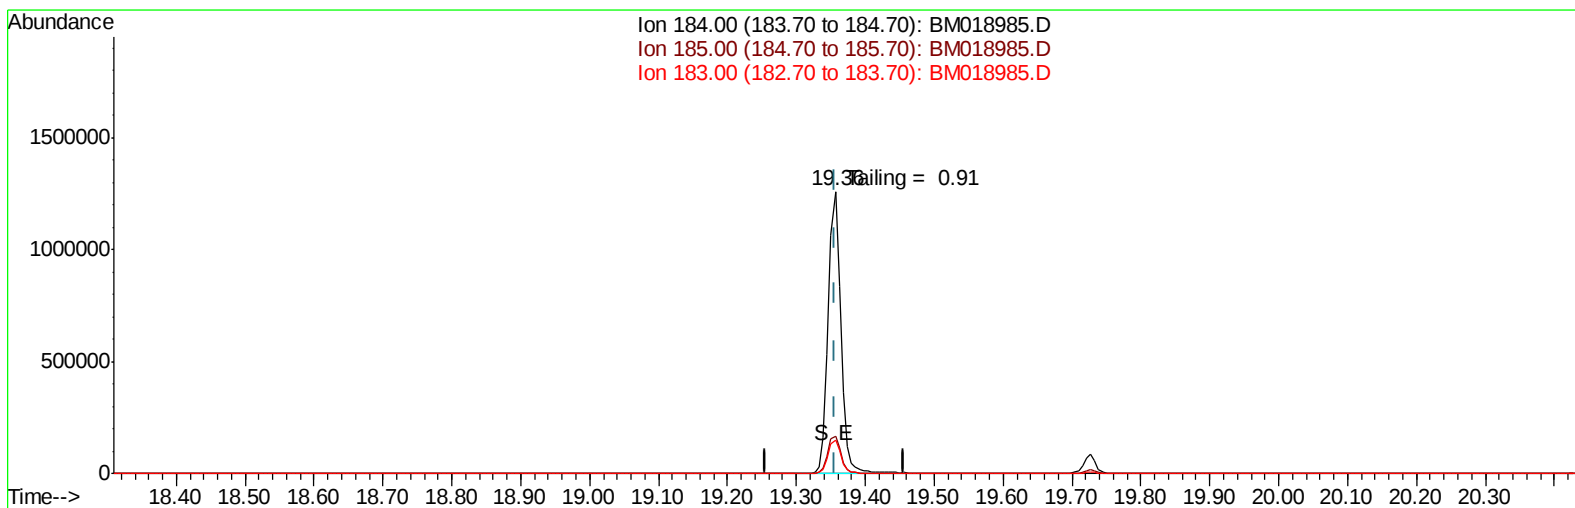

TIC: BM018985.D

(77) Benzidine

19.356min (0.000) 45.66ng

response 1591643

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.36
183.00	12.10	12.02
0.00	0.00	0.00