


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030119\
 Data File : BM018984.D
 Acq On : 01 Mar 2019 12:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 11 16:02:12 2019

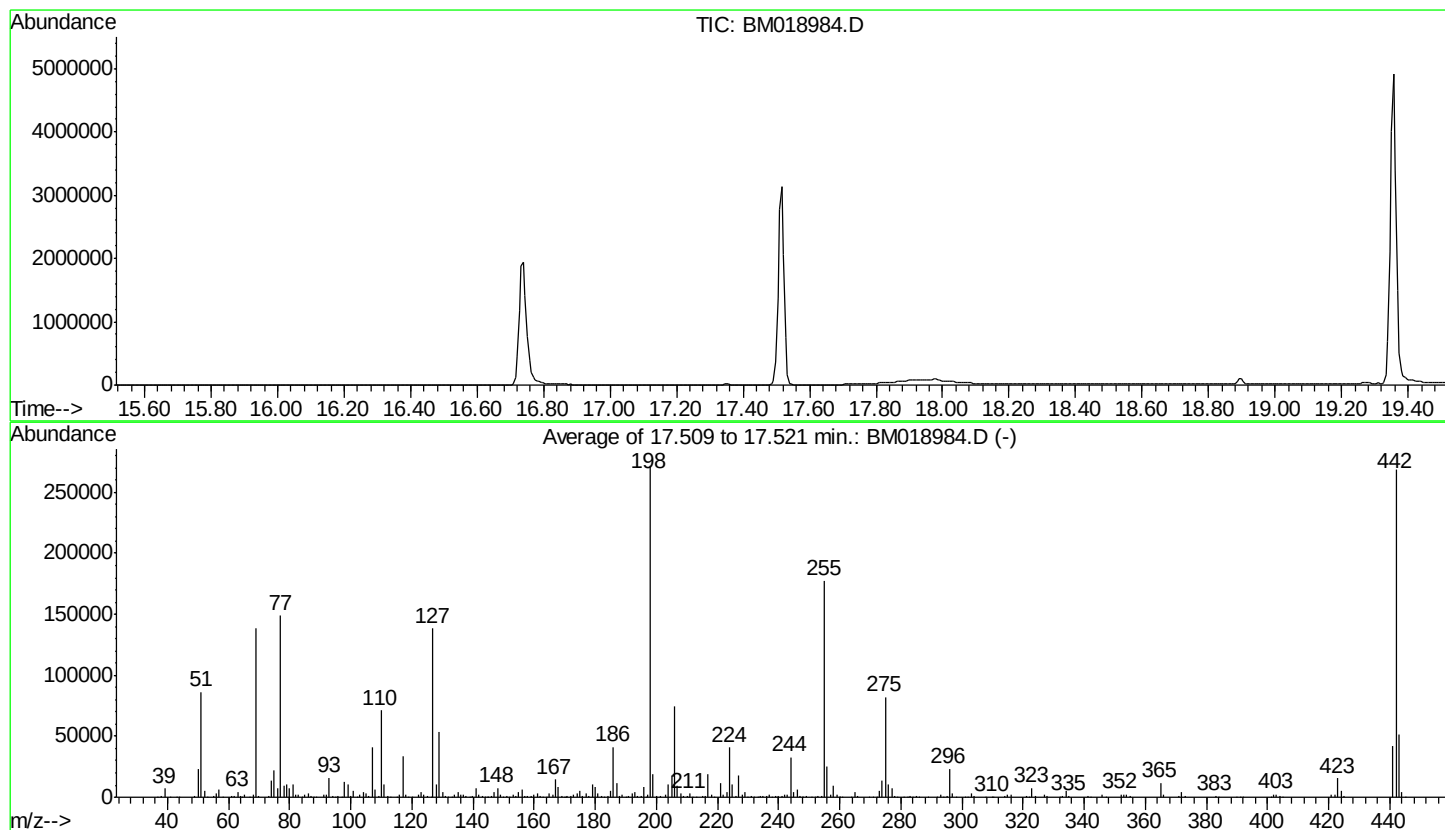

AutoFind: Scans 2452, 2453, 2454; Background Corrected with Scan 2445

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	86365	PASS
68	69	0.00	2	1.8	2449	PASS
69	198	0.00	100	51.1	139010	PASS
70	69	0.00	2	0.5	671	PASS
127	198	10	80	50.8	138058	PASS
197	198	0.00	2	0.7	2013	PASS
198	198	100	100	100.0	271850	PASS
199	198	5	9	6.8	18446	PASS
275	198	10	60	30.2	82184	PASS
365	198	1	100	4.3	11748	PASS
441	198	0.01	100	15.3	41672	PASS
442	198	50	100	98.9	268800	PASS
443	442	15	24	19.1	51474	PASS