

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030123\
 Data File : BM038826.D
 Acq On : 01 Mar 2023 14:51
 Operator : CG/JU
 Sample : PB150960BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK960

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038826.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.117	3	5	11	rVB	103214	112673	1.42%	0.162%
2	3.381	46	50	56	rBV	59196	81371	1.02%	0.117%
3	3.799	119	121	137	rBV	778086	1227156	15.45%	1.768%
4	4.146	176	180	186	rBV	18029	25396	0.32%	0.037%
5	4.375	214	219	225	rVB4	17953	27466	0.35%	0.040%
6	4.793	285	290	295	rVB4	14358	22246	0.28%	0.032%
7	7.158	684	692	704	rBV	1087486	1663343	20.94%	2.396%
8	7.334	715	722	732	rBV	920116	1433291	18.04%	2.065%
9	7.534	747	756	765	rBV	1079157	1672649	21.05%	2.409%
10	8.010	828	837	846	rBV	843986	1312588	16.52%	1.891%
11	8.710	949	956	970	rBV	1326836	2064153	25.98%	2.973%
12	9.175	1027	1035	1046	rBV	1000996	1581259	19.90%	2.278%
13	9.899	1150	1158	1174	rBV	714316	1133390	14.27%	1.633%
14	10.440	1242	1250	1262	rBV	1235541	2044535	25.74%	2.945%
15	10.828	1308	1316	1324	rVB	1230297	2008812	25.29%	2.894%
16	10.957	1331	1338	1350	rBV	1392205	2284466	28.76%	3.291%
17	12.410	1579	1585	1591	rBV2	24011	40065	0.50%	0.058%
18	14.057	1858	1865	1881	rBV	2674911	3483659	43.85%	5.018%
19	14.339	1906	1913	1923	rBV	2809003	4010252	50.48%	5.777%
20	14.645	1958	1965	1973	rBV	1973419	2744217	34.54%	3.953%
21	14.822	1988	1995	2014	rBV	1162623	1656970	20.86%	2.387%
22	15.057	2031	2035	2041	rVB7	5351	8952	0.11%	0.013%
23	15.633	2126	2133	2143	rBV	3633052	5130166	64.58%	7.390%
24	15.739	2145	2151	2161	rBV	854948	1180055	14.85%	1.700%
25	15.875	2170	2174	2182	rVB4	16174	28057	0.35%	0.040%
26	17.028	2367	2370	2373	rVB3	8198	10273	0.13%	0.015%
27	17.169	2390	2394	2402	rBV4	6395	14474	0.18%	0.021%
28	17.386	2425	2431	2440	rBV	2421732	3366187	42.37%	4.849%
29	17.486	2441	2448	2469	rVB	4147474	5623581	70.79%	8.100%
30	19.174	2731	2735	2739	rVB3	18715	25774	0.32%	0.037%
31	19.339	2759	2763	2769	rBV2	43291	59344	0.75%	0.085%
32	19.410	2771	2775	2780	rVB	43546	58298	0.73%	0.084%
33	19.774	2831	2837	2850	rBV	5371999	7036512	88.57%	10.136%
34	21.568	3136	3142	3152	rBV	2787544	3810990	47.97%	5.490%
35	23.862	3525	3532	3546	rBV2	3998554	7944248	100.00%	11.443%
36	24.021	3552	3559	3572	rVB2	2245073	4496240	56.60%	6.477%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030123\
Data File : BM038826.D
Acq On : 01 Mar 2023 14:51
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK960

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Title : SVOA CALIBRATION




Sum of corrected areas: 69423108

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030123\
Data File : BM038826.D
Acq On : 01 Mar 2023 14:51
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK960

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

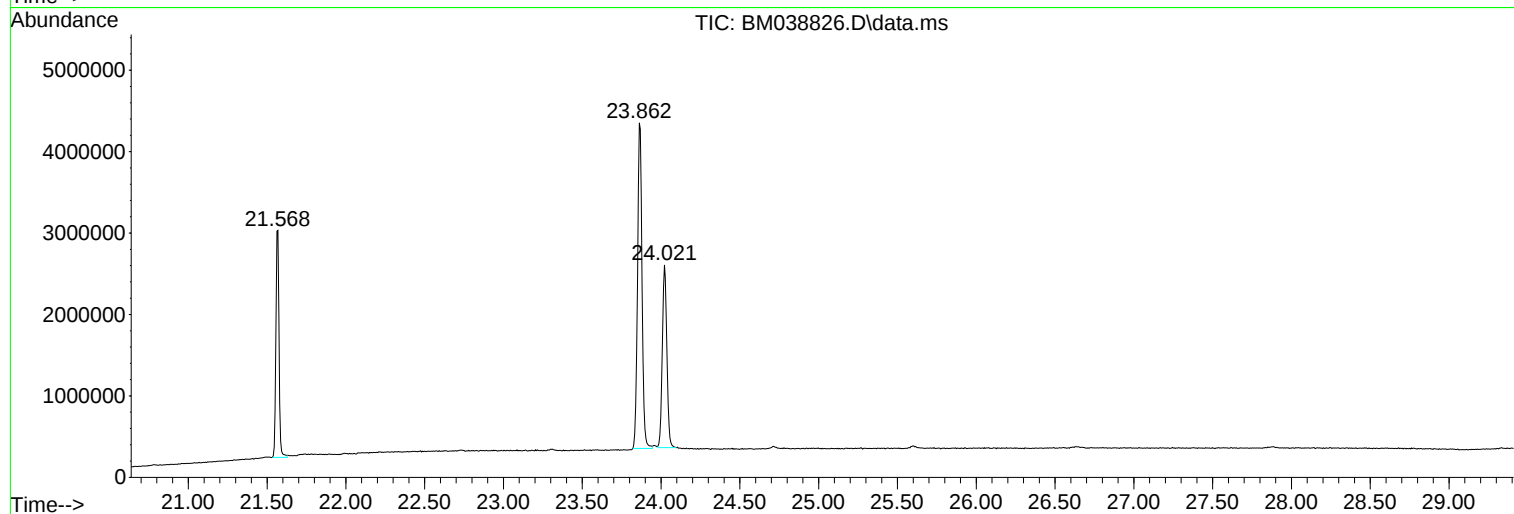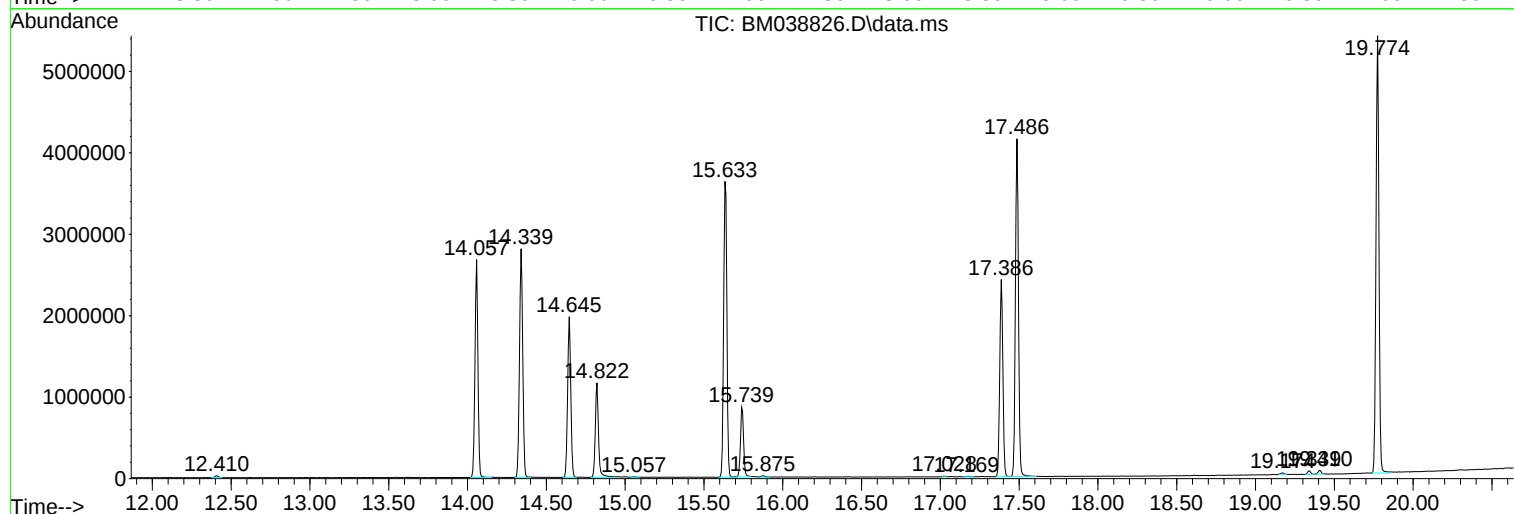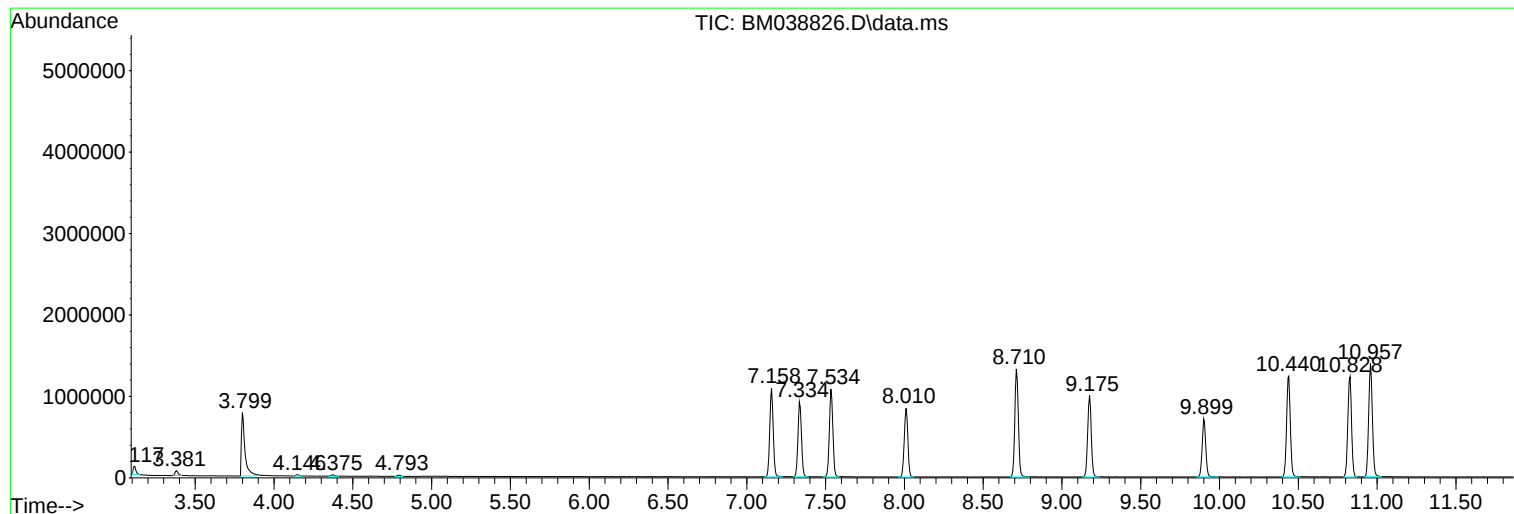

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030123\
Data File : BM038826.D
Acq On : 01 Mar 2023 14:51
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK960

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030123\
Data File : BM038826.D
Acq On : 01 Mar 2023 14:51
Operator : CG/JU
Sample : PB150960BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK960

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc