

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038840.D
 Acq On : 02 Mar 2023 17:29
 Operator : CG/JU
 Sample : 01710-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAA6

Quant Time: Mar 03 00:16:25 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	211364	20.000	ng/ul	0.00
20) Naphthalene-d8	10.827	136	930493	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	563762	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1252123	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	1243810	20.000	ng/ul	0.00
88) Perylene-d12	24.021	264	1507757	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	15137	2.674	ng/uL	0.00
4) Pyridine-d5	3.804	84	644	0.041	ng/ul	0.00
7) Phenol-d5	7.157	99	248616	12.546	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	168897	13.340	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	195903	13.267	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	181368	11.618	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	82245	12.590	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	75386	12.316	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.439	165	176199	12.388	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	193854	8.177	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	608924	13.945	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	676654	13.259	ng/ul	0.00
54) 4-Nitrophenol-d4	14.821	143	56214	6.431	ng/ul	0.00
60) Fluorene-d10	15.633	176	550434	14.293	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	42252	6.491	ng/ul	0.00
73) Anthracene-d10	17.486	188	858730	13.908	ng/ul	0.00
81) Pyrene-d10	19.774	212	1091466	15.955	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.862	264	1104215	14.533	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.181	94	25575	1.206	ng/ul	98
16) Acetophenone	8.833	105	69818	2.573	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038840.D
Acq On : 02 Mar 2023 17:29
Operator : CG/JU
Sample : 01710-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAA6

Quant Time: Mar 03 00:16:25 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration




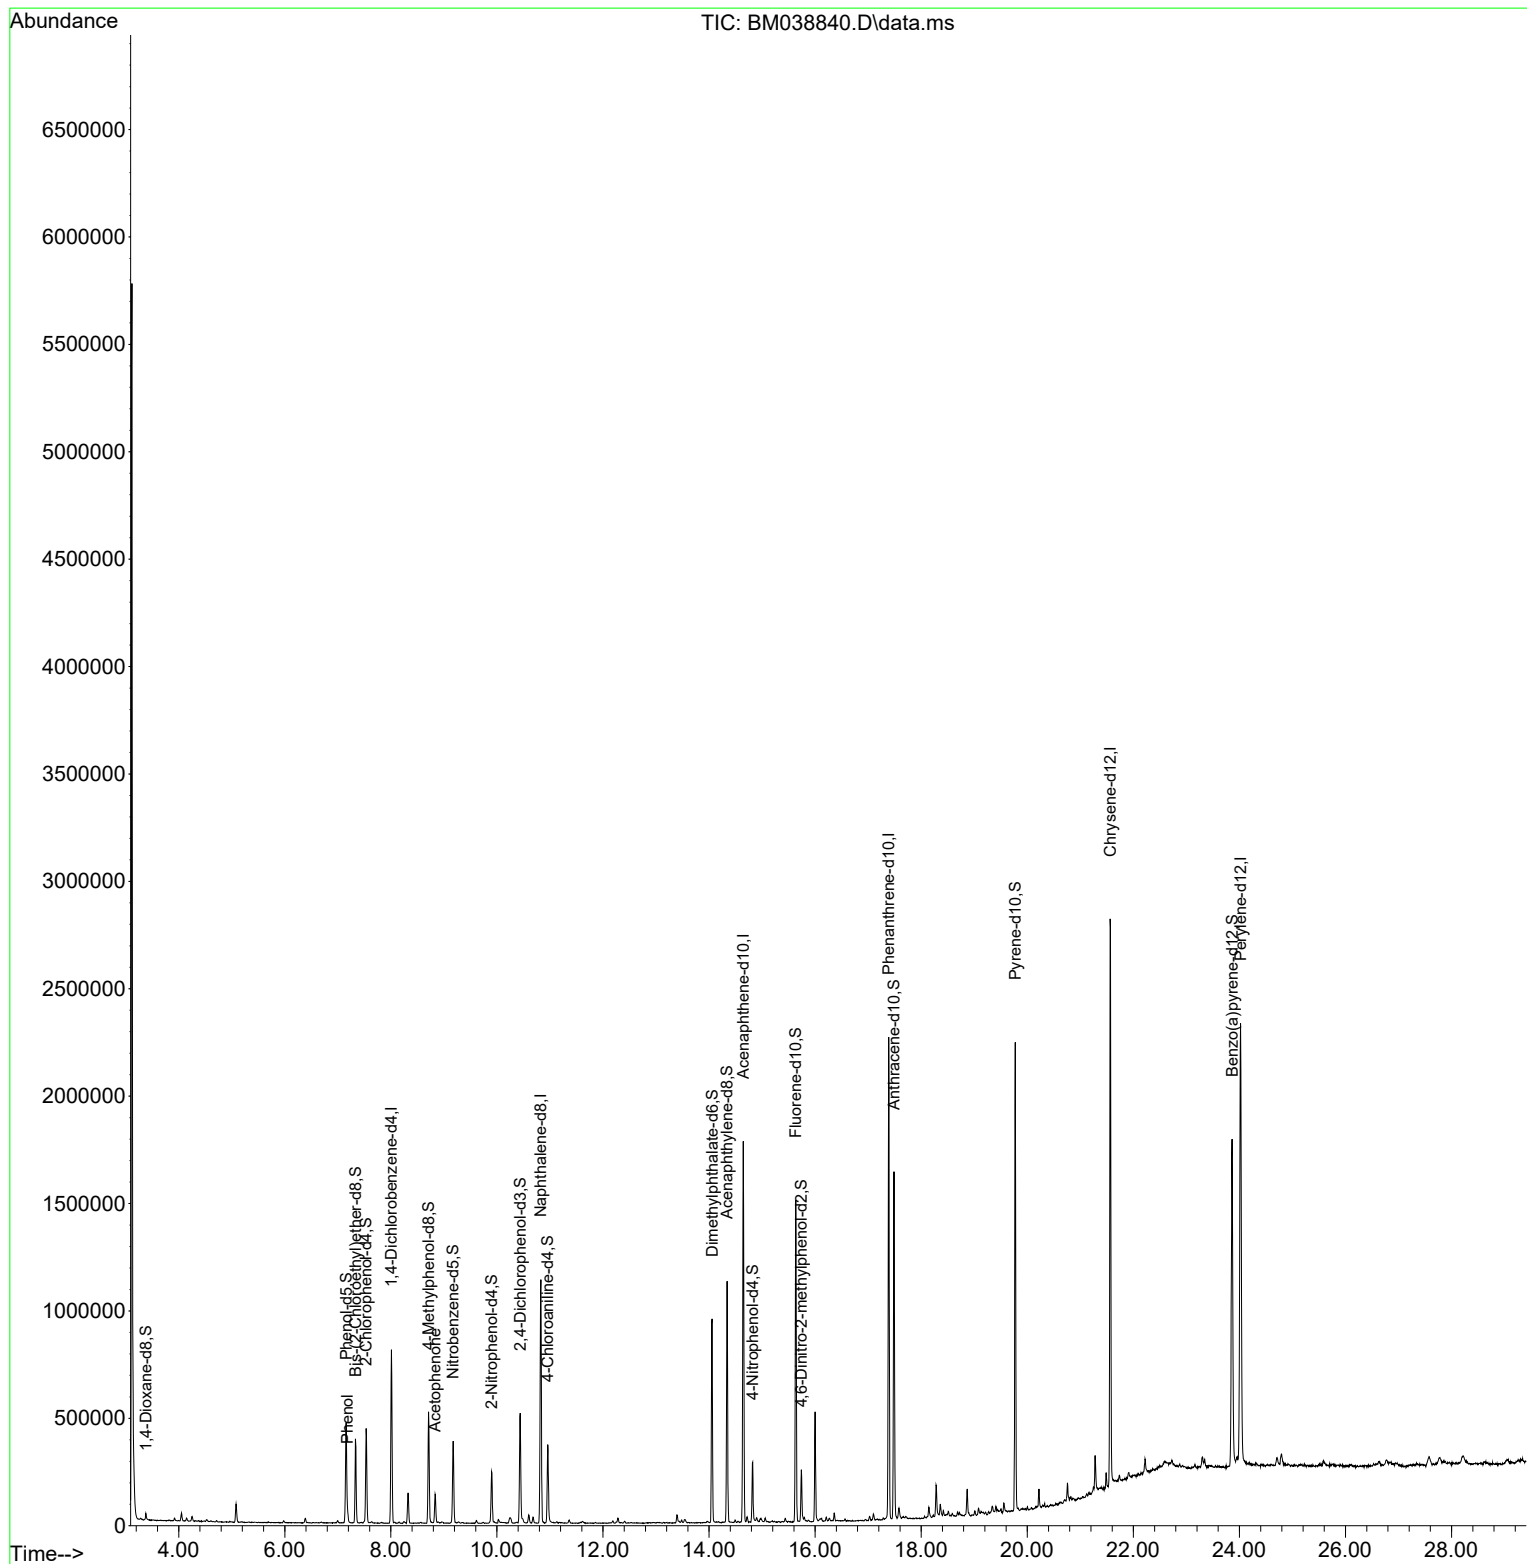


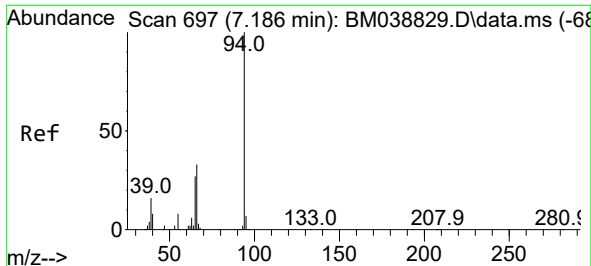

#8
Phenol
Concen: 1.206 ng/ul
RT: 7.181 min Scan# 697
Delta R.T. -0.006 min
Lab File: BM038840.D
Acq: 02 Mar 2023 17:29

Instrument :
BNA_M
ClientSampleId :
DBAA6

Tgt Ion: 94 Resp: 25575
Ion Ratio Lower Upper
94 100
65 29.6 22.1 33.1
66 35.8 28.6 43.0

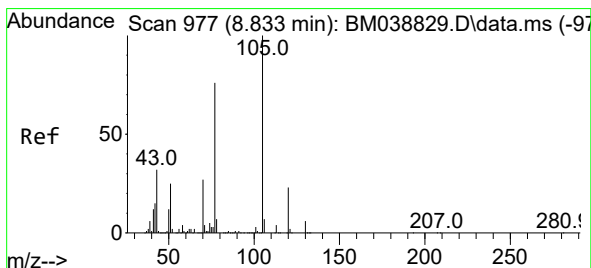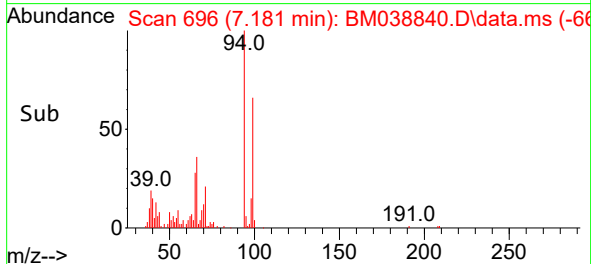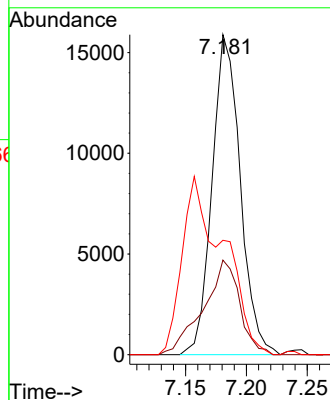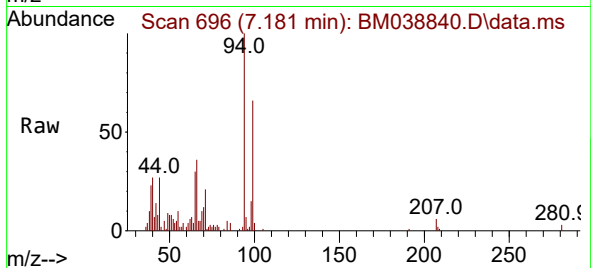

#16
Acetophenone
Concen: 2.573 ng/ul
RT: 8.833 min Scan# 977
Delta R.T. -0.006 min
Lab File: BM038840.D
Acq: 02 Mar 2023 17:29

Tgt Ion: 105 Resp: 69818
Ion Ratio Lower Upper
105 100
77 74.6 62.6 93.8
51 27.6 20.8 31.2

