

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038841.D
 Acq On : 02 Mar 2023 18:06
 Operator : CG/JU
 Sample : 01710-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAA7

Quant Time: Mar 03 00:16:34 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	227788	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	1000155	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	621190	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1393004	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	1405198	20.000	ng/ul	0.00
88) Perylene-d12	24.021	264	1714779	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	16105	2.640	ng/uL	0.00
4) Pyridine-d5	3.805	84	431	0.026	ng/ul	0.00
7) Phenol-d5	7.157	99	277277	12.984	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	181847	13.327	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	217216	13.650	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	213729	12.704	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	90594	12.903	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	85657	13.019	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.439	165	203873	13.335	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	222921	8.748	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	693826	14.421	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	765342	13.610	ng/ul	0.00
54) 4-Nitrophenol-d4	14.821	143	81611	8.473	ng/ul	0.00
60) Fluorene-d10	15.633	176	617737	14.558	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	53844	7.435	ng/ul	0.00
73) Anthracene-d10	17.486	188	984574	14.334	ng/ul	0.00
81) Pyrene-d10	19.774	212	1247248	16.138	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.856	264	1301694	15.063	ng/ul	-0.01
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.451	93	25147	1.382	ng/ul#	24
13) 2-Methylphenol	8.322	108	62756	3.673	ng/ul#	16
16) Acetophenone	8.834	105	46479	1.590	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038841.D
Acq On : 02 Mar 2023 18:06
Operator : CG/JU
Sample : 01710-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAA7

Quant Time: Mar 03 00:16:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration




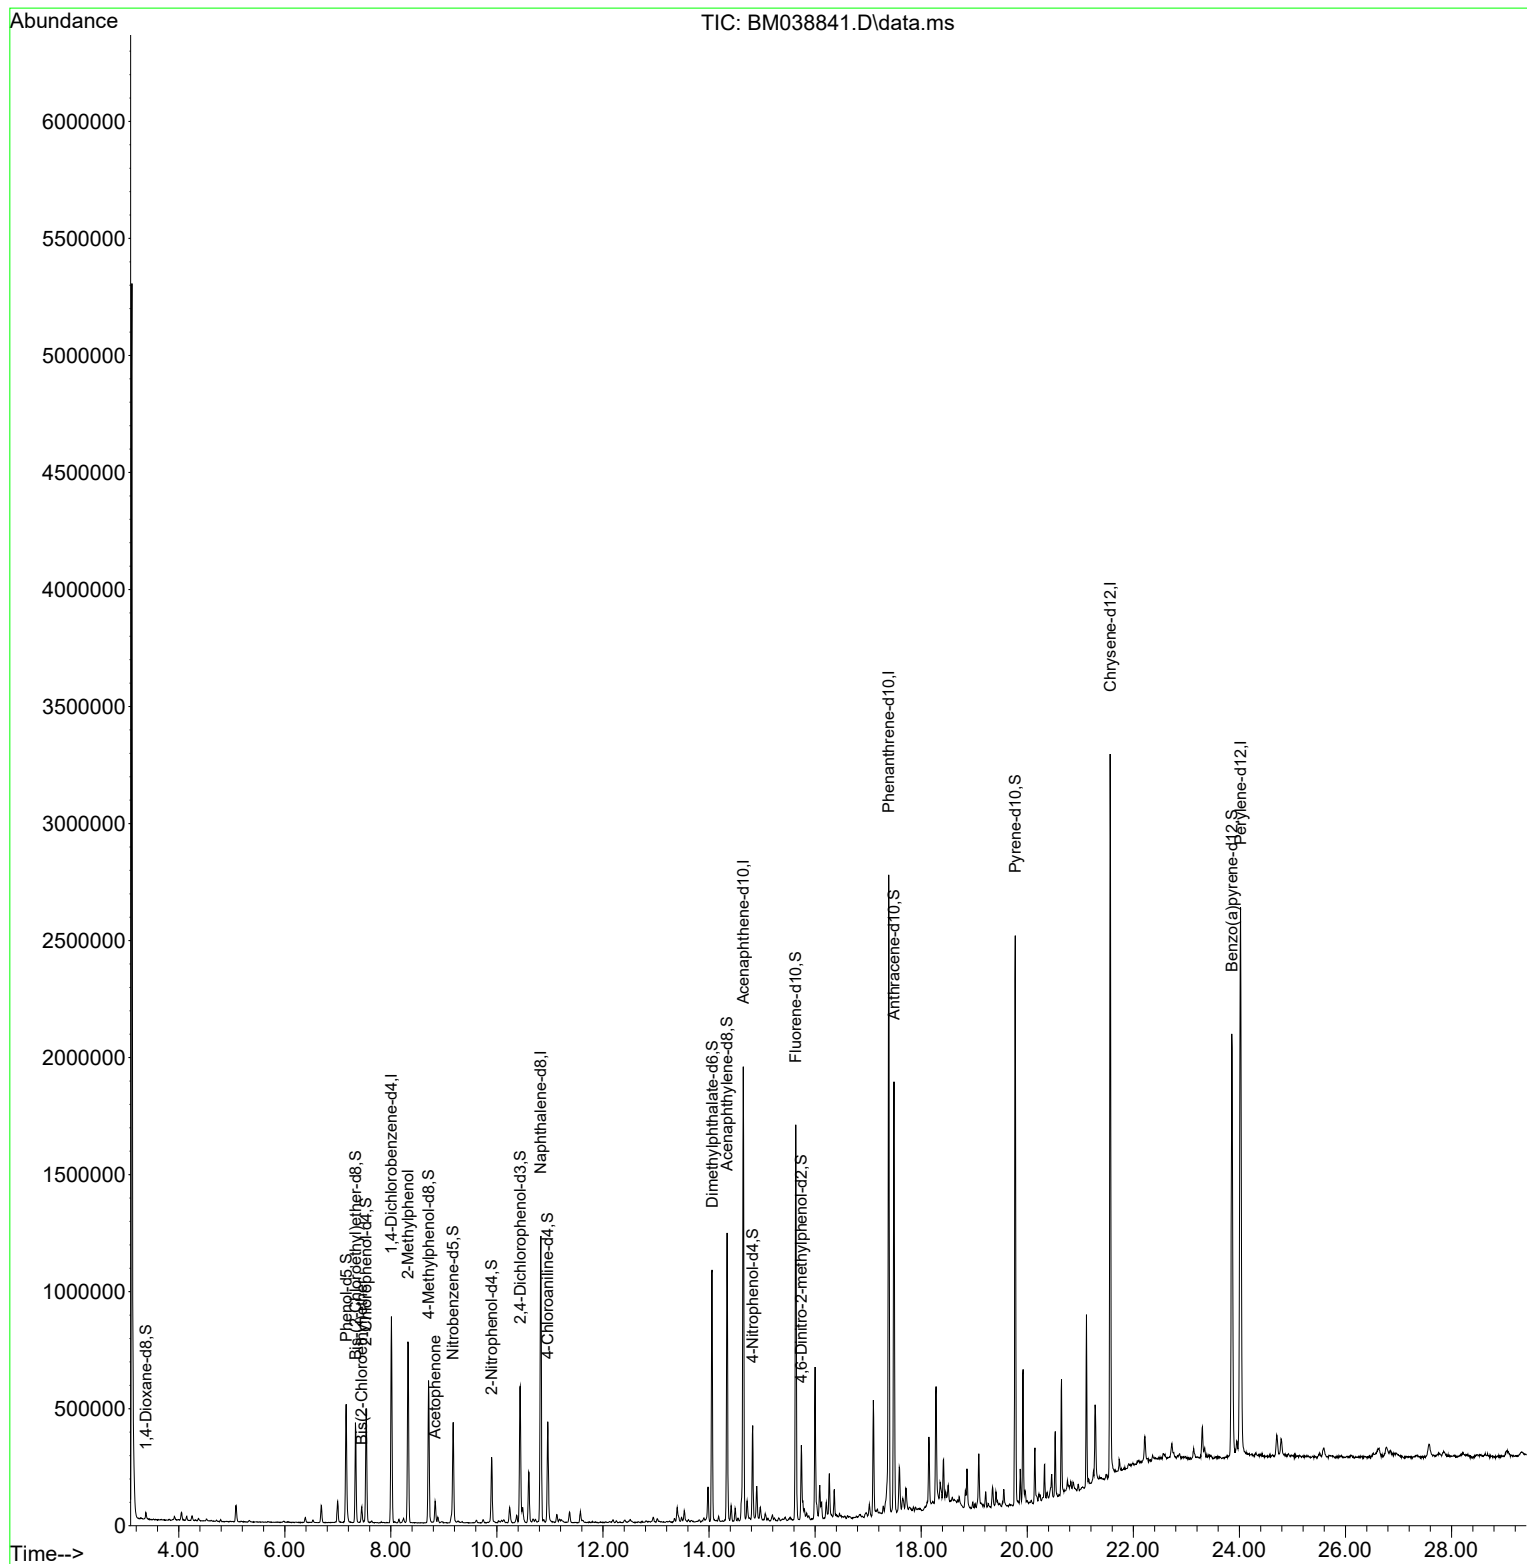


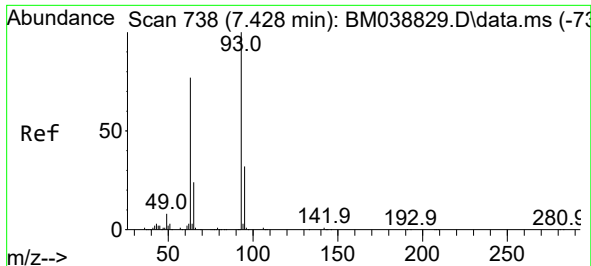

#10
Bis(2-Chloroethyl)ether
Concen: 1.382 ng/ul
RT: 7.451 min Scan# 742
Delta R.T. 0.017 min
Lab File: BM038841.D
Acq: 02 Mar 2023 18:06




Instrument :
BNA_M
ClientSampleId :
DBAA7


Tgt Ion: 93 Resp: 25147
Ion Ratio Lower Upper
93 100
63 2.3 60.3 90.5#
95 1.3 25.8 38.6#

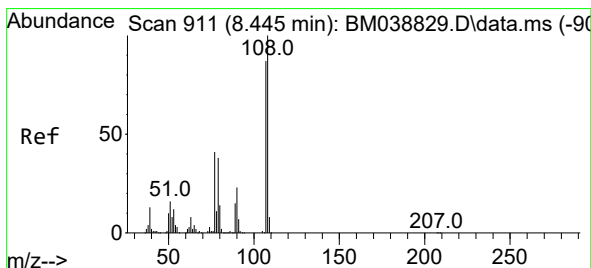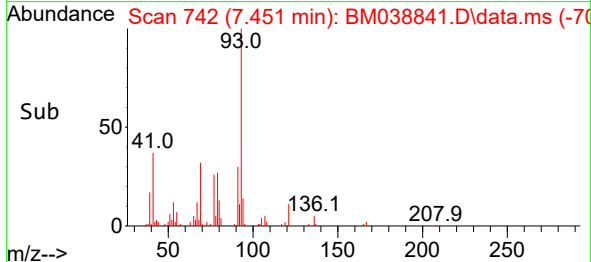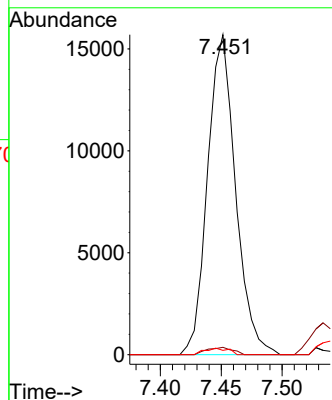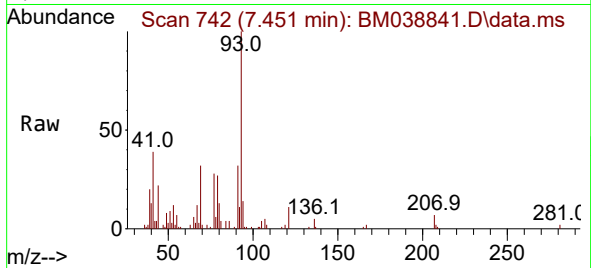

#13
2-Methylphenol
Concen: 3.673 ng/ul
RT: 8.322 min Scan# 890
Delta R.T. -0.130 min
Lab File: BM038841.D
Acq: 02 Mar 2023 18:06


Tgt Ion: 108 Resp: 62756
Ion Ratio Lower Upper
108 100
107 9.2 69.0 103.6#

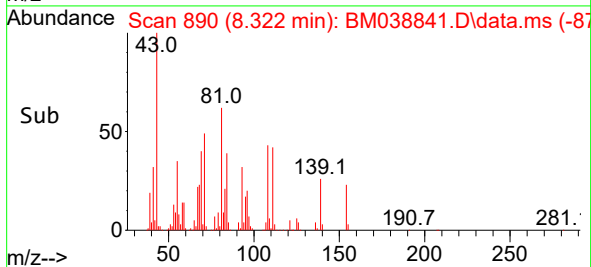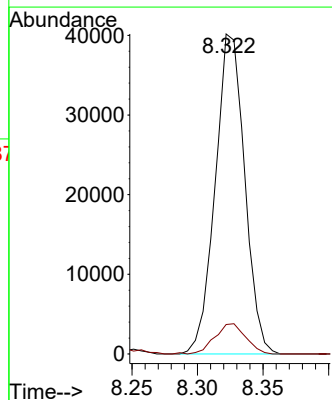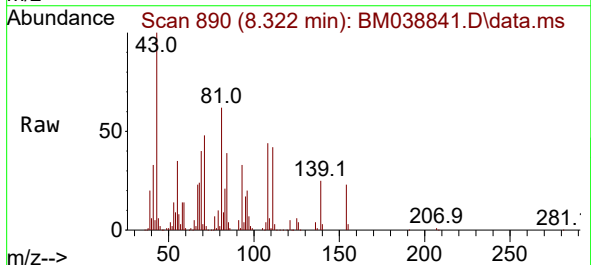

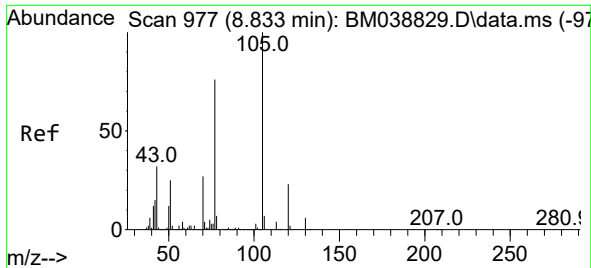

#16
Acetophenone
Concen: 1.590 ng/ul
RT: 8.834 min Scan# 91
Delta R.T. -0.006 min
Lab File: BM038841.D
Acq: 02 Mar 2023 18:06

Instrument :
BNA_M
ClientSampleId :
DBAA7

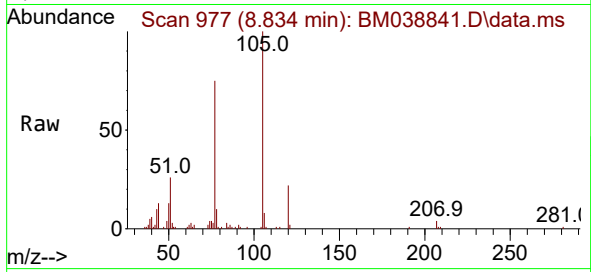

Tgt Ion:105 Resp: 46479
Ion Ratio Lower Upper
105 100
77 74.7 62.6 93.8
51 26.0 20.8 31.2

