

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038842.D
 Acq On : 02 Mar 2023 18:44
 Operator : CG/JU
 Sample : 01710-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAA9

Quant Time: Mar 03 00:16:44 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	263172	20.000	ng/ul	0.00
20) Naphthalene-d8	10.828	136	1144378	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	706478	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1538341	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	1522661	20.000	ng/ul	0.00
88) Perylene-d12	24.015	264	1846805	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	16230	2.303	ng/uL	0.00
4) Pyridine-d5	3.816	84	581	0.030	ng/ul	0.01
7) Phenol-d5	7.157	99	288158	11.679	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	191378	12.140	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	225615	12.272	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	219178	11.276	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	98703	12.286	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	93047	12.360	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.439	165	206960	11.831	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	173933	5.965	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	674935	12.335	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	767628	12.003	ng/ul	0.00
54) 4-Nitrophenol-d4	14.821	143	75899	6.929	ng/ul	0.00
60) Fluorene-d10	15.633	176	601560	12.465	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	50893	6.364	ng/ul	0.00
73) Anthracene-d10	17.486	188	908442	11.976	ng/ul	0.00
81) Pyrene-d10	19.774	212	1140082	13.613	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.856	264	1182125	12.702	ng/ul	-0.01
Target Compounds						
					Qvalue	
16) Acetophenone	8.834	105	38174	1.130	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038842.D
Acq On : 02 Mar 2023 18:44
Operator : CG/JU
Sample : 01710-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAA9


Quant Time: Mar 03 00:16:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration

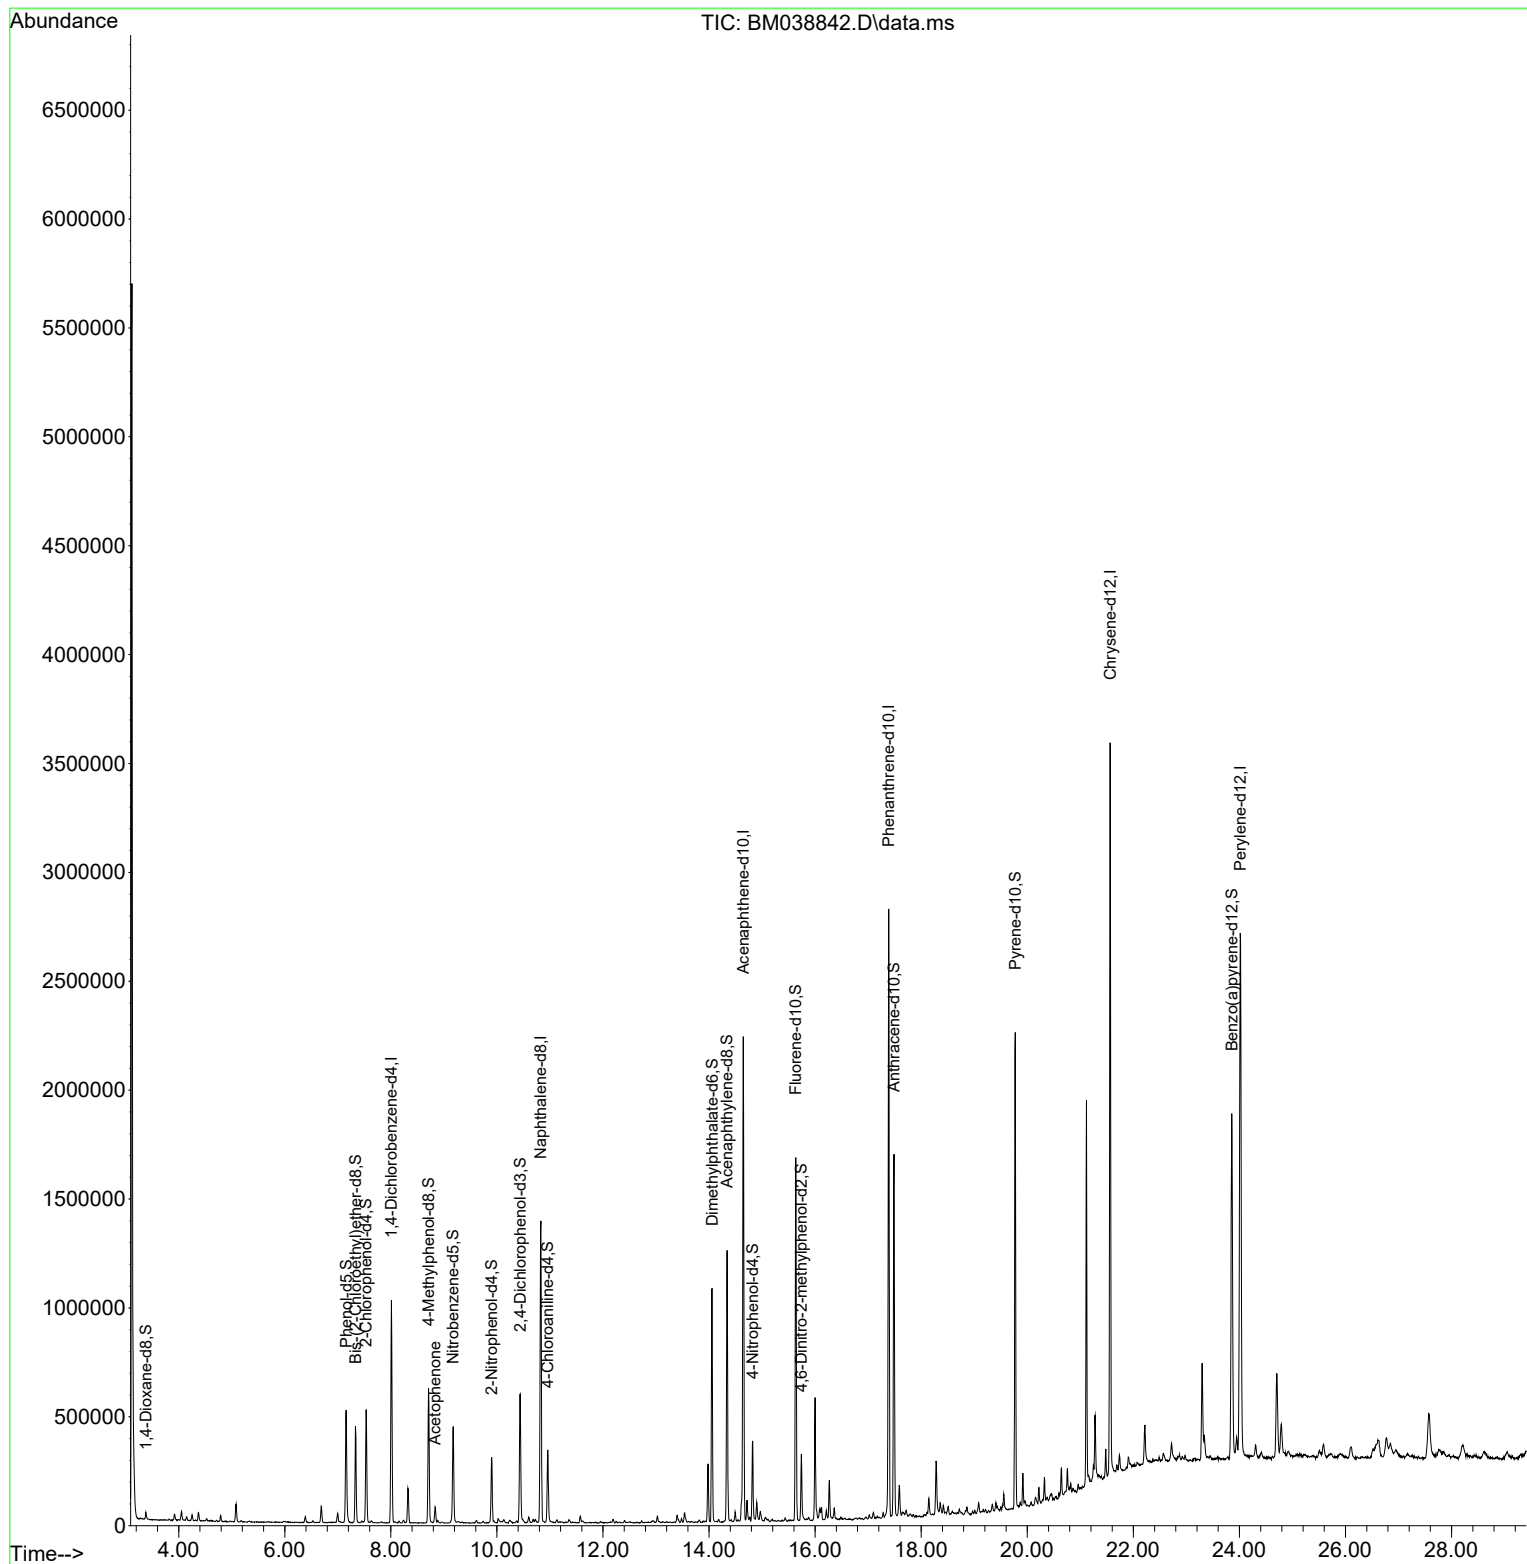

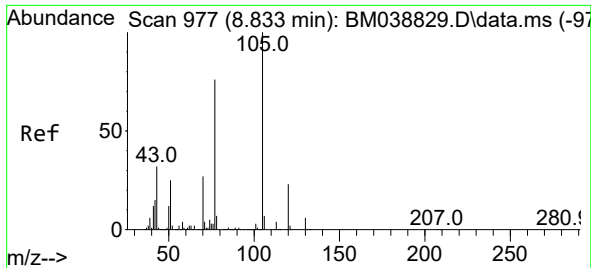

#16
 Acetophenone
 Concen: 1.130 ng/ul
 RT: 8.834 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BM038842.D
 Acq: 02 Mar 2023 18:44

Instrument :
 BNA_M
 ClientSampleId :
 DBAA9

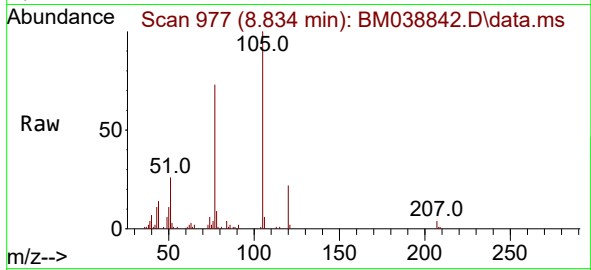

Tgt Ion:	105	Resp:	38174
Ion	Ratio	Lower	Upper
105	100		
77	73.5	62.6	93.8
51	25.7	20.8	31.2

