

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038843.D
 Acq On : 02 Mar 2023 19:21
 Operator : CG/JU
 Sample : 01710-14
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAB1

Quant Time: Mar 03 00:16:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	247860	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1085967	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	674222	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1486668	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	1480606	20.000	ng/ul	0.00
88) Perylene-d12	24.015	264	1805195	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	18452	2.780	ng/uL	0.00
4) Pyridine-d5	3.810	84	366	0.020	ng/ul	0.00
7) Phenol-d5	7.157	99	319143	13.734	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.333	67	218957	14.747	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	263372	15.210	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	251084	13.716	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	120779	15.842	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	112395	15.733	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.439	165	246045	14.822	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	235379	8.507	ng/ul	0.00
46) Dimethylphthalate-d6	14.057	166	829269	15.880	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	944239	15.470	ng/ul	0.00
54) 4-Nitrophenol-d4	14.821	143	77315	7.396	ng/ul	0.00
60) Fluorene-d10	15.633	176	735388	15.967	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	70645	9.140	ng/ul	0.00
73) Anthracene-d10	17.486	188	1145261	15.623	ng/ul	0.00
81) Pyrene-d10	19.768	212	1436632	17.642	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.850	264	1497280	16.459	ng/ul	-0.02
Target Compounds						
					Qvalue	
16) Acetophenone	8.833	105	51290	1.612	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038843.D
Acq On : 02 Mar 2023 19:21
Operator : CG/JU
Sample : 01710-14
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAB1

Quant Time: Mar 03 00:16:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration

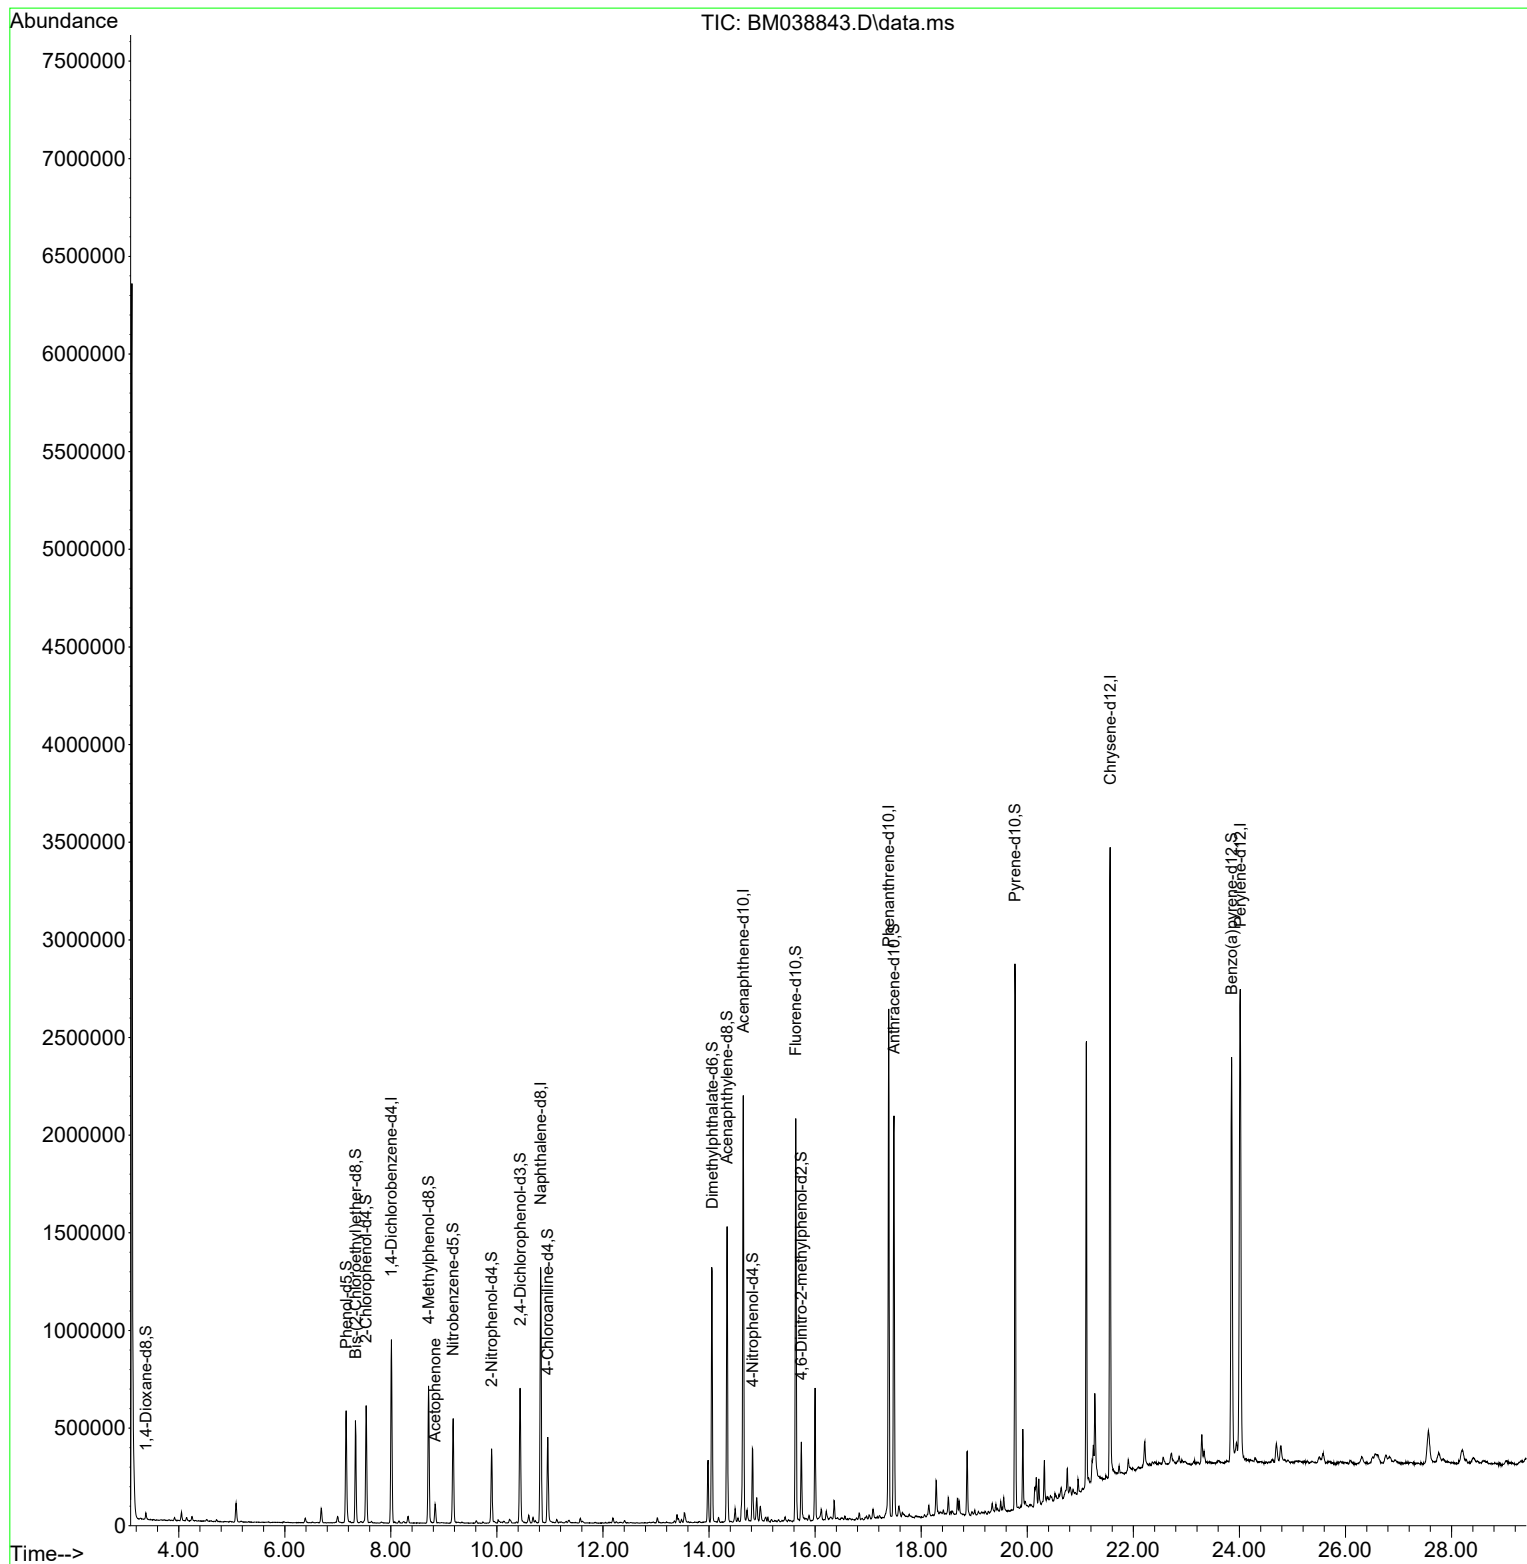

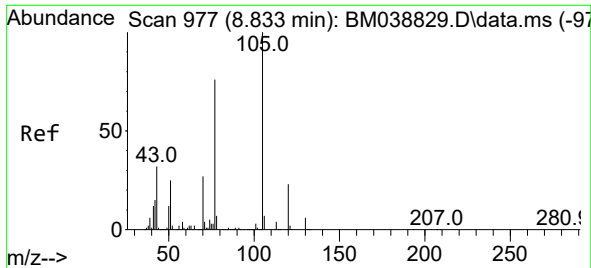

#16
 Acetophenone
 Concen: 1.612 ng/ul
 RT: 8.833 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BM038843.D
 Acq: 02 Mar 2023 19:21

Instrument :
 BNA_M
 ClientSampleId :
 DBAB1

Tgt Ion:105 Resp: 51290
 Ion Ratio Lower Upper
 105 100
 77 75.1 62.6 93.8
 51 25.3 20.8 31.2

