

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038844.D
 Acq On : 02 Mar 2023 19:59
 Operator : CG/JU
 Sample : 01710-17
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAB4

Quant Time: Mar 03 00:17:02 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	218643	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	970433	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	613447	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1342012	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	1328436	20.000	ng/ul	0.00
88) Perylene-d12	24.015	264	1619562	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	16731	2.857	ng/uL	0.00
4) Pyridine-d5	3.805	84	234	0.015	ng/ul	0.00
7) Phenol-d5	7.157	99	324817	15.846	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	212251	16.206	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	257791	16.877	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	237014	14.677	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	116538	17.106	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	114838	17.989	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	235402	15.869	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	316108	12.785	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	818550	17.228	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	911954	16.422	ng/ul	0.00
54) 4-Nitrophenol-d4	14.816	143	104389	10.975	ng/ul	0.00
60) Fluorene-d10	15.633	176	721913	17.228	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	64041	9.179	ng/ul	0.00
73) Anthracene-d10	17.480	188	1112941	16.818	ng/ul	-0.01
81) Pyrene-d10	19.768	212	1425273	19.507	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.856	264	1494916	18.316	ng/ul	-0.01
Target Compounds						
16) Acetophenone	8.834	105	33278	1.186	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038844.D
Acq On : 02 Mar 2023 19:59
Operator : CG/JU
Sample : 01710-17
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAB4

Quant Time: Mar 03 00:17:02 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration

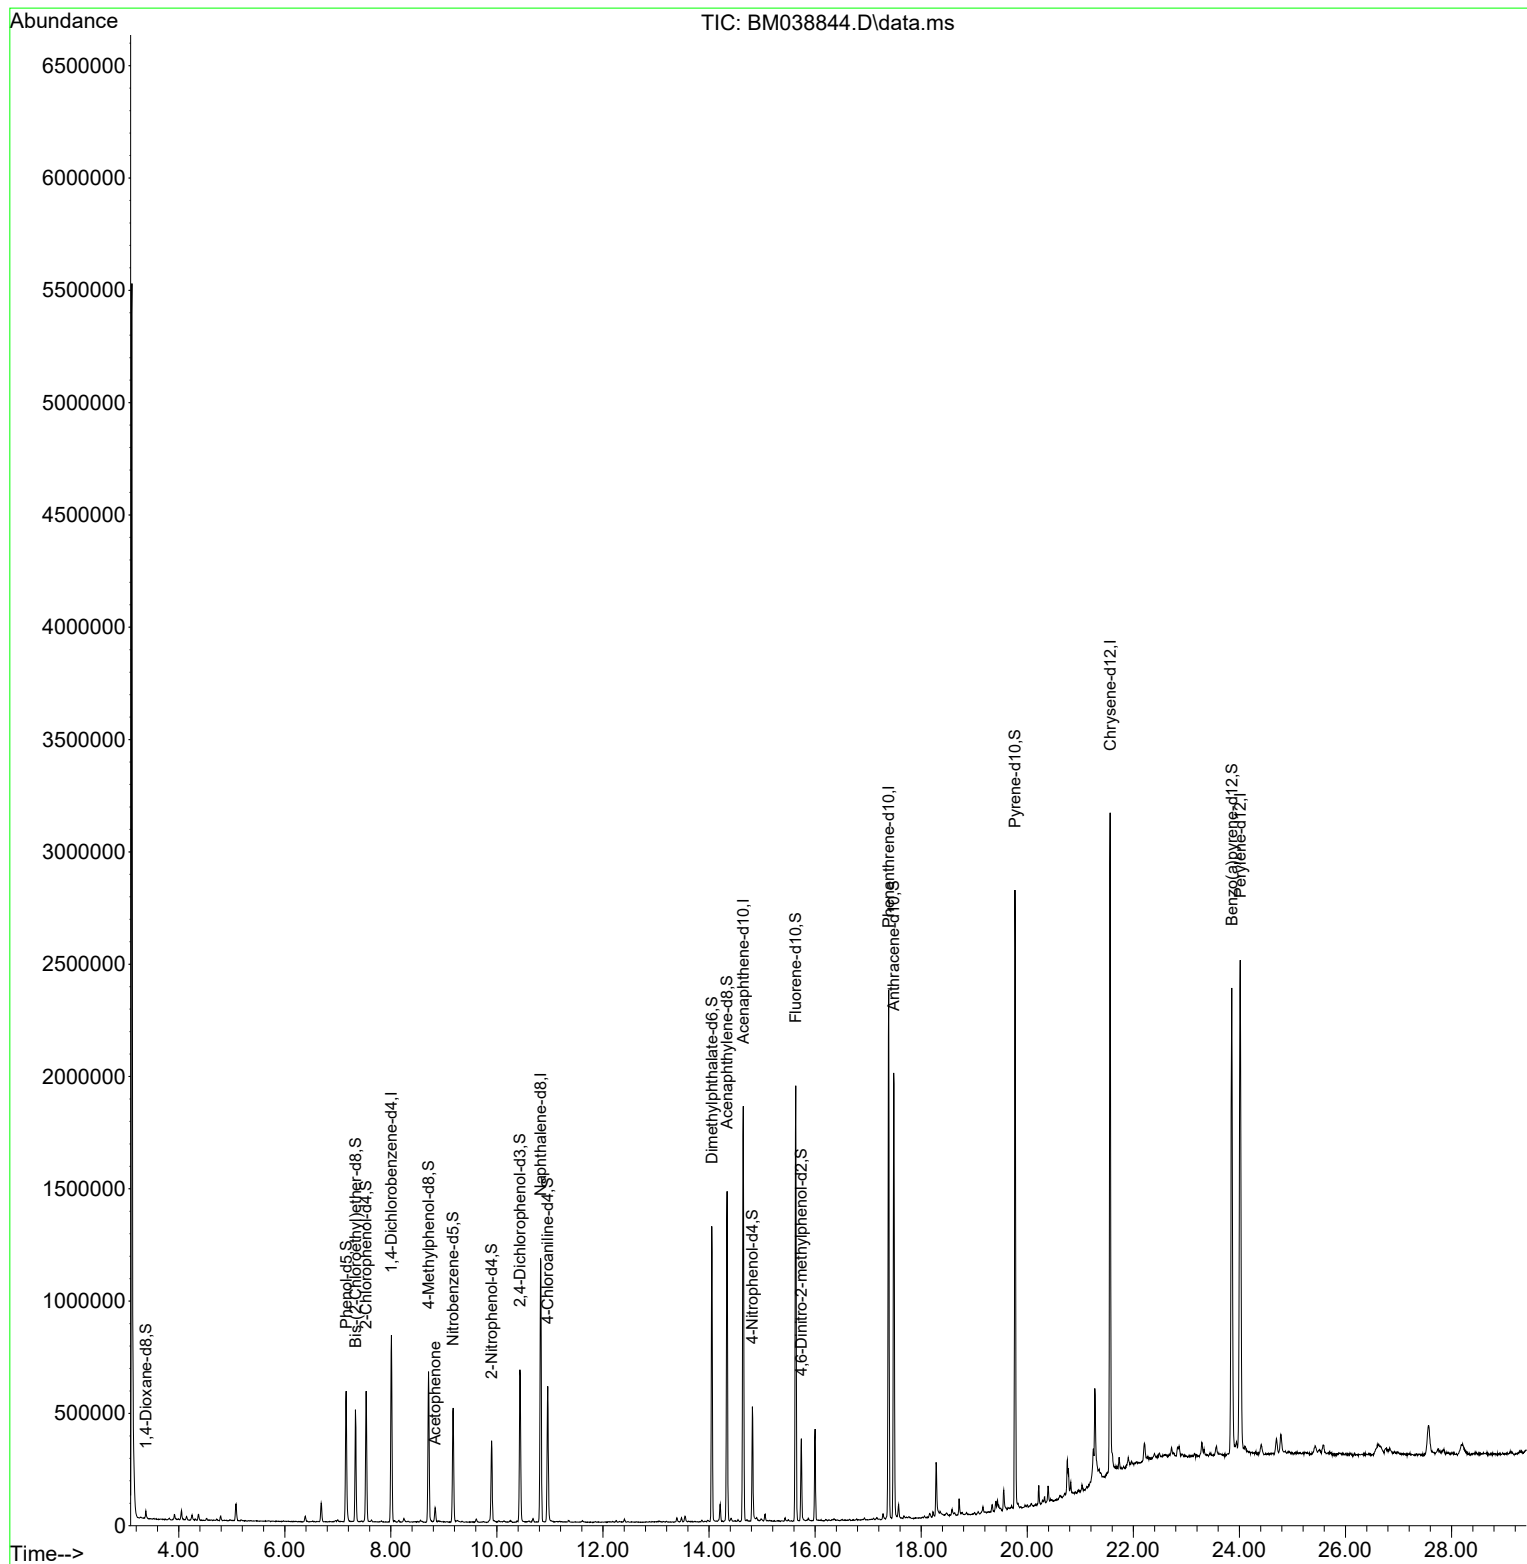

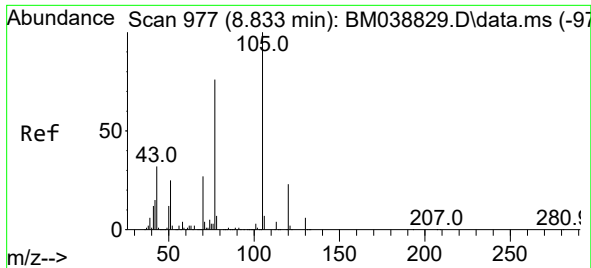

#16
 Acetophenone
 Concen: 1.186 ng/ul
 RT: 8.834 min Scan# 91
 Delta R.T. -0.006 min
 Lab File: BM038844.D
 Acq: 02 Mar 2023 19:59

Instrument :
 BNA_M
 ClientSampleId :
 DBAB4

Tgt Ion:	105	Resp:	33278
Ion	Ratio	Lower	Upper
105	100		
77	79.0	62.6	93.8
51	28.8	20.8	31.2

