




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038846.D
Acq On : 02 Mar 2023 21:13
Operator : CG/JU
Sample : 01710-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAB6

Manual IntegrationsAPPROVED

Quant Time: Mar 03 00:17:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/03/2023
Supervised By :Jagrut Upadhyay 03/03/2023

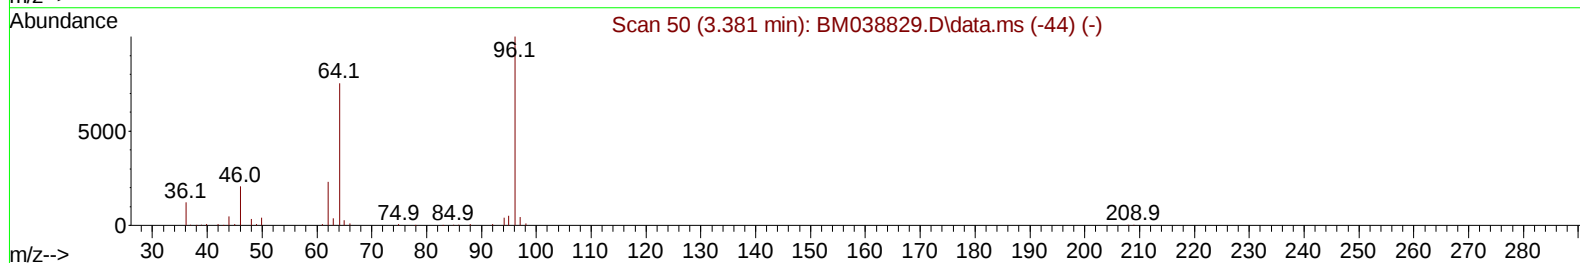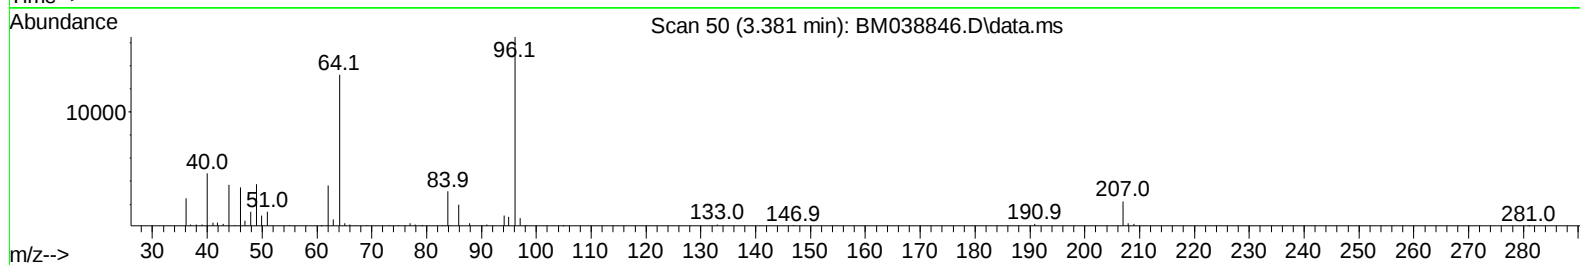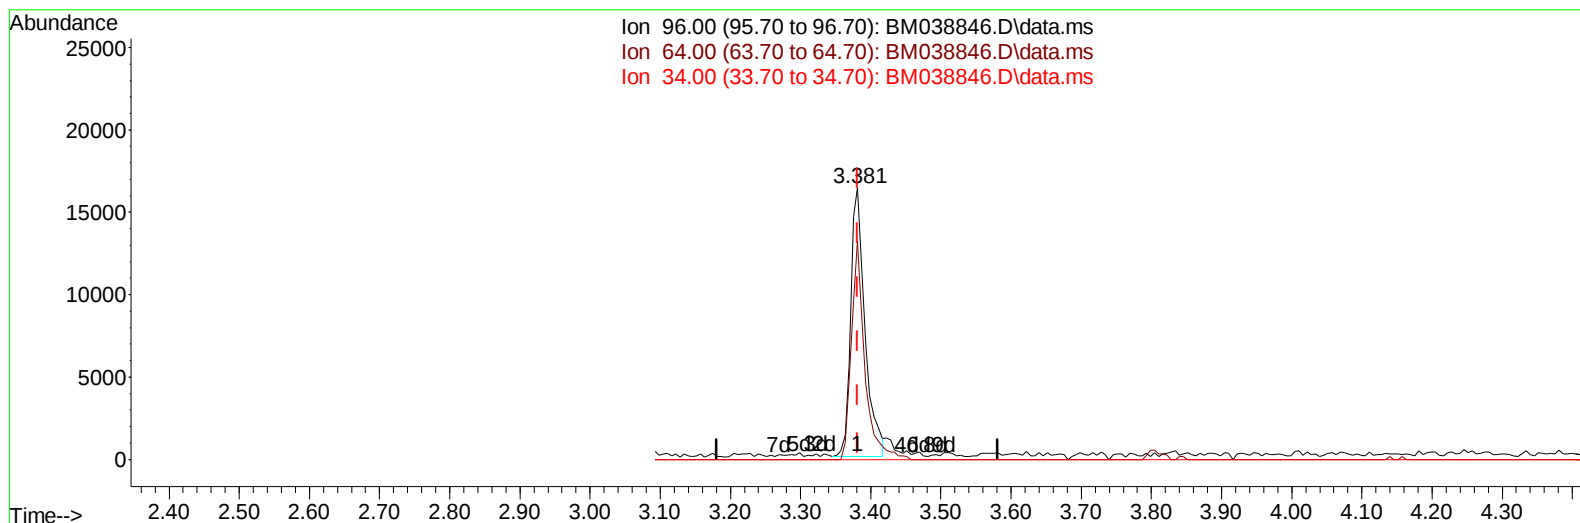

TIC: BM038846.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (+ 0.000) 3.68 ng/uL

response 23178

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.20	80.36
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038846.D
 Acq On : 02 Mar 2023 21:13
 Operator : CG/JU
 Sample : 01710-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAB6

Manual IntegrationsAPPROVED

Quant Time: Mar 03 00:17:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/03/2023
 Supervised By :Jagrut Upadhyay 03/03/2023

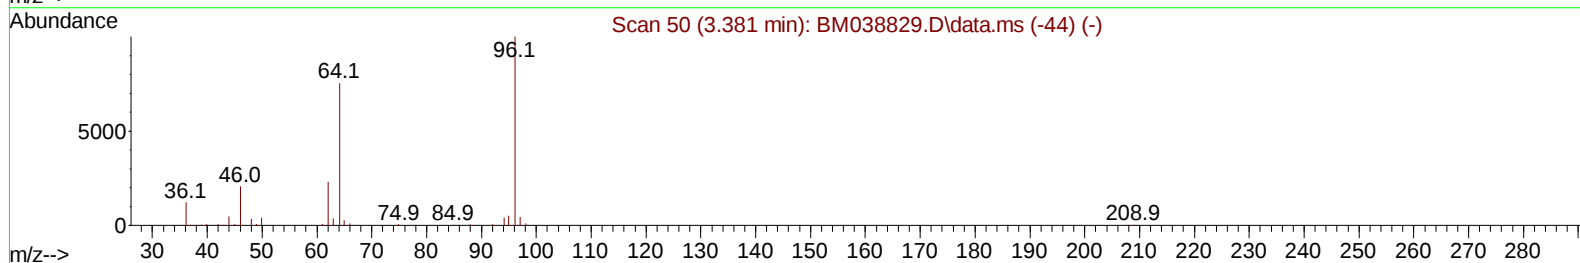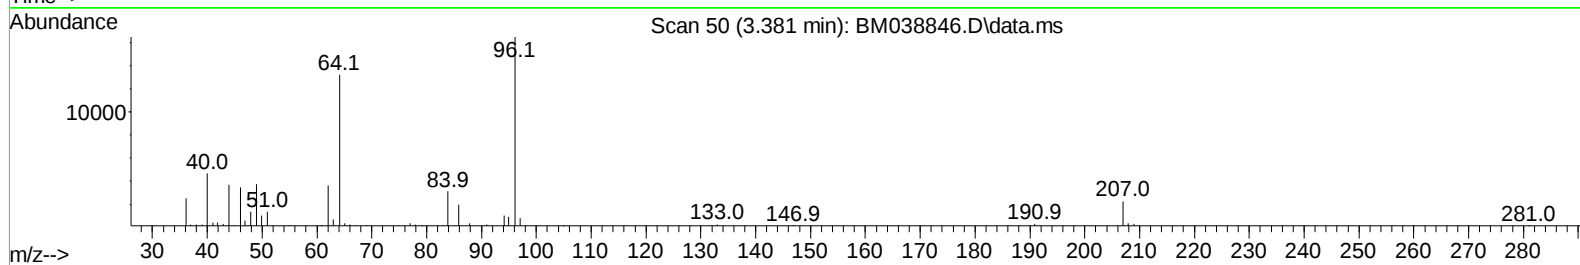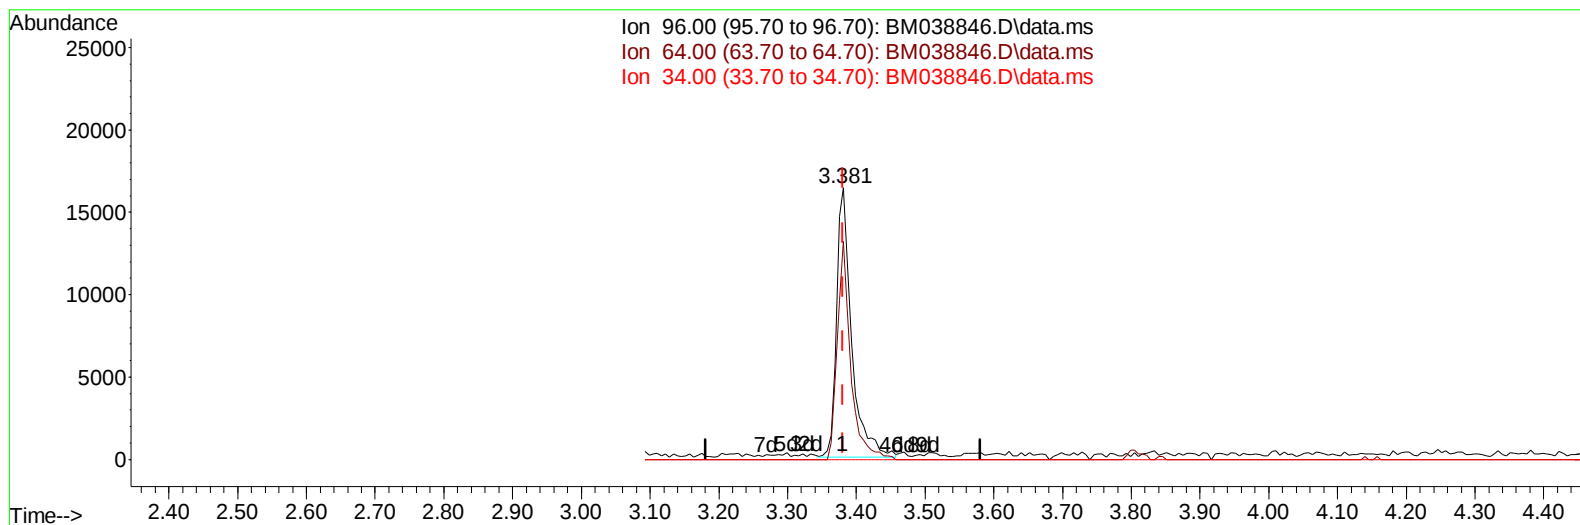

TIC: BM038846.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.381min (+ 0.000) 3.92 ng/uL m

response 24704

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	76.20	80.36
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038846.D
 Acq On : 02 Mar 2023 21:13
 Operator : CG/JU
 Sample : 01710-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBAB6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/03/2023
 Supervised By :Jagrut Upadhyay 03/03/2023

Quant Time: Mar 03 00:17:19 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 01 02:09:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.010	152	235203	20.000	ng/ul	0.00
20) Naphthalene-d8	10.822	136	1034638	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.645	164	640733	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.386	188	1398015	20.000	ng/ul	0.00
79) Chrysene-d12	21.562	240	1348538	20.000	ng/ul	0.00
88) Perylene-d12	24.015	264	1658579	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.381	96	24704m	3.922	ng/uL	0.00
4) Pyridine-d5	3.799	84	324192	18.719	ng/ul	0.00
7) Phenol-d5	7.157	99	439679	19.939	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.334	67	289426	20.542	ng/ul	0.00
11) 2-Chlorophenol-d4	7.534	132	347986	21.178	ng/ul	0.00
15) 4-Methylphenol-d8	8.710	113	345722	19.901	ng/ul	0.00
21) Nitrobenzene-d5	9.175	128	161147	22.186	ng/ul	0.00
24) 2-Nitrophenol-d4	9.898	143	154704	22.730	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.434	165	322241	20.375	ng/ul	0.00
31) 4-Chloroaniline-d4	10.957	131	534558	20.278	ng/ul	0.00
46) Dimethylphthalate-d6	14.051	166	1174167	23.660	ng/ul	0.00
49) Acenaphthylene-d8	14.339	160	1311871	22.617	ng/ul	0.00
54) 4-Nitrophenol-d4	14.821	143	167504	16.861	ng/ul	0.00
60) Fluorene-d10	15.633	176	1039254	23.745	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.739	200	96800	13.319	ng/ul	0.00
73) Anthracene-d10	17.480	188	1654144	23.995	ng/ul	-0.01
81) Pyrene-d10	19.768	212	1979345	26.686	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.856	264	2087487	24.975	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038846.D
Acq On : 02 Mar 2023 21:13
Operator : CG/JU
Sample : 01710-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBAB6

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/03/2023
Supervised By :Jagrut Upadhyay 03/03/2023

Quant Time: Mar 03 00:17:19 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 01 02:09:21 2023
Response via : Initial Calibration

