

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
 Data File : BM038835.D
 Acq On : 02 Mar 2023 14:21
 Operator : CG/JU
 Sample : PB150981BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK981

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038835.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.116	3	5	12	rVB	75205	83581	1.25%	0.139%
2	3.381	45	50	60	rVB2	60689	89522	1.34%	0.149%
3	3.799	119	121	156	rBV	722014	1201817	18.00%	1.997%
4	4.146	176	180	185	rVB2	13739	19710	0.30%	0.033%
5	4.375	215	219	223	rVB5	7617	10111	0.15%	0.017%
6	7.157	685	692	702	rBV	992134	1491871	22.35%	2.479%
7	7.334	716	722	730	rBV	841824	1277334	19.13%	2.122%
8	7.534	749	756	766	rBV	953655	1493176	22.37%	2.481%
9	8.010	830	837	844	rBV	784910	1205438	18.06%	2.003%
10	8.710	949	956	969	rBV	1182096	1856368	27.81%	3.084%
11	9.175	1028	1035	1043	rBV	893758	1411029	21.14%	2.344%
12	9.904	1151	1159	1170	rBV	615891	1014084	15.19%	1.685%
13	10.439	1242	1250	1268	rBV	1111909	1827170	27.37%	3.036%
14	10.827	1308	1316	1323	rBV	1112089	1811238	27.13%	3.009%
15	10.957	1331	1338	1352	rBV	1237349	2025226	30.34%	3.365%
16	12.410	1580	1585	1590	rBV2	19993	33160	0.50%	0.055%
17	14.057	1858	1865	1877	rBV	2199372	2931267	43.91%	4.870%
18	14.339	1906	1913	1925	rBV	2437968	3493055	52.33%	5.803%
19	14.645	1958	1965	1974	rBV	1732410	2445938	36.64%	4.064%
20	14.821	1989	1995	2011	rBV	973477	1368389	20.50%	2.273%
21	15.639	2127	2134	2140	rBV	3092045	4426472	66.31%	7.354%
22	15.745	2145	2152	2164	rVV	697781	975645	14.62%	1.621%
23	15.874	2170	2174	2180	rVB4	15328	24316	0.36%	0.040%
24	17.386	2425	2431	2439	rBV	2152782	2945081	44.12%	4.893%
25	17.486	2442	2448	2464	rBV2	3471867	4820459	72.21%	8.009%
26	19.339	2760	2763	2768	rVB2	33932	41265	0.62%	0.069%
27	19.409	2771	2775	2781	rVB2	34247	44415	0.67%	0.074%
28	19.774	2831	2837	2851	rBV	4501454	5823159	87.23%	9.674%
29	21.568	3137	3142	3155	rBV	2511608	3300543	49.44%	5.483%
30	23.868	3525	3533	3545	rBV2	3312529	6675417	100.00%	11.090%
31	24.027	3552	3560	3571	rVB2	1953362	4024995	60.30%	6.687%




Sum of corrected areas: 60191251

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038835.D
Acq On : 02 Mar 2023 14:21
Operator : CG/JU
Sample : PB150981BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

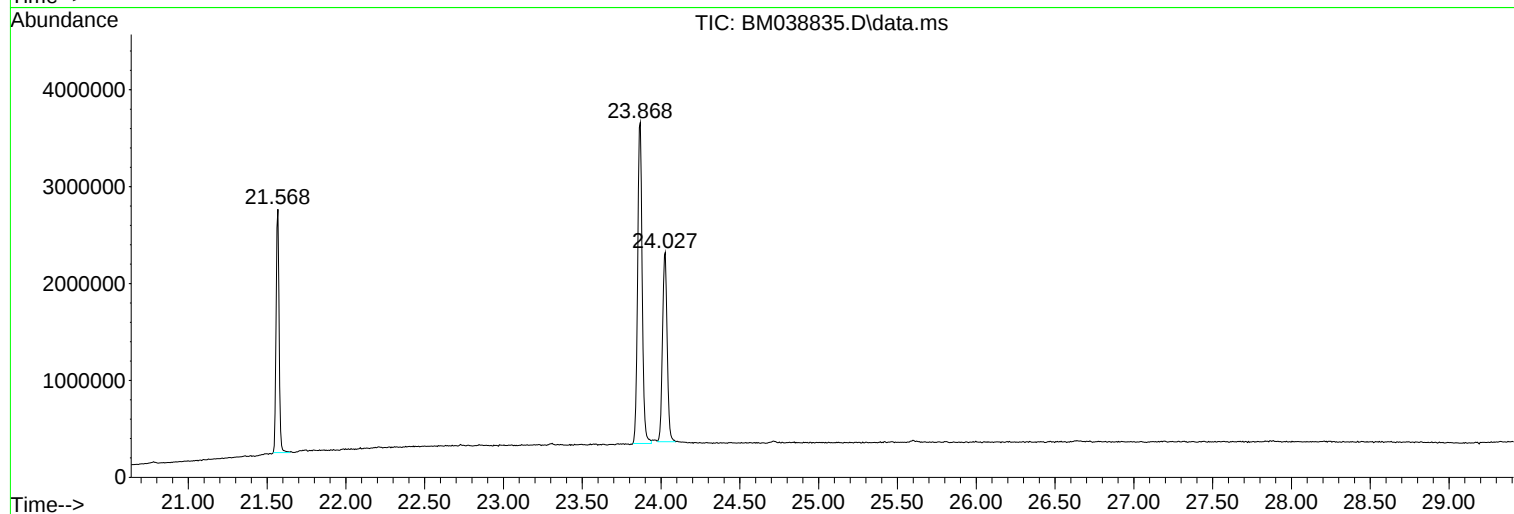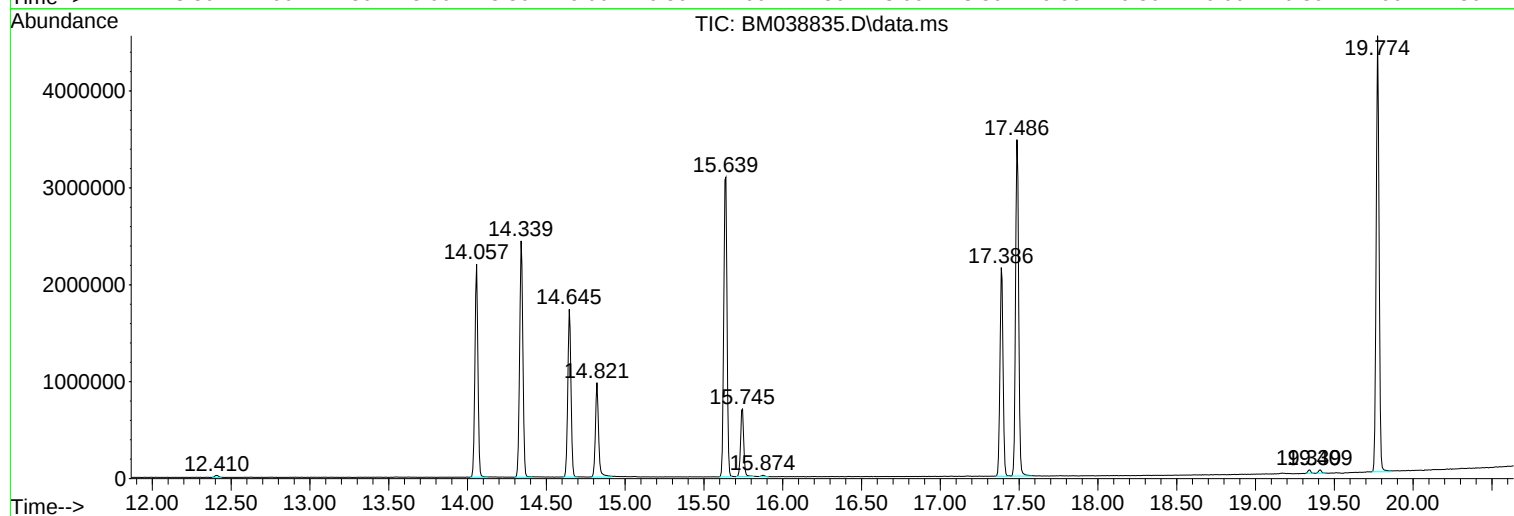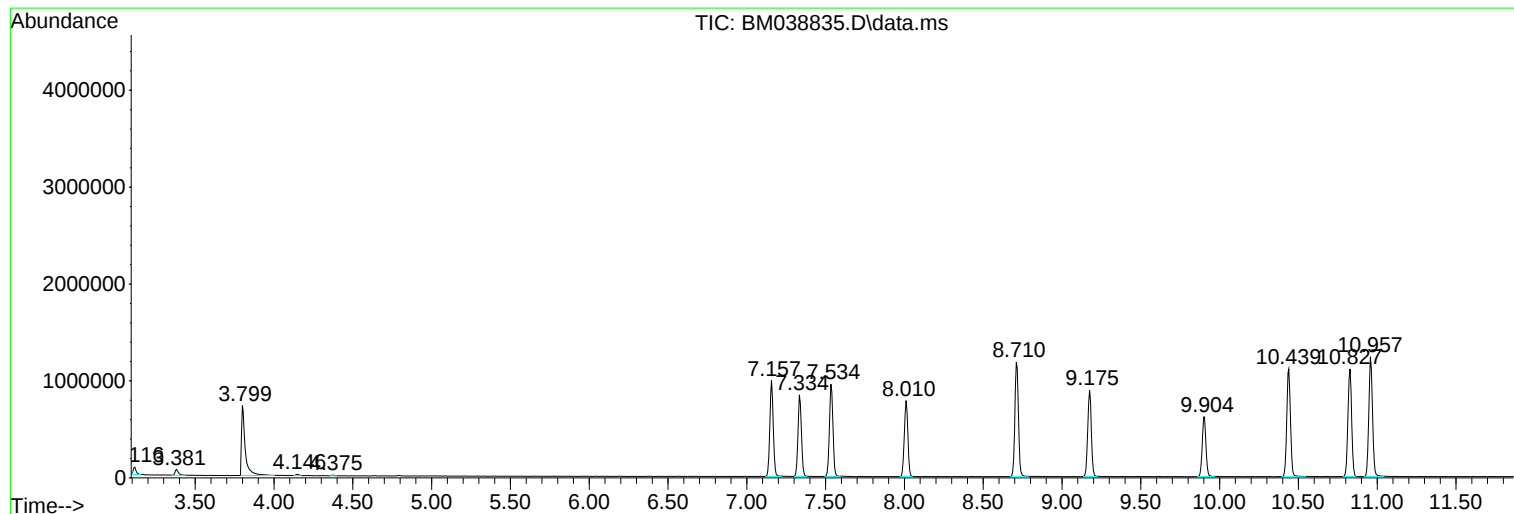

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038835.D
Acq On : 02 Mar 2023 14:21
Operator : CG/JU
Sample : PB150981BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030223\
Data File : BM038835.D
Acq On : 02 Mar 2023 14:21
Operator : CG/JU
Sample : PB150981BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK981

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM022823.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc