
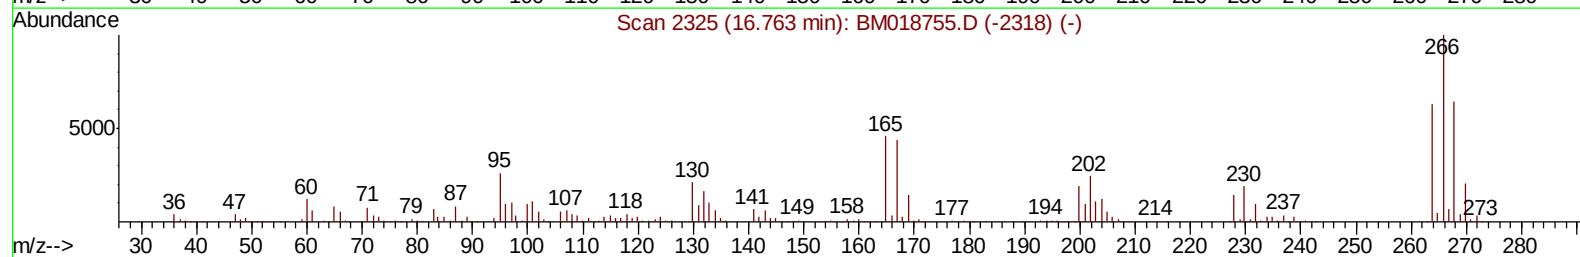
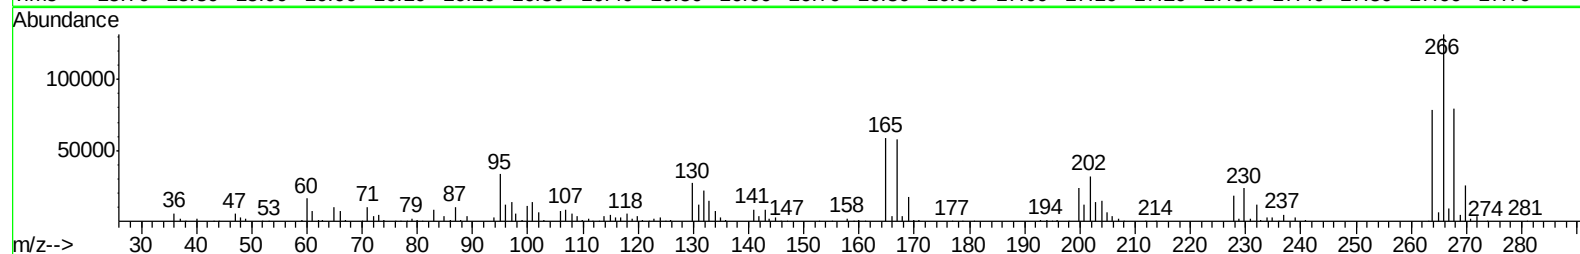


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030519\
Data File : BM019036.D
Acq On : 05 Mar 2019 12:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 06 07:25:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

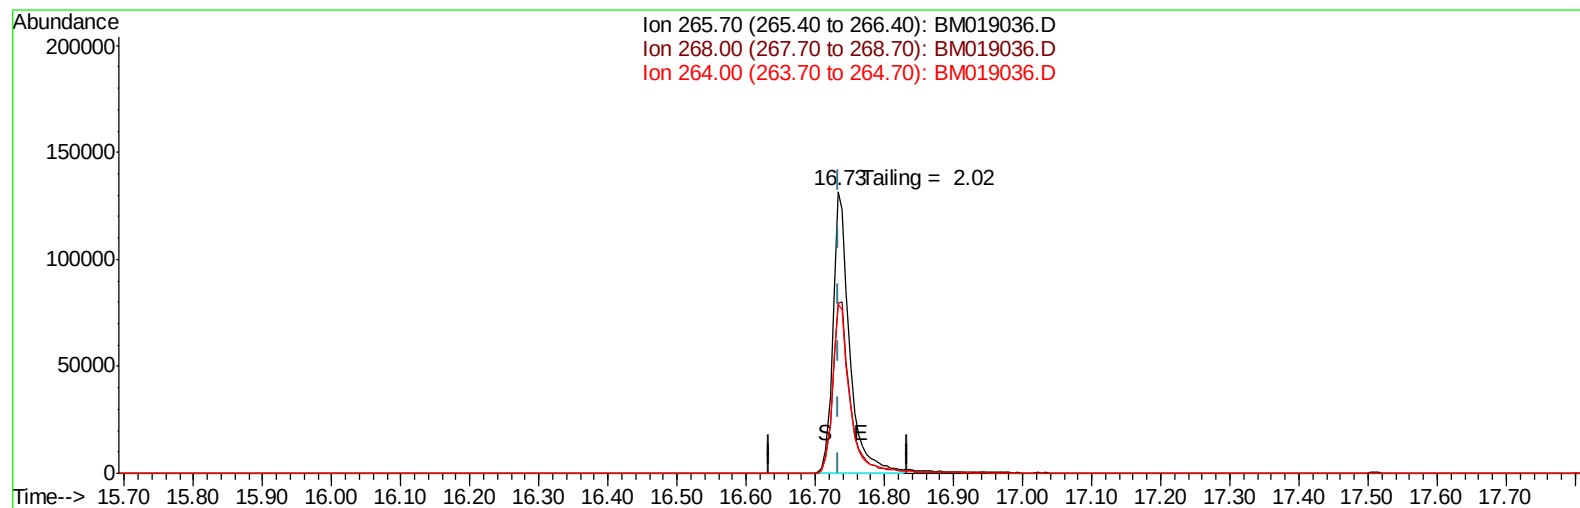

TIC: BM019036.D

(70) Pentachlorophenol (C)




16.733min (-0.000) 0.00ng m

response 220984

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	60.61
264.00	63.20	60.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030519\
Data File : BM019036.D
Acq On : 05 Mar 2019 12:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 06 07:25:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

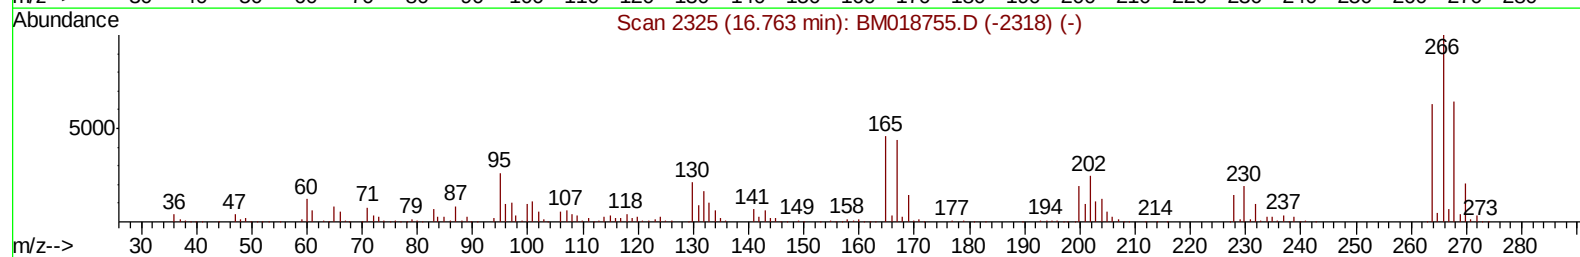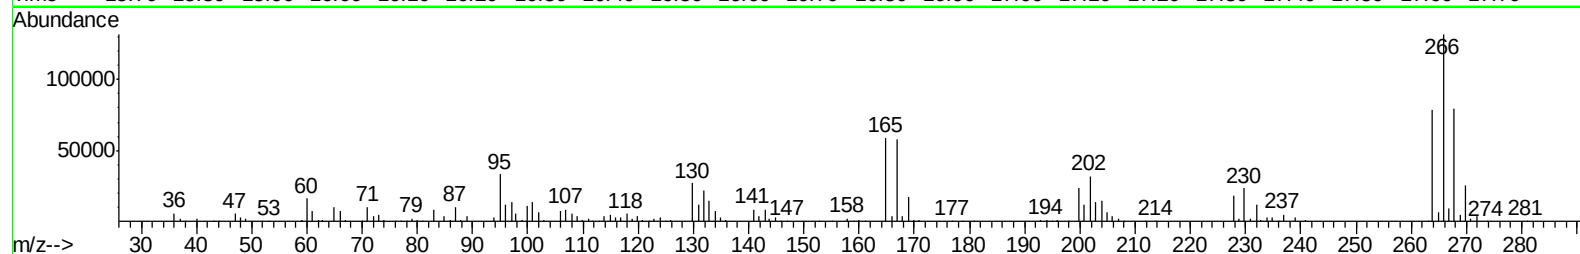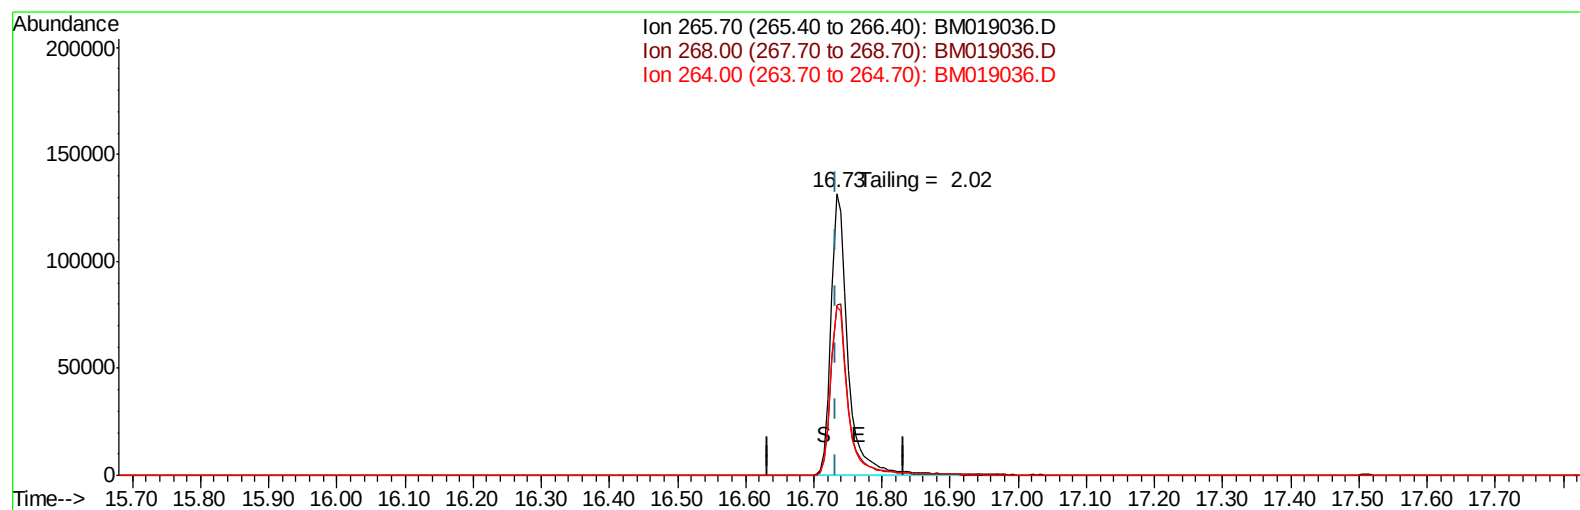

TIC: BM019036.D

(70) Pentachlorophenol (C)




16.733min (-0.000) 0.00ng m

response 220984

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	60.61
264.00	63.20	60.00
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030519\
Data File : BM019036.D
Acq On : 05 Mar 2019 12:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 06 07:25:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

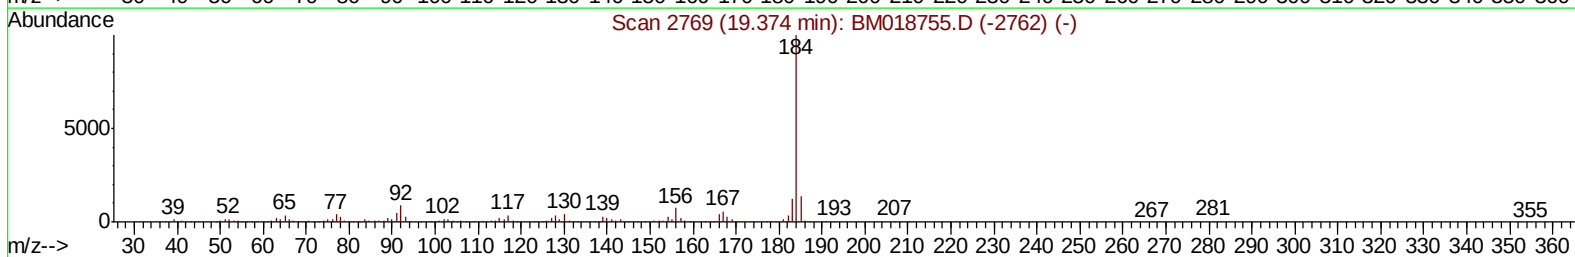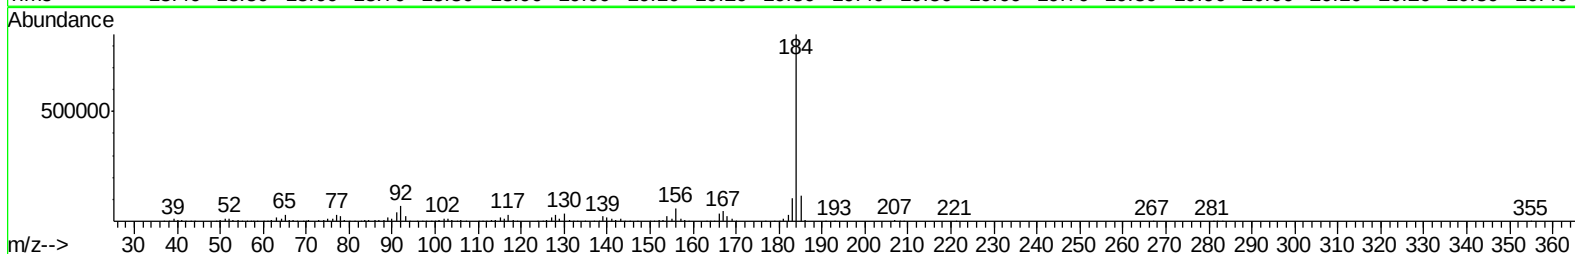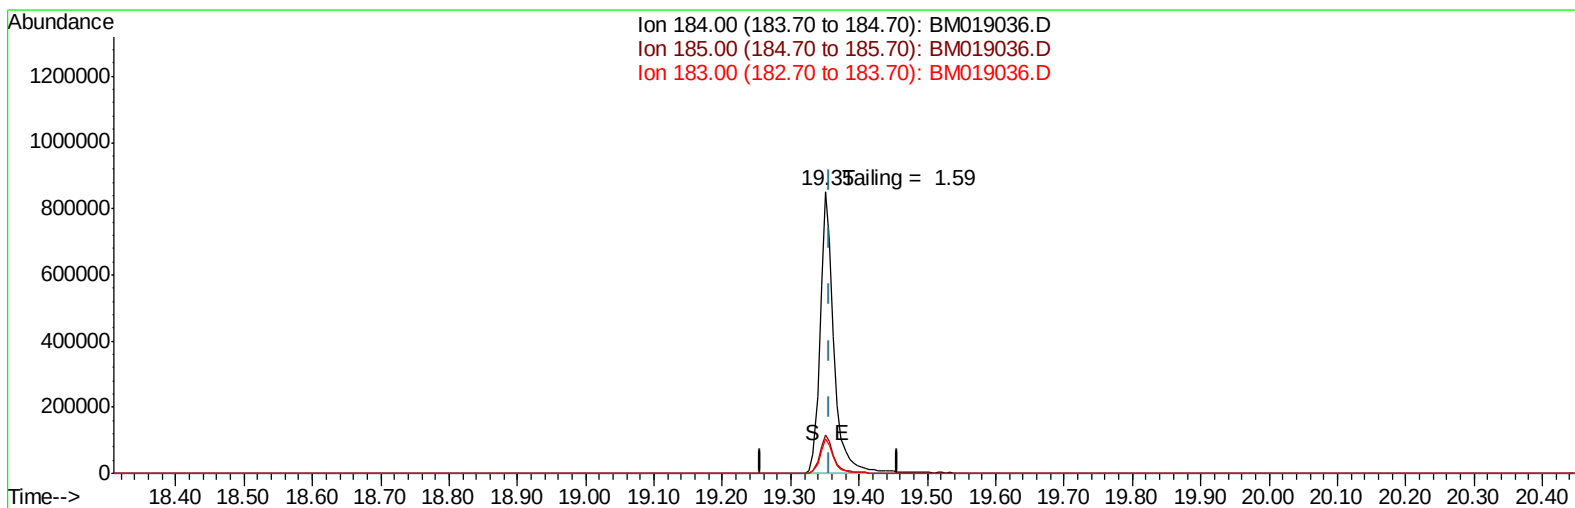

TIC: BM019036.D

(77) Benzidine

19.350min (-0.006) 36063.52ng

response 1200434

Ion	Exp%	Act%
184.00	100	100
185.00	14.00	13.81
183.00	12.10	12.08
0.00	0.00	0.00