
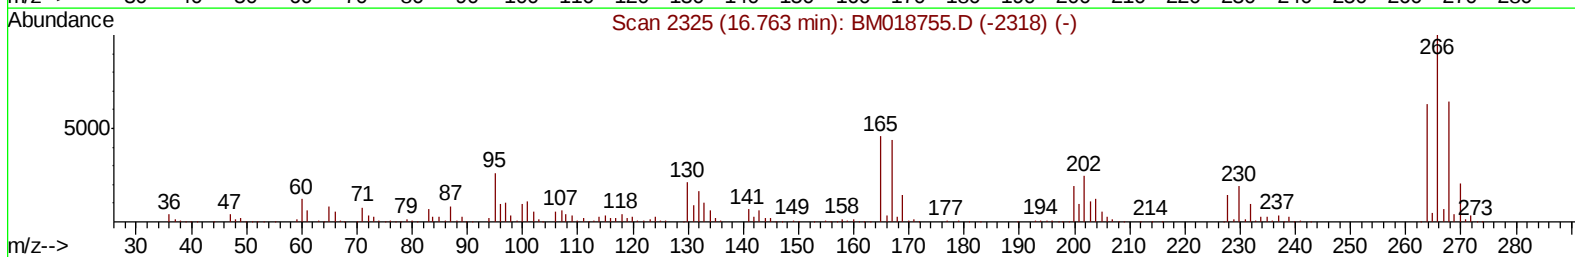
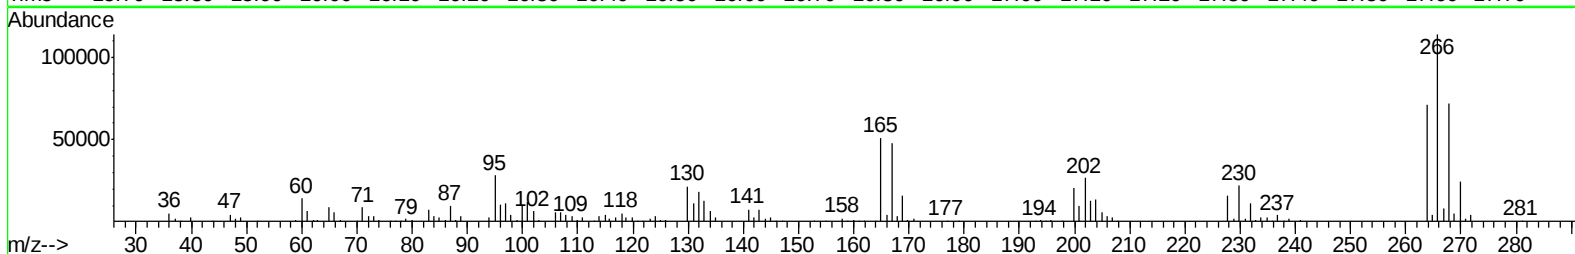


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM030519\
Data File : BM019051.D
Acq On : 06 Mar 2019 01:13
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 06 07:27:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 05 03:36:13 2019
Response via : Initial Calibration

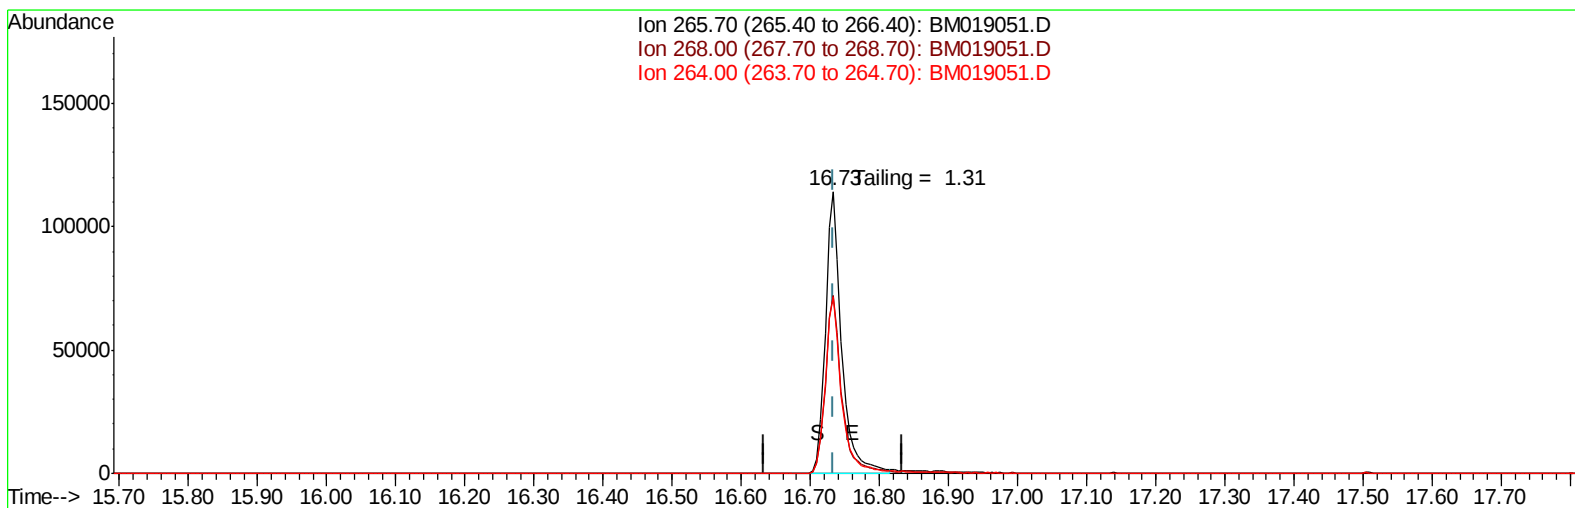

TIC: BM019051.D

(70) Pentachlorophenol (C)

16.733min (-0.000) 151008.74ng

response 184694

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.25
264.00	63.20	62.68
0.00	0.00	0.00

