


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030519\
 Data File : BM019051.D
 Acq On : 06 Mar 2019 01:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM021119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 05 03:36:13 2019

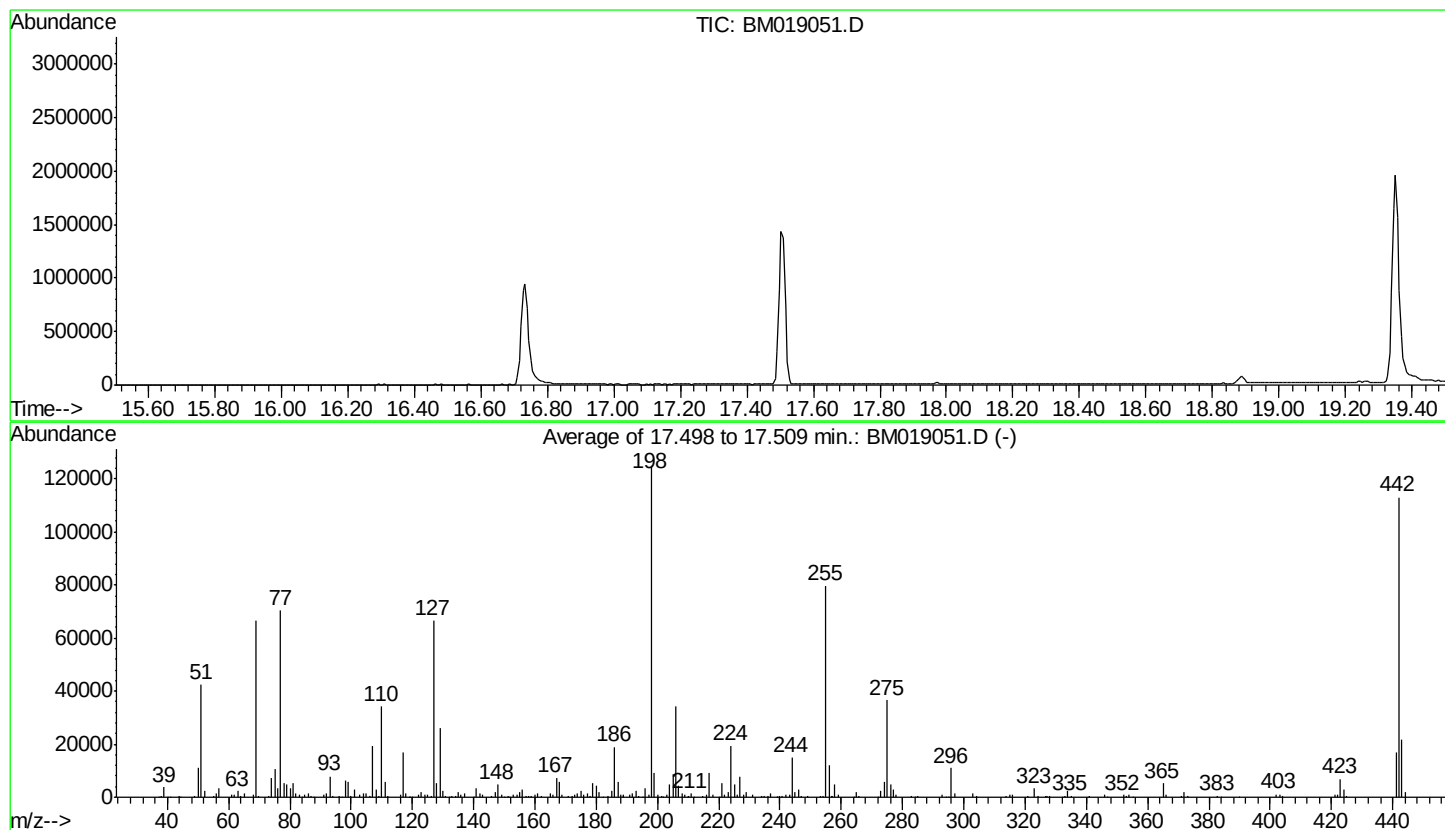

AutoFind: Scans 2450, 2451, 2452; Background Corrected with Scan 2444

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.0	42461	PASS
68	69	0.00	2	1.4	916	PASS
69	198	0.00	100	53.4	66768	PASS
70	69	0.00	2	0.4	279	PASS
127	198	10	80	53.1	66416	PASS
197	198	0.00	2	0.8	1015	PASS
198	198	100	100	100.0	124984	PASS
199	198	5	9	7.2	8945	PASS
275	198	10	60	29.3	36640	PASS
365	198	1	100	4.1	5186	PASS
441	198	0.01	100	13.4	16723	PASS
442	198	50	100	90.4	113042	PASS
443	442	15	24	19.0	21504	PASS