

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025381.D
 Acq On : 08 Mar 2020 12:00
 Operator : CG/JU
 Sample : L1616-21
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 09 01:15:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	4971	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	21182	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	15045	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.22	240	32552	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	31775	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	9793	0.25	ng/ul	-0.02
14) Fluoranthene-d10	19.07	212	27954	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
17) Pyrene	19.46	202	4171	0.034	ng/ul#	96
23) Benzo(a)pyrene	23.27	252	7639	0.072	ng/ul#	81


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025381.D
Acq On : 08 Mar 2020 12:00
Operator : CG/JU
Sample : L1616-21
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 09 01:15:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration




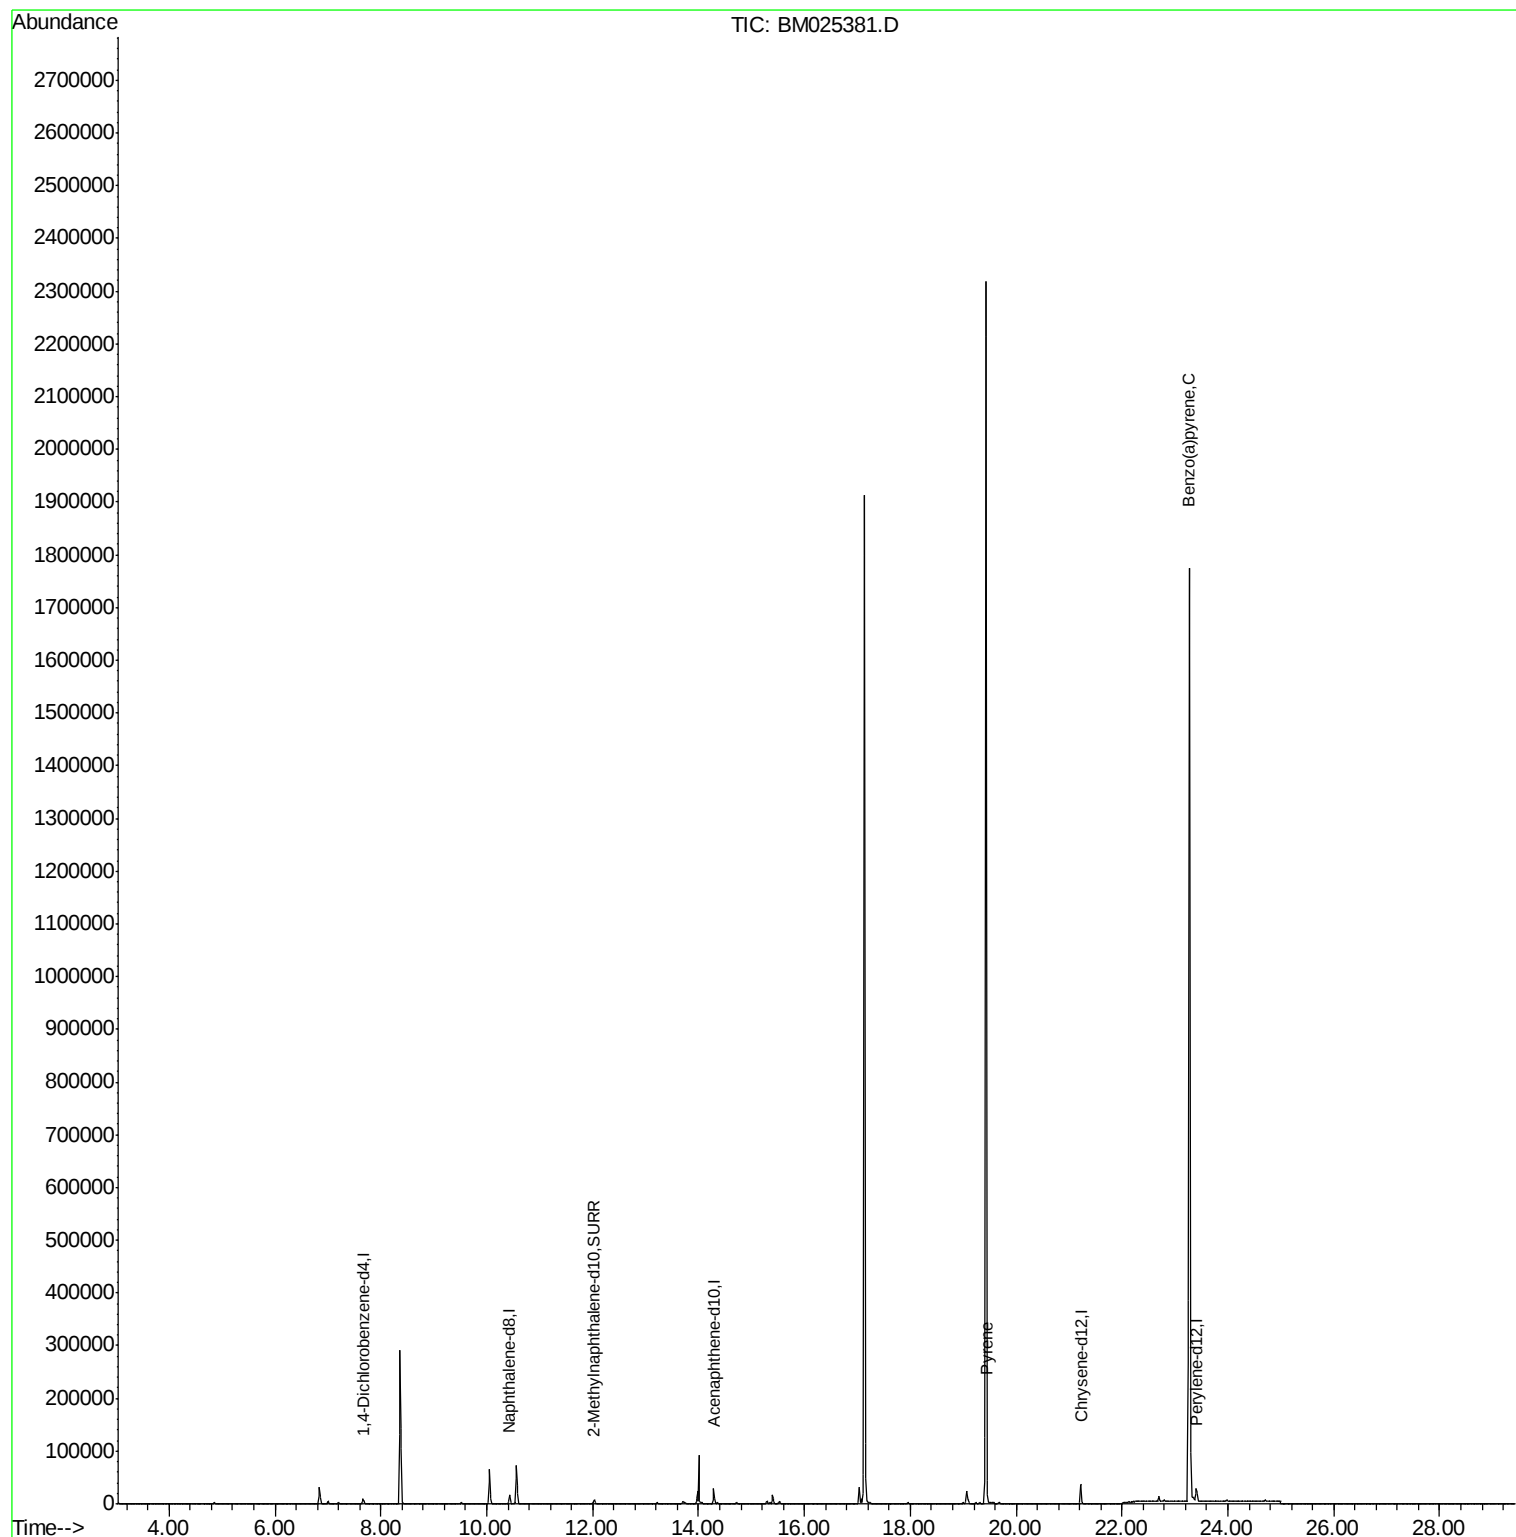


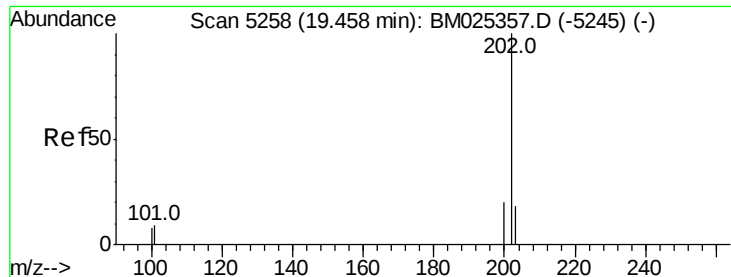

#17
Pvrene
Concen: 0.034 ng/ul
RT: 19.46 min Scan# 5258
Delta R.T. -0.01 min
Lab File: BM025381.D
Acq: 08 Mar 2020 12:00

Instrument :
BNA_M
ClientSampleId :

Tot Ion:202 Resp: 4171
Ion Ratio Lower Upper
202 100
101 11.8 8.7 13.1
100 11.5 7.3 10.9#

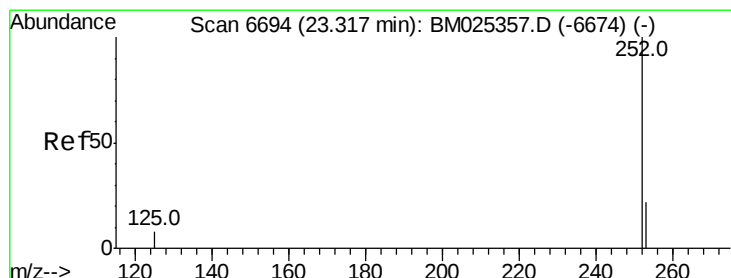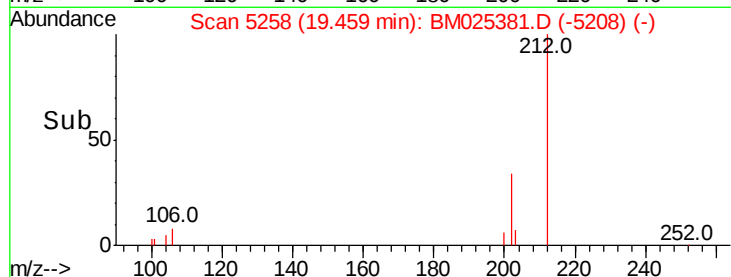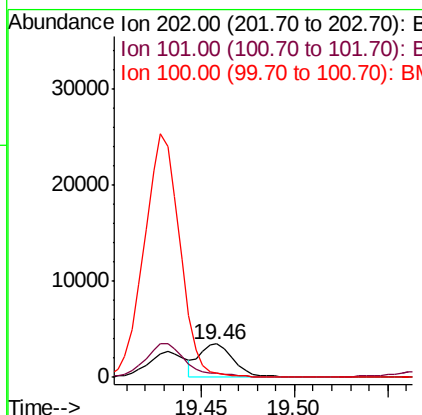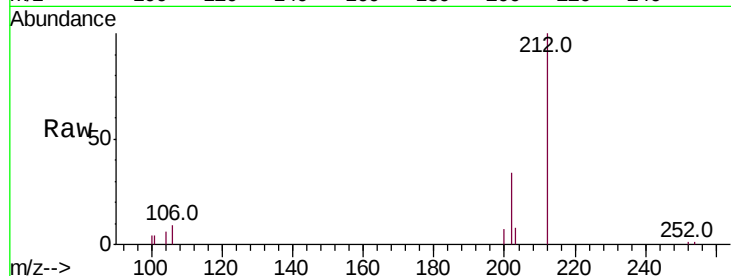

#23
Benzo(a)pyrene
Concen: 0.072 ng/ul
RT: 23.27 min Scan# 6676
Delta R.T. -0.05 min
Lab File: BM025381.D
Acq: 08 Mar 2020 12:00

Tgt Ion:252 Resp: 7639
Ion Ratio Lower Upper
252 100
253 35.2 20.3 30.5#
125 24.2 13.0 19.4#

