

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025390.D
 Acq On : 08 Mar 2020 17:58
 Operator : CG/JU
 Sample : L1617-06
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 09 01:15:49 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	5793	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	25049	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	18047	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.22	240	36802	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	32485	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.02	152	13549	0.29	ng/ul	-0.02
14) Fluoranthene-d10	19.07	212	36423	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.43	202	4774	0.034	ng/ul#	Ovalue 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025390.D
Acq On : 08 Mar 2020 17:58
Operator : CG/JU
Sample : L1617-06
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 09 01:15:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

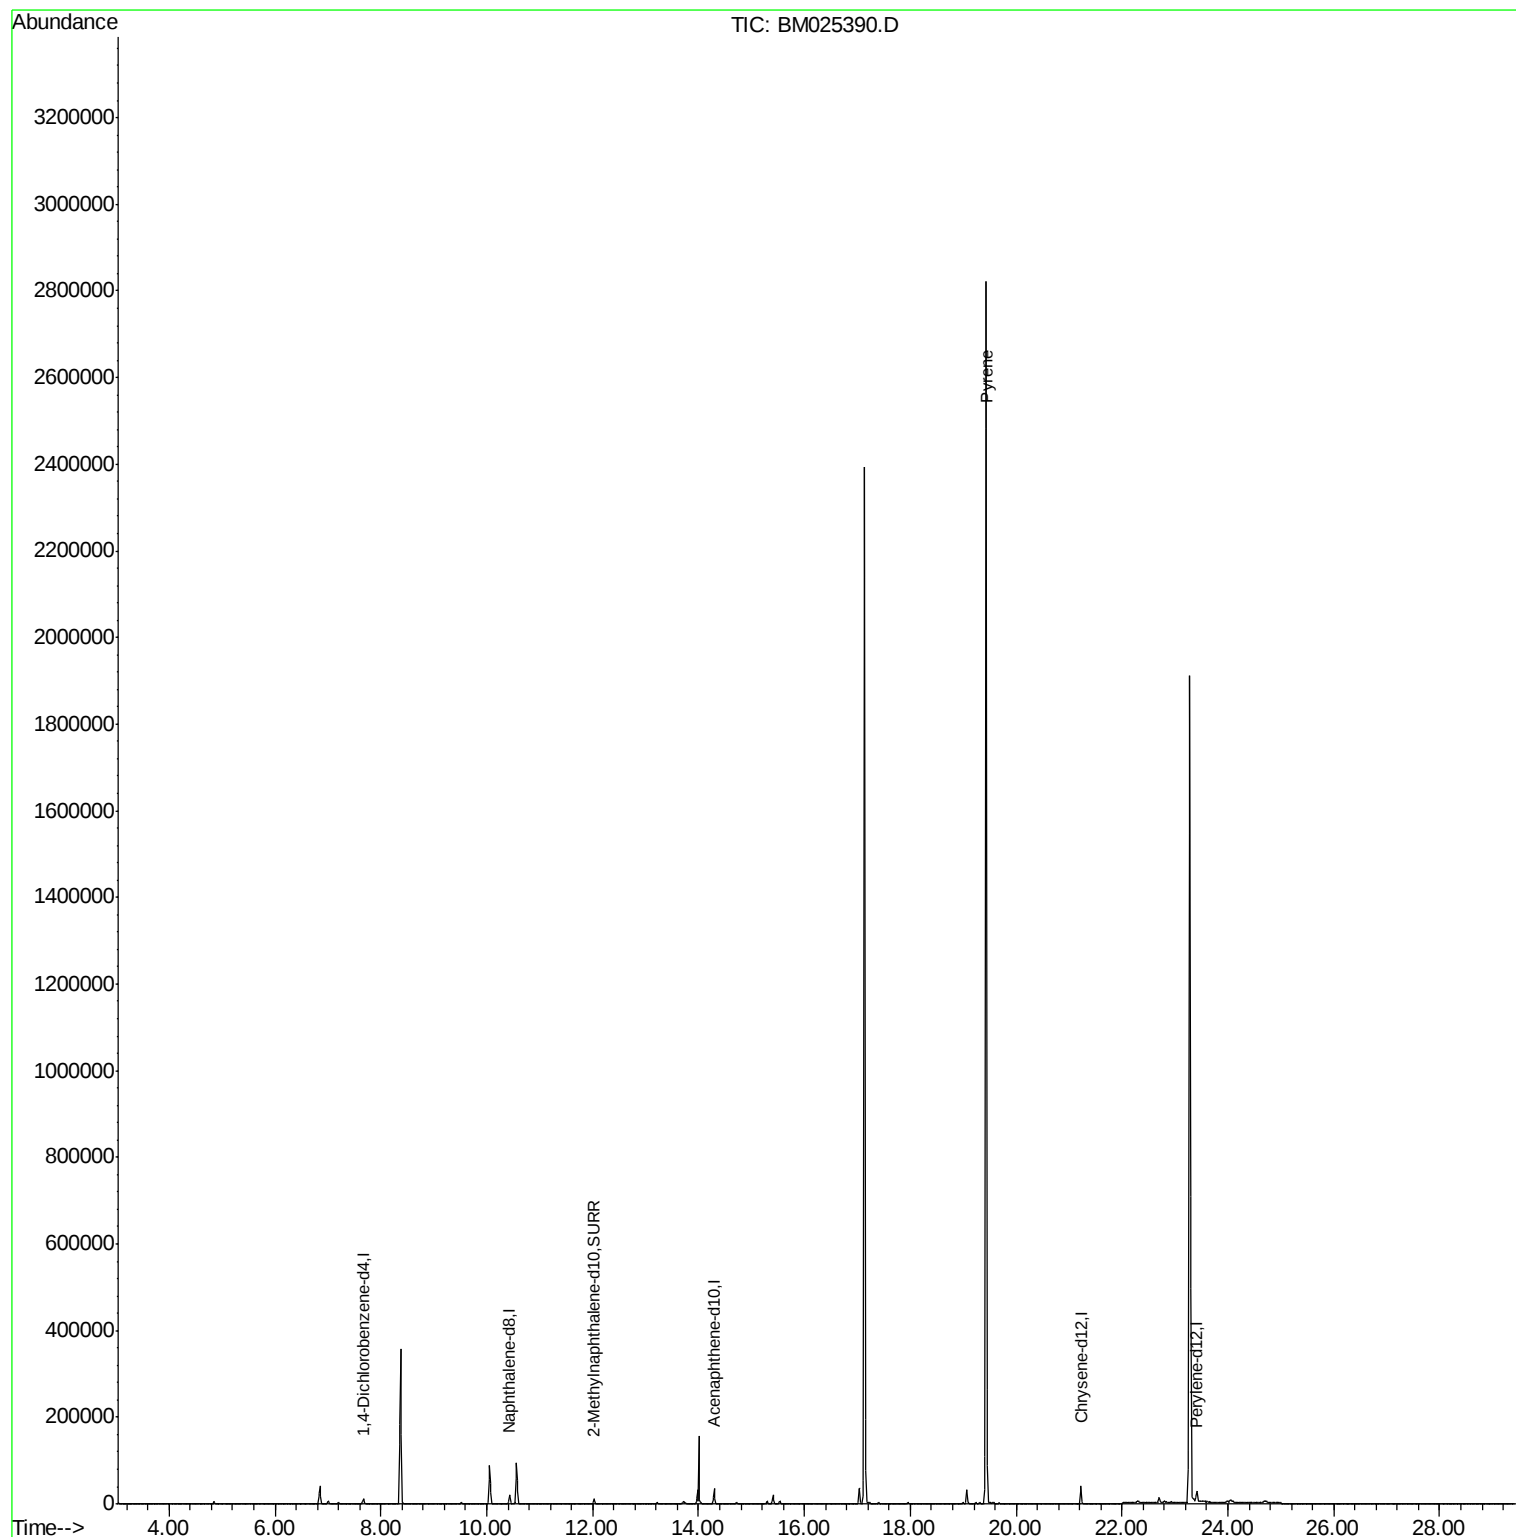

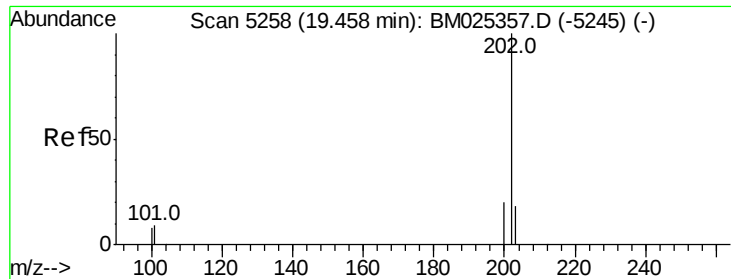

#17
 Pvrene
 Concen: 0.034 ng/ul
 RT: 19.43 min Scan# 5251
 Delta R.T. -0.04 min
 Lab File: BM025390.D
 Acq: 08 Mar 2020 17:58

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:202 Resp: 4774
 Ion Ratio Lower Upper
 202 100
 101 136.8 8.7 13.1#
 100 986.8 7.3 10.9#

