

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025392.D
 Acq On : 08 Mar 2020 19:10
 Operator : CG/JU
 Sample : L1617-05
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 09 01:15:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	6182	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.43	136	26638	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	19029	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.22	240	38222	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	33241	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	12489	0.25	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	33309	0.00	ng/ul	-0.01
Target Compounds						
23) Benzo(a)pyrene	23.28	252	7478	0.067	ng/ul#	Ovalue 79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025392.D
Acq On : 08 Mar 2020 19:10
Operator : CG/JU
Sample : L1617-05
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 09 01:15:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

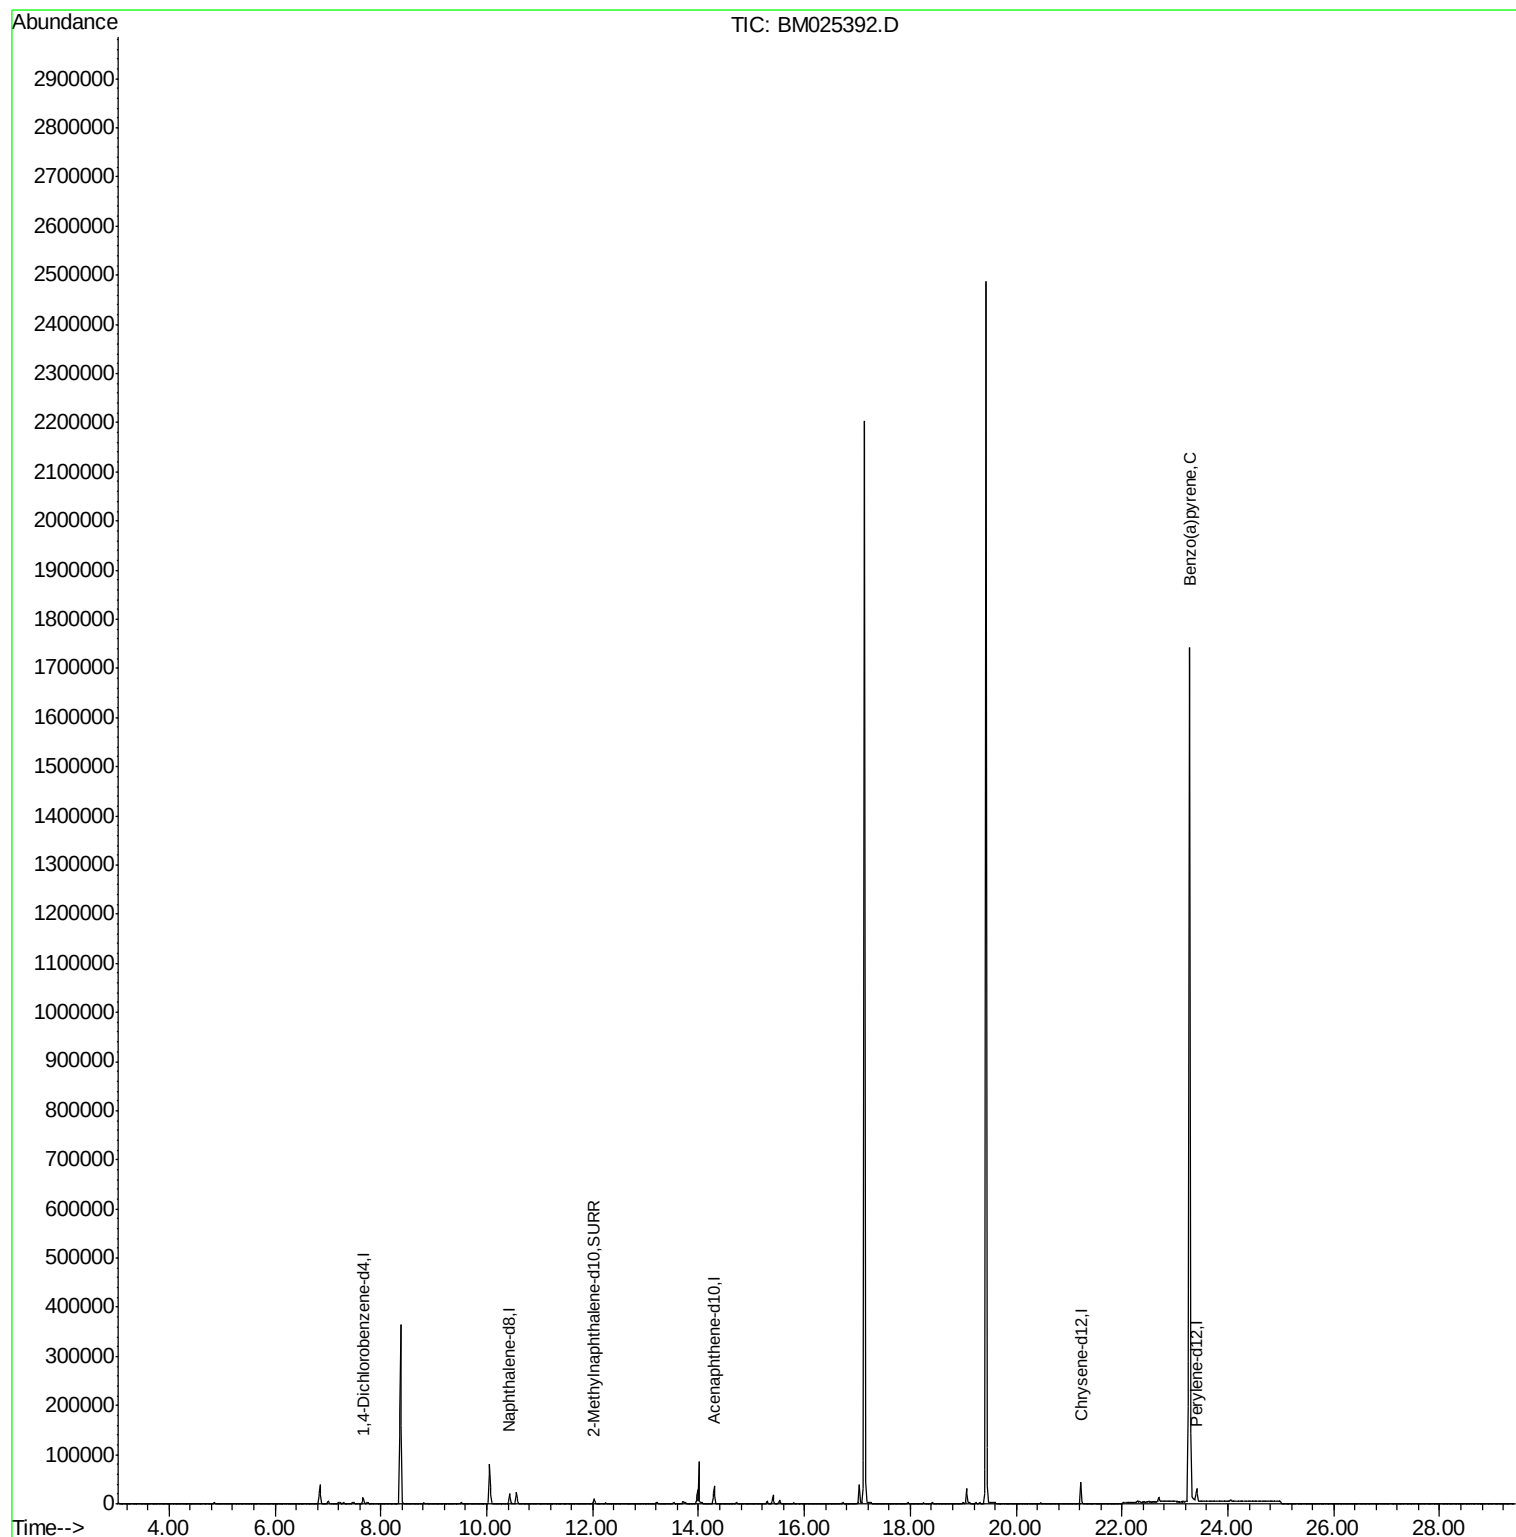

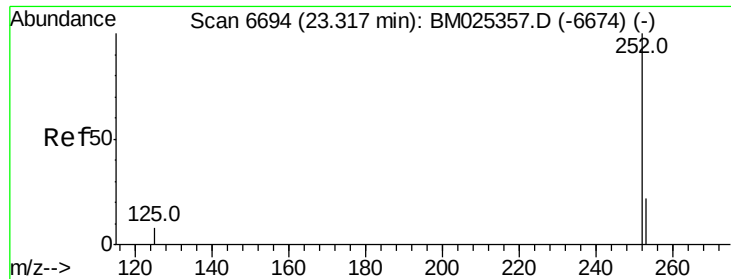

#23

Benzo(a)pyrene

Concen: 0.067 ng/ul

RT: 23.28 min Scan# 6677

Delta R.T. -0.05 min


Lab File: BM025392.D

Acq: 08 Mar 2020 19:10

Instrument :

BNA_M

ClientSampleId :

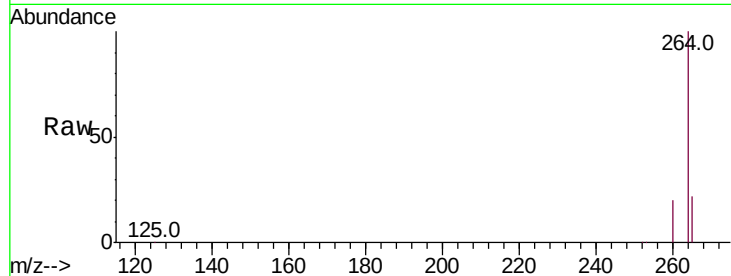


Tot Ion: 252 Resp: 7478

Ion Ratio Lower Upper

252 100

253 35.8 20.3 30.5#

125 24.8 13.0 19.4#

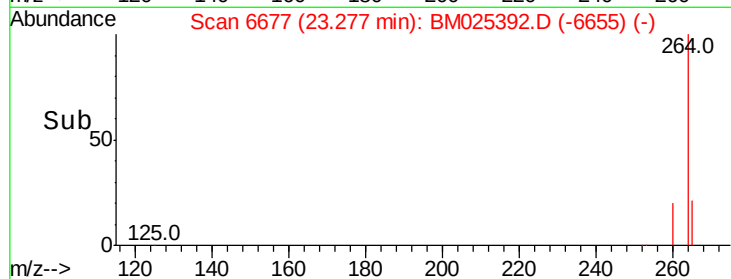

Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

