

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025393.D
 Acq On : 08 Mar 2020 19:46
 Operator : CG/JU
 Sample : L1617-11
 Misc :
 ALS Vial : 79 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 09 01:16:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3912	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	17479	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	13232	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.22	240	28773	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	26022	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	10469	0.32	ng/ul	-0.02
14) Fluoranthene-d10	19.07	212	30797	0.00	ng/ul	0.00
Target Compounds						
17) Pyrene	19.43	202	4960	0.045	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025393.D
Acq On : 08 Mar 2020 19:46
Operator : CG/JU
Sample : L1617-11
Misc :
ALS Vial : 79 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 09 01:16:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

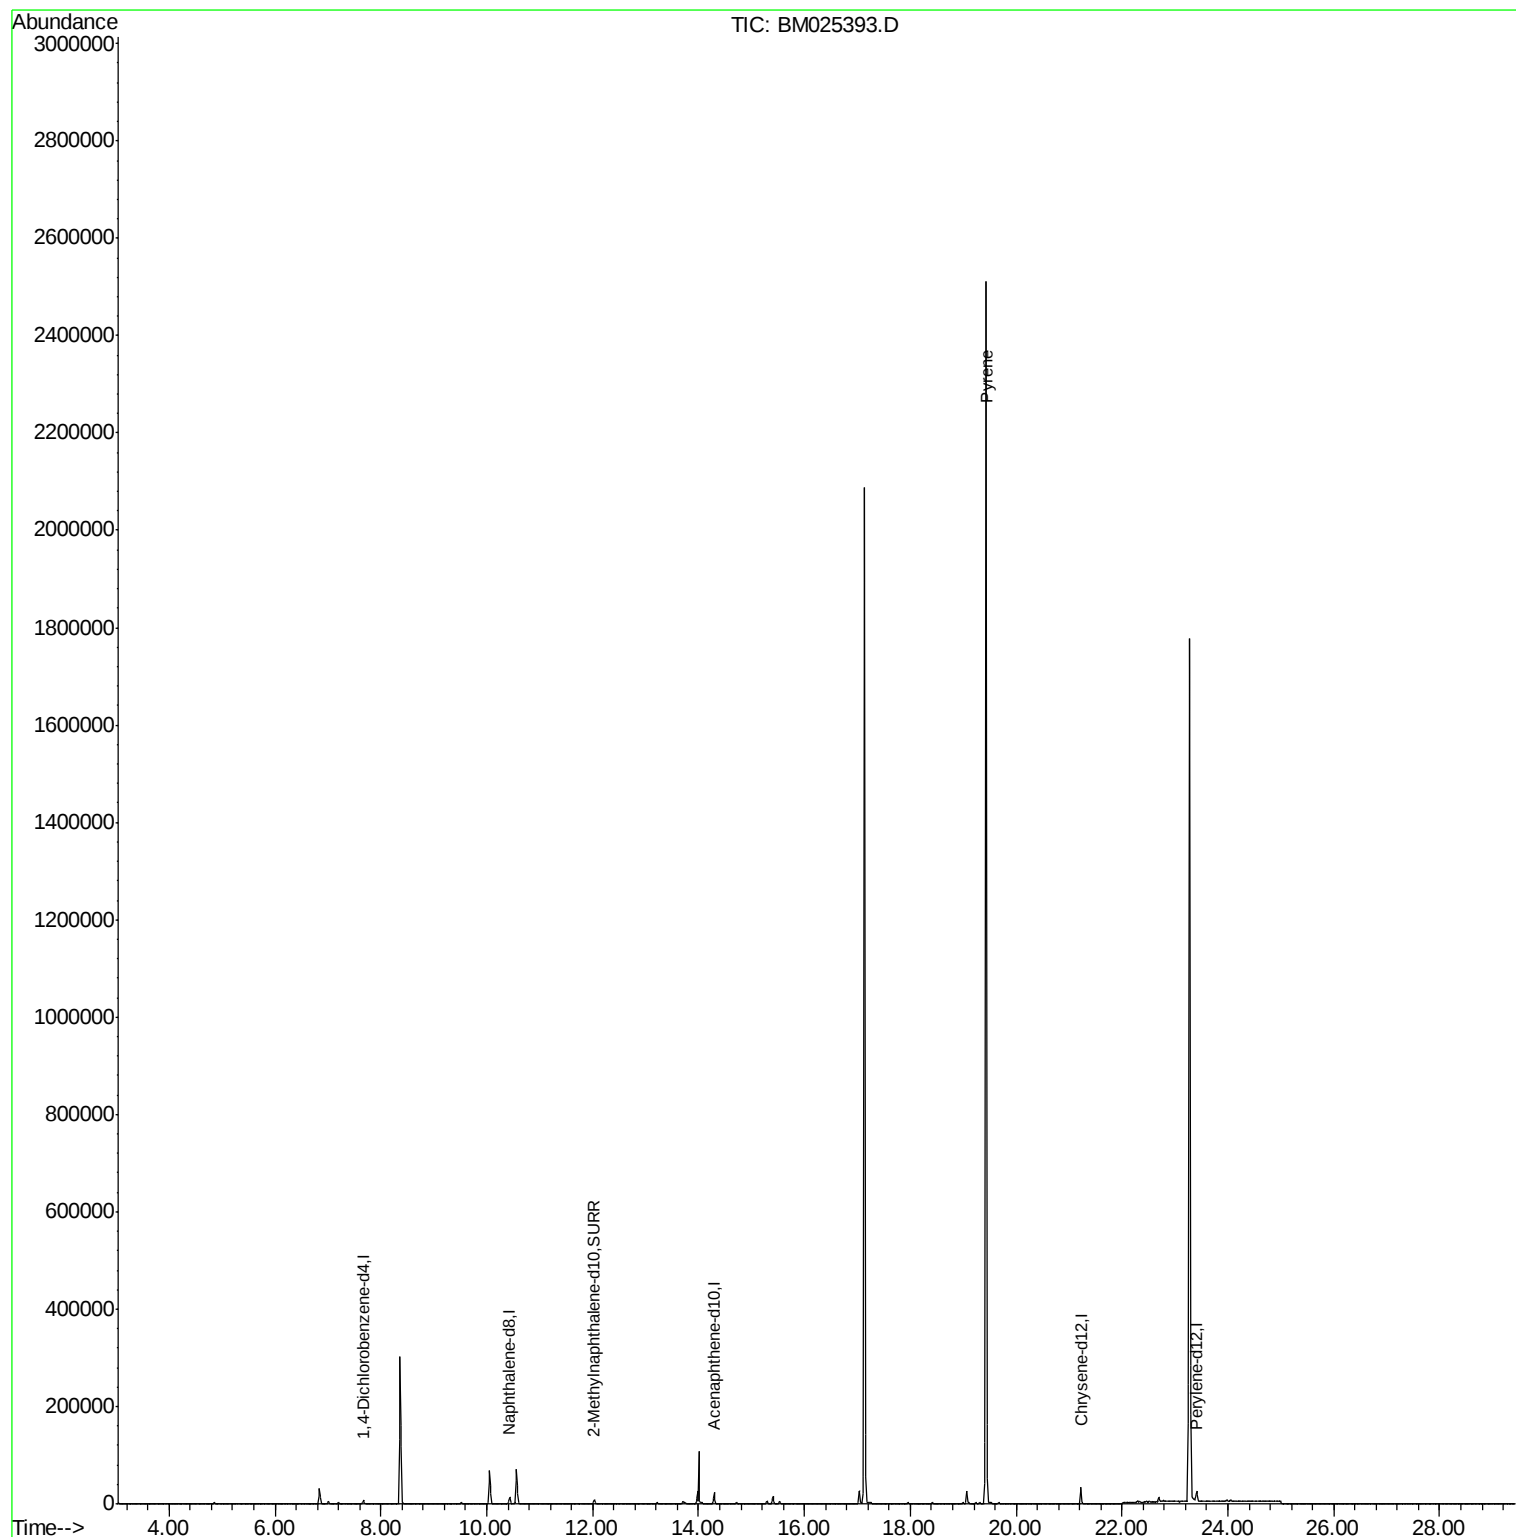


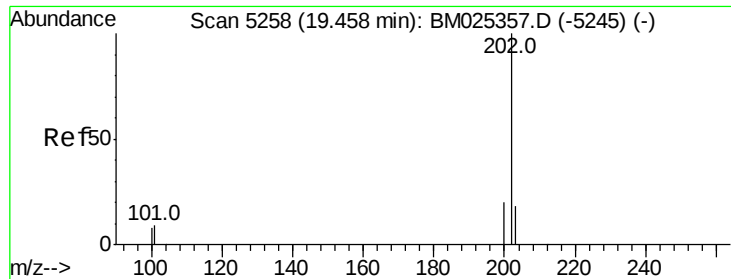

#17
 Pvrene
 Concen: 0.045 ng/ul
 RT: 19.43 min Scan# 5251
 Delta R.T. -0.04 min
 Lab File: BM025393.D
 Acq: 08 Mar 2020 19:46

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
202	100		
101	142.3	8.7	13.1#
100	967.6	7.3	10.9#

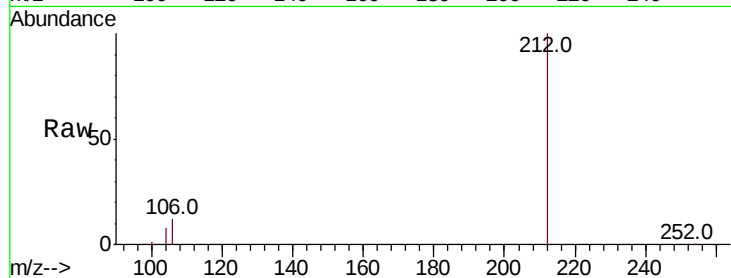

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

