

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
 Data File : BM025398.D
 Acq On : 08 Mar 2020 23:21
 Operator : CG/JU
 Sample : L1617-16
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 09 01:16:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	4494	0.40	ng/ul	-0.01
2) Naphthalene-d8	10.43	136	19204	0.40	ng/ul	-0.01
6) Acenaphthene-d10	14.29	164	14042	0.40	ng/ul	-0.01
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-17.05
16) Chrysene-d12	21.22	240	29468	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	26799	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	8879	0.25	ng/ul	-0.01
14) Fluoranthene-d10	19.06	212	24436	0.00	ng/ul	-0.01
Target Compounds						
17) Pyrene	19.46	202	4304	0.039	ng/ul#	Ovalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM030620\
Data File : BM025398.D
Acq On : 08 Mar 2020 23:21
Operator : CG/JU
Sample : L1617-16
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 09 01:16:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

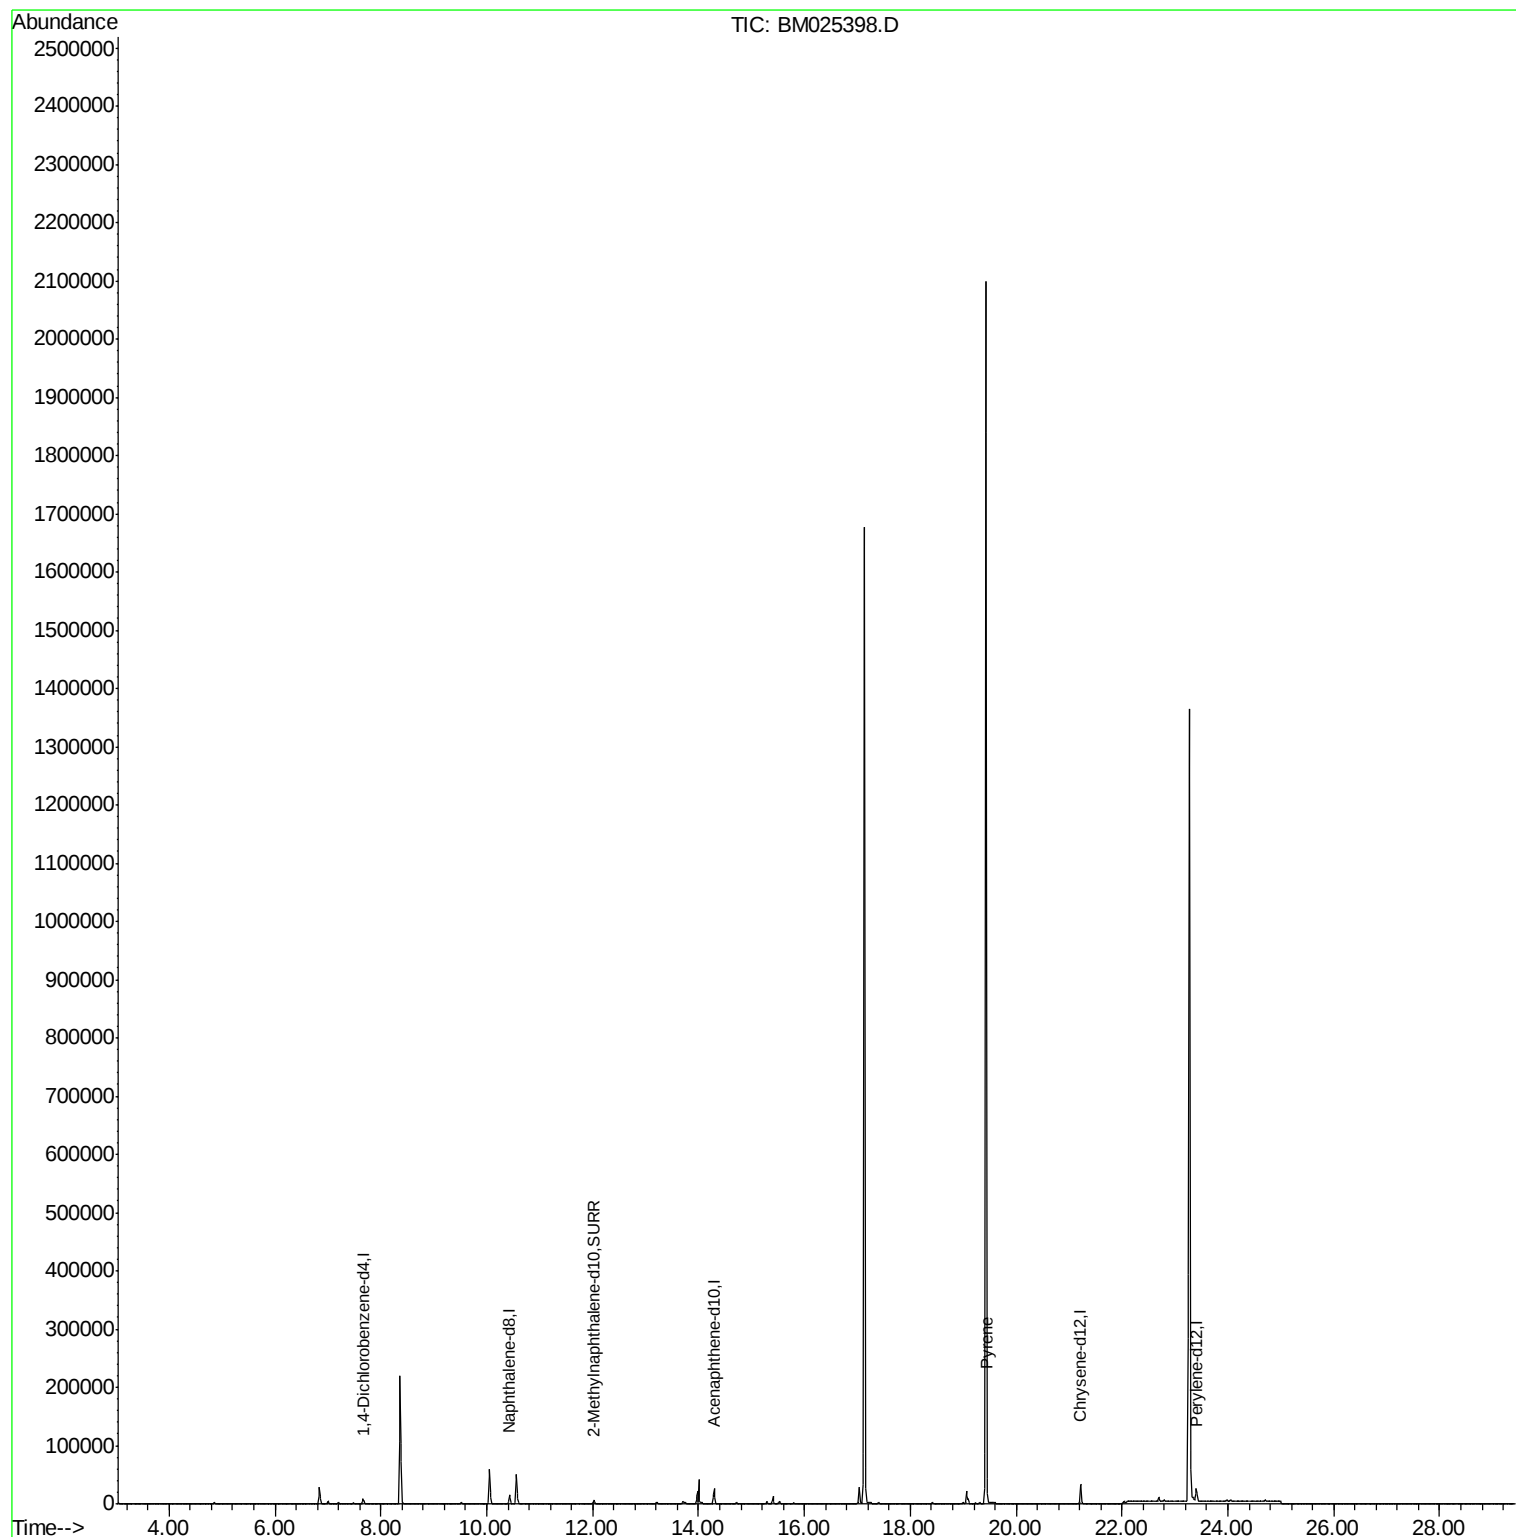

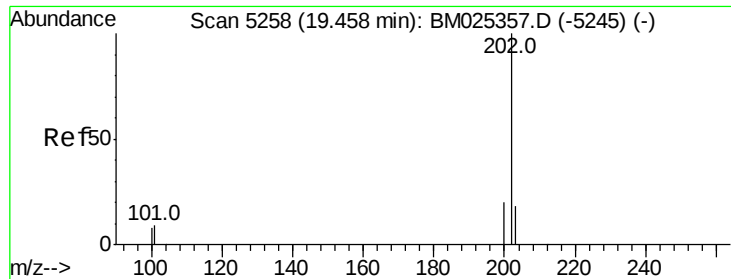

#17

Pvrene

Concen: 0.039 ng/ul

RT: 19.46 min Scan# 5257

Delta R.T. -0.01 min

Lab File: BM025398.D

Acq: 08 Mar 2020 23:21

Instrument :

BNA_M

ClientSampleId :

Tot Ion:202 Resp: 4304

Ion Ratio Lower Upper

202 100

101 11.5 8.7 13.1

100 12.4 7.3 10.9#

