


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025316.D
Acq On : 06 Mar 2020 15:21
Operator : CG/JU
Sample : PB127028BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 06 16:14:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK28

Manual Integrations
APPROVED

mohammad
3/9/2020 2:59:59 PM

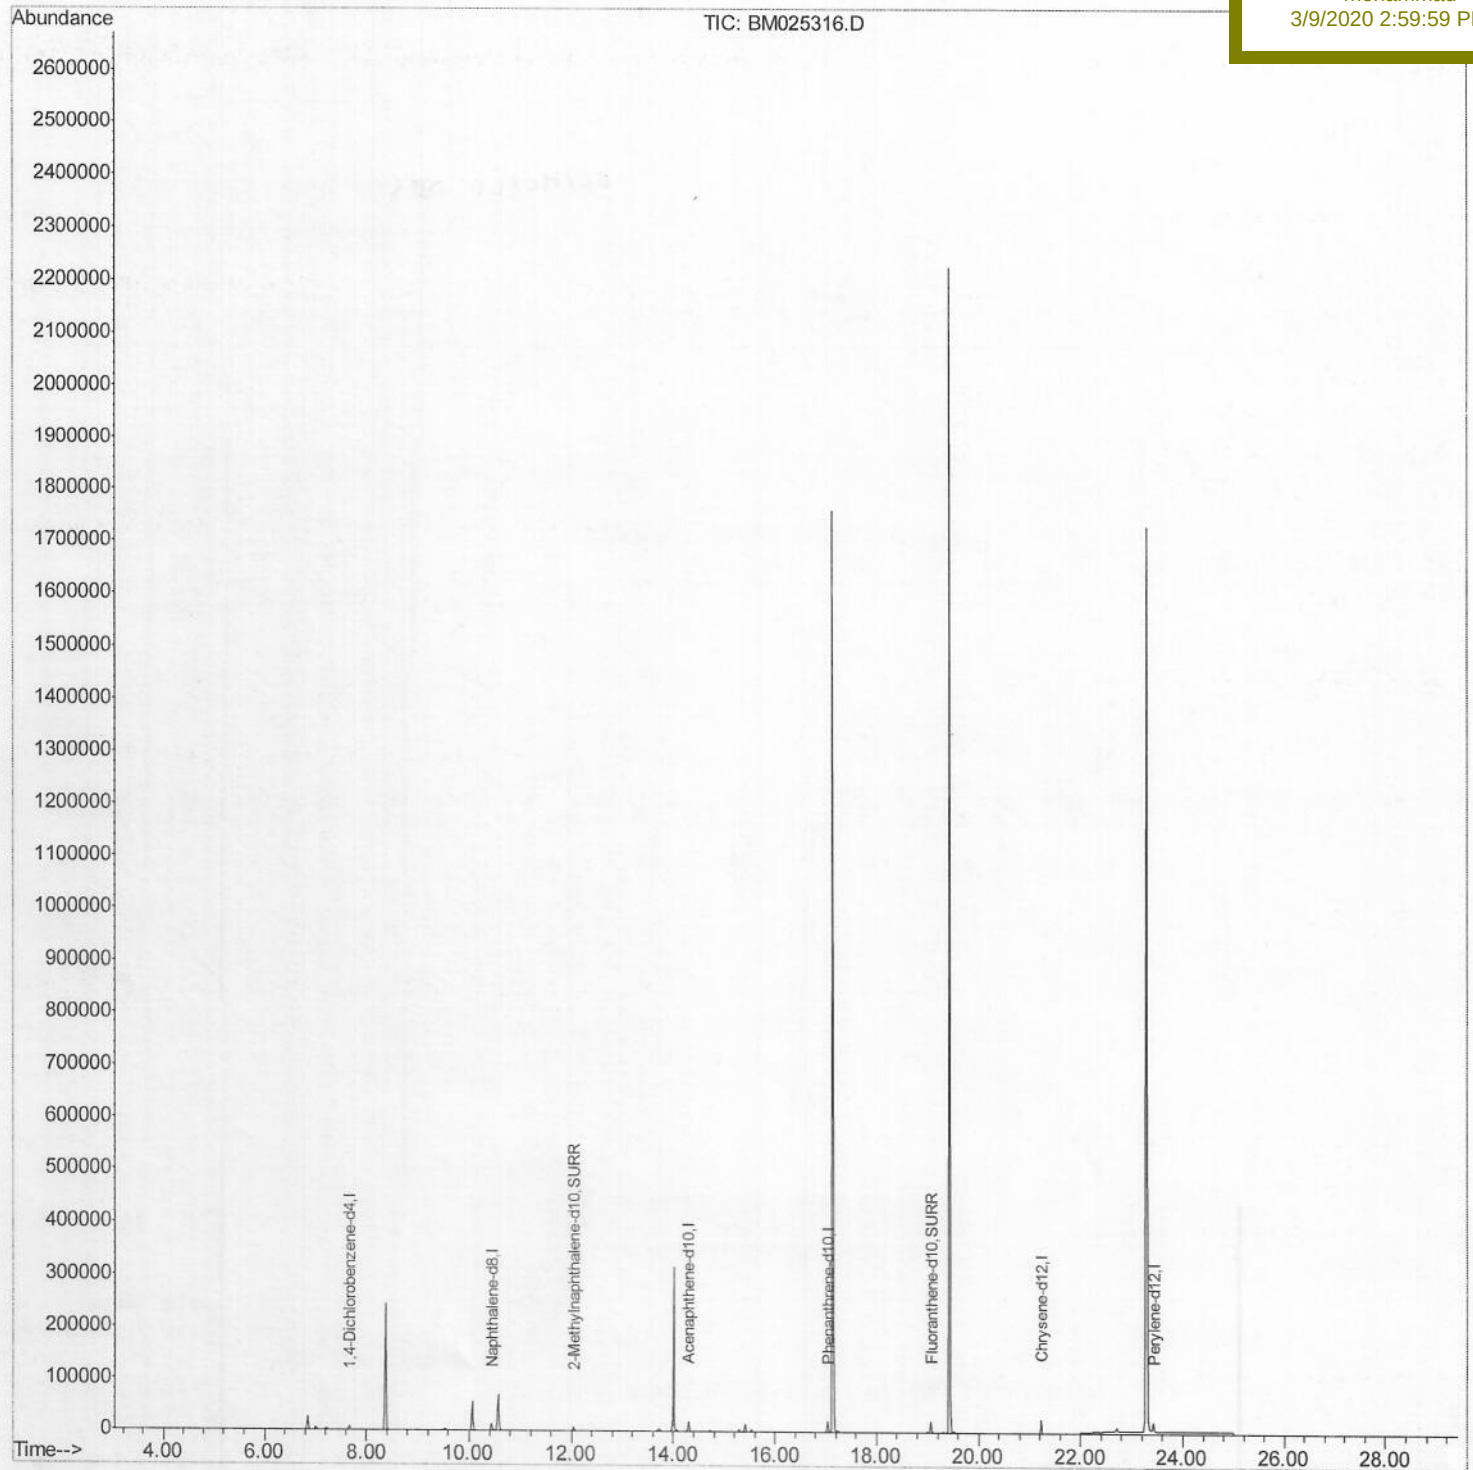

Quantitation Report (Qedit)


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
 Data File : BM025316.D
 Acq On : 06 Mar 2020 15:21
 Operator : CG/JU
 Sample : PB127028BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 06 16:12:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 SBLK28

Manual Integrations
 APPROVED

mohammad
 3/9/2020 2:59:59 PM

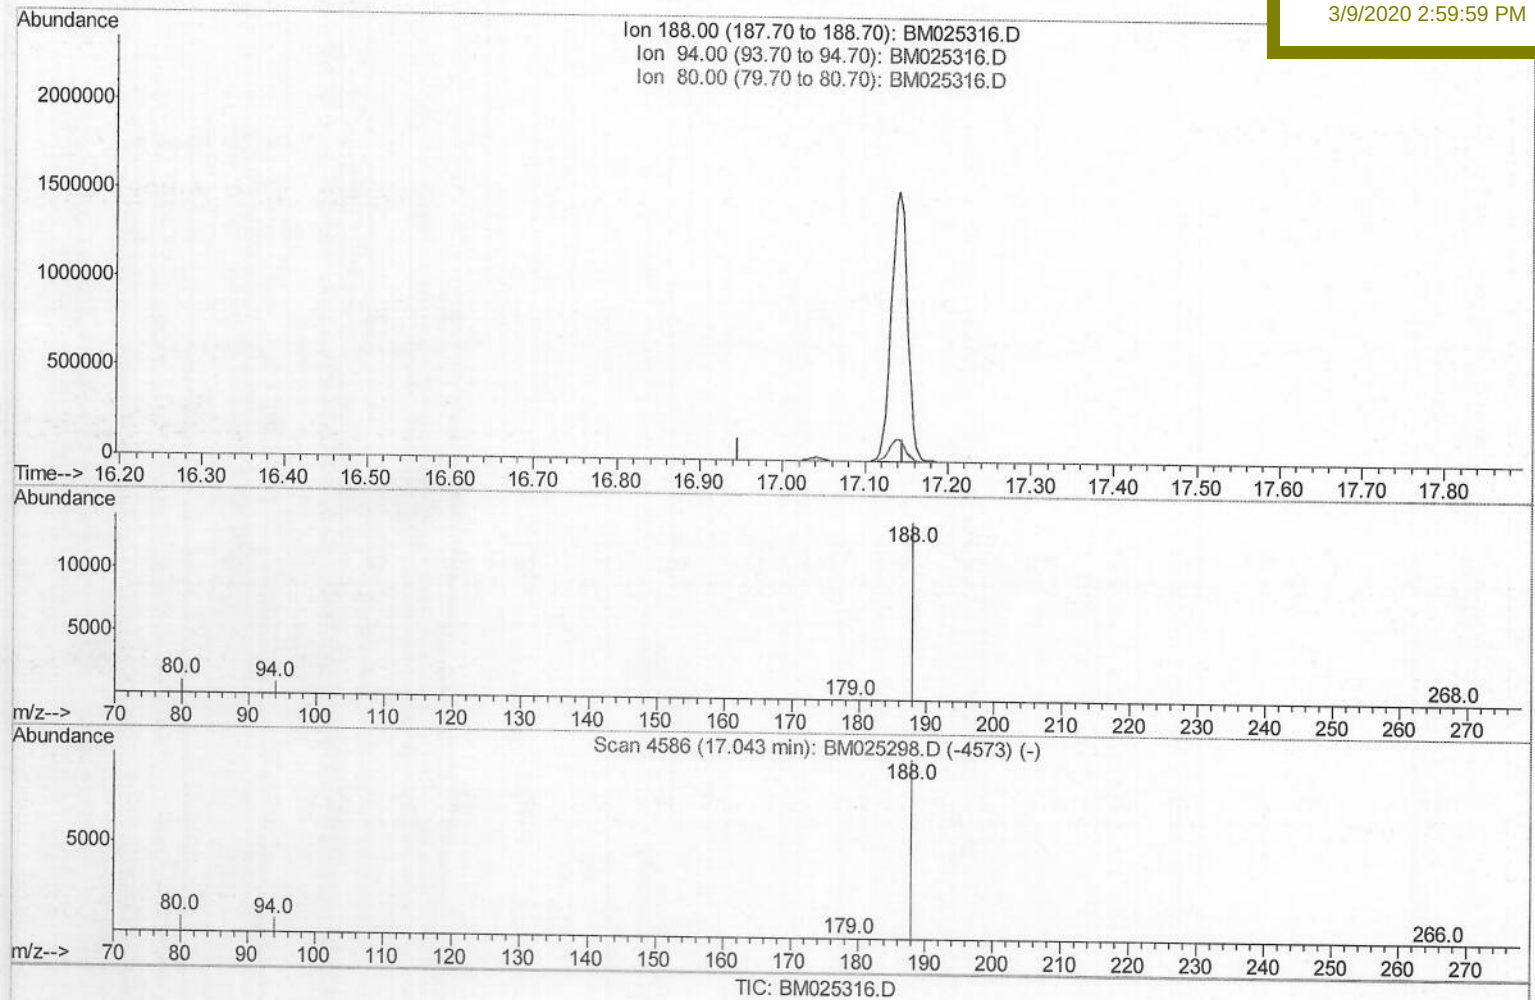

(10) Phenanthrene-d10 (I)
 17.046min (-17.046) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025316.D
Acq On : 06 Mar 2020 15:21
Operator : CG/JU
Sample : PB127028BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Quant Time: Mar 06 16:12:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 04 08:02:03 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
SBLK28

Manual Integrations
APPROVED

mohammad
3/9/2020 2:59:59 PM

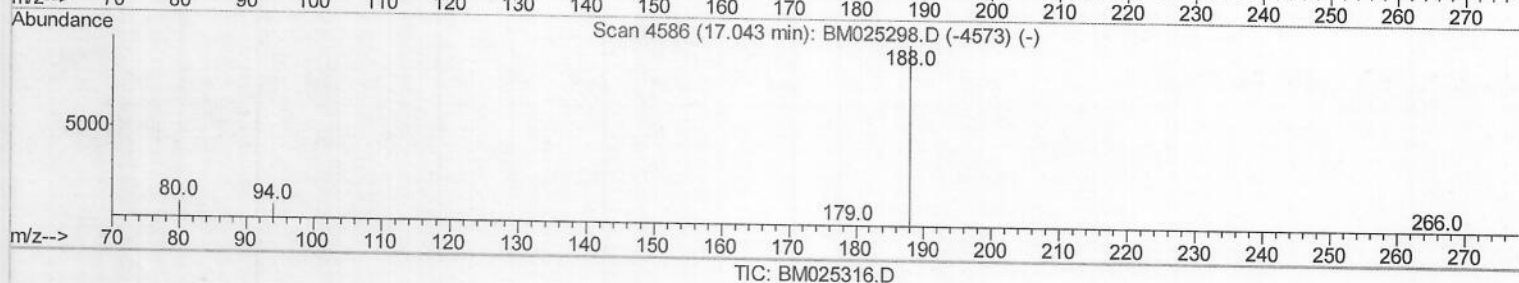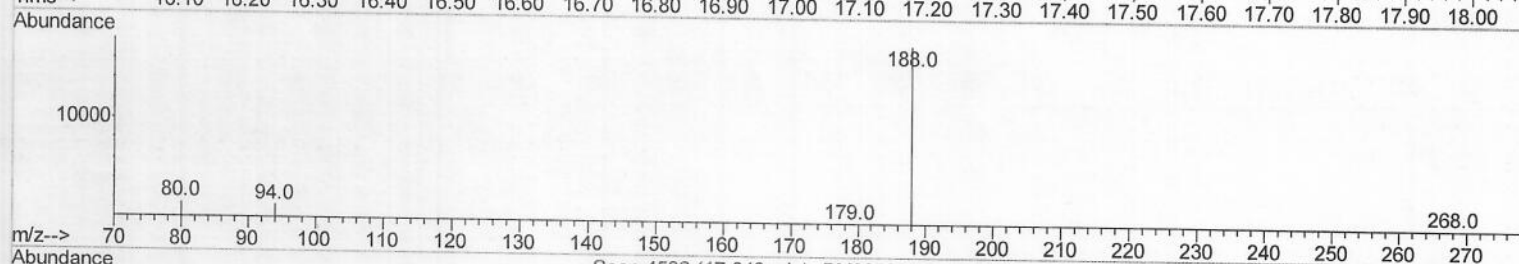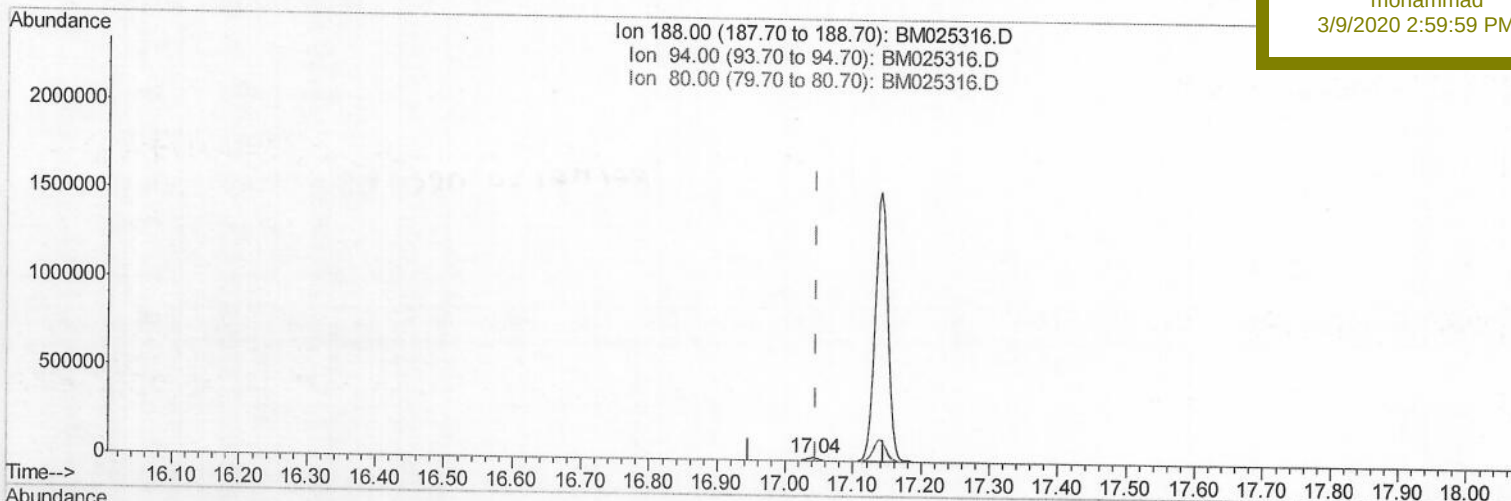

(10) Phenanthrene-d10 (I)

17.041min (-0.005) 0.40ng/ul m> Ju 03/11/20

response 24612

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.47#
80.00	22.60	8.77#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
 Data File : BM025316.D
 Acq On : 06 Mar 2020 15:21
 Operator : CG/JU
 Sample : PB127028BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK28

Manual Integrations
 APPROVED

mohammad
 3/9/2020 2:59:59 PM

Quant Time: Mar 06 16:14:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 04 08:02:03 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3207	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	13896	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	10458	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	24612m>	0.40	ng/ul	0.00
16) Chrysene-d12	21.23	240	23061	0.40	ng/ul	0.00
20) Perylene-d12	23.42	264	21488	0.40	ng/ul	0.00

JU 03/11/20

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	12.03	152	8566	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	24288	0.30	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed