


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025334.D
Acq On : 07 Mar 2020 05:06
Operator : CG/JU
Sample : L1612-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 07 05:57:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 00:01:42 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDM2

Manual Integrations
APPROVED

mohammad
3/9/2020 3:00:45 PM

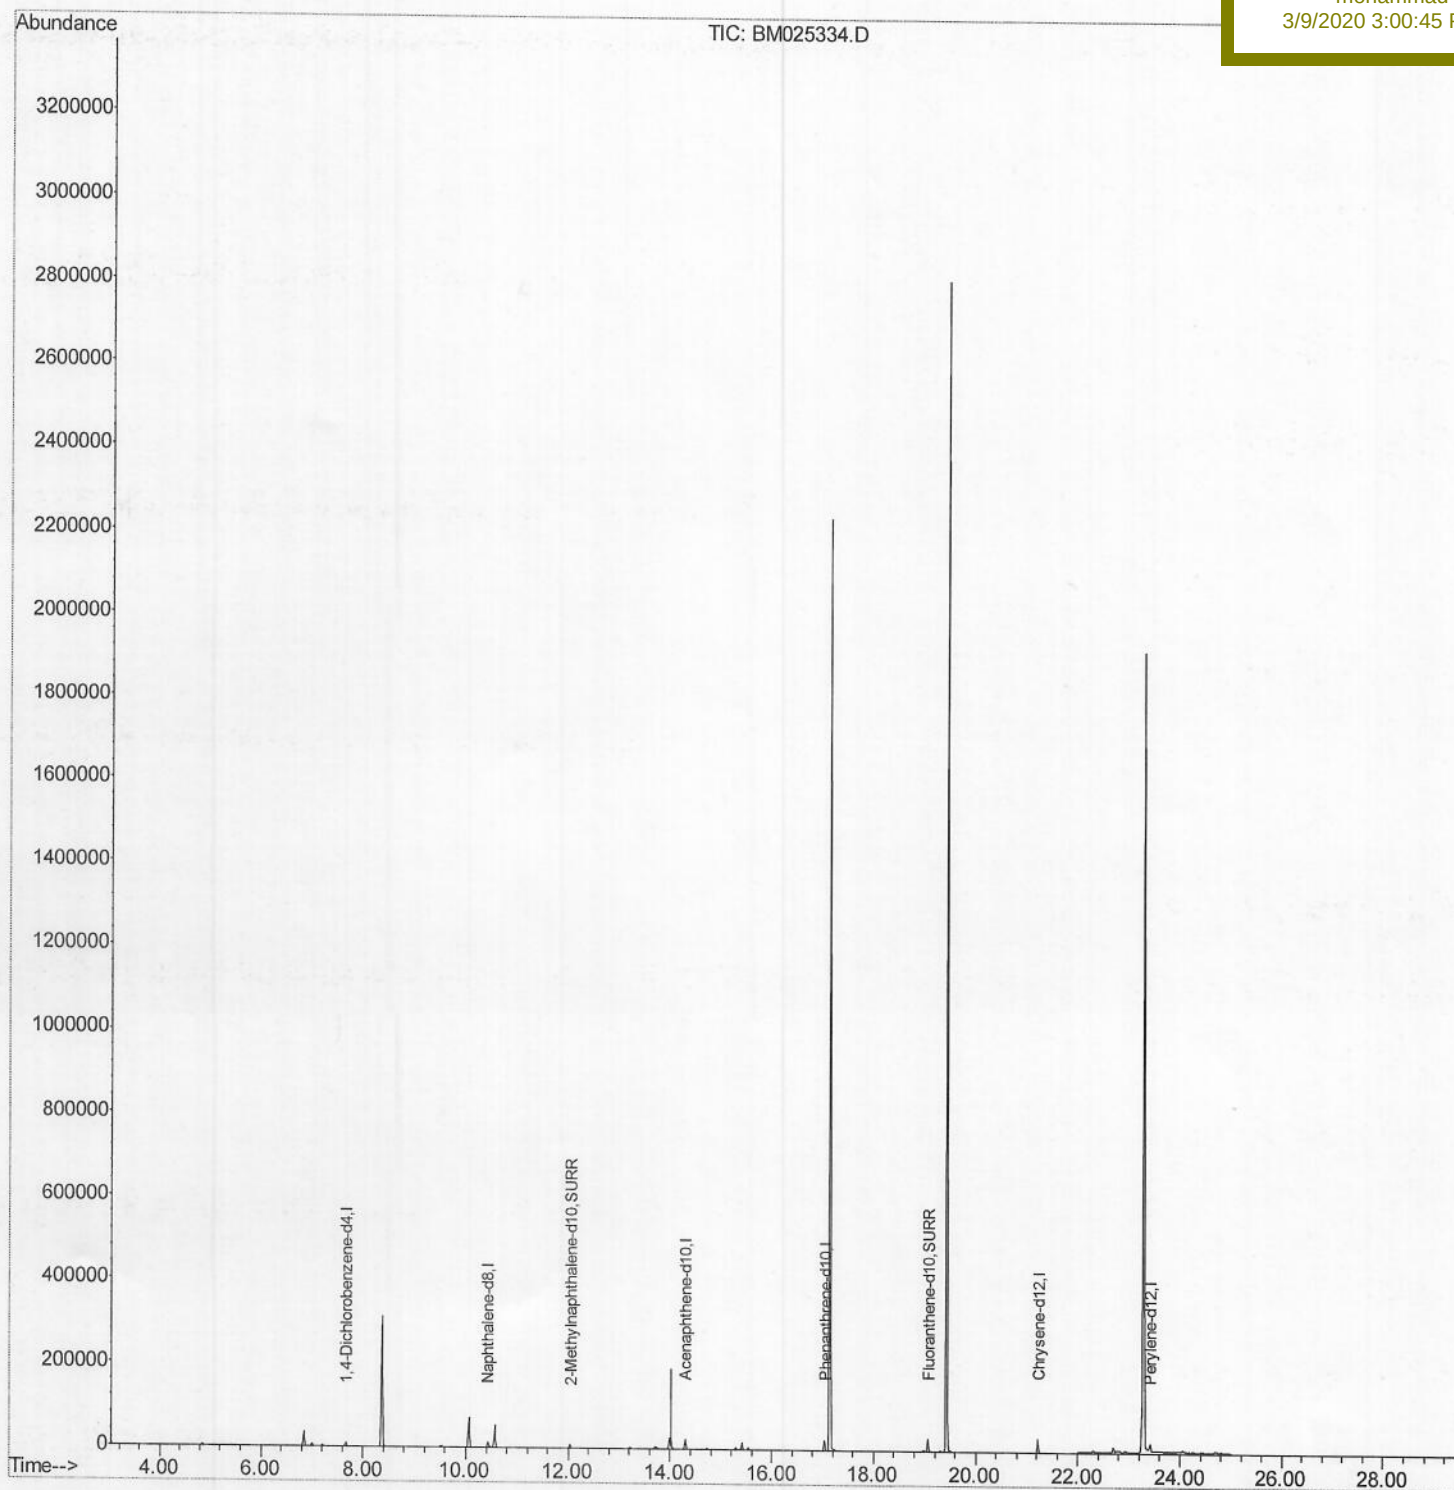

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\

Data File : BM025334.D

Acq On : 07 Mar 2020 05:06

Operator : CG/JU

Sample : L1612-20

Misc :

ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 07 05:56:11 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Mar 07 00:01:42 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBDM2

Manual Integrations

APPROVED

mohammad

3/9/2020 3:00:45 PM

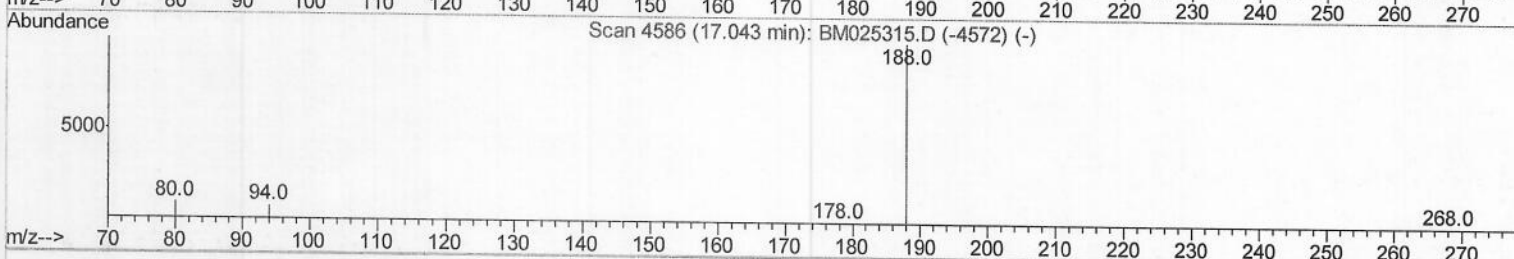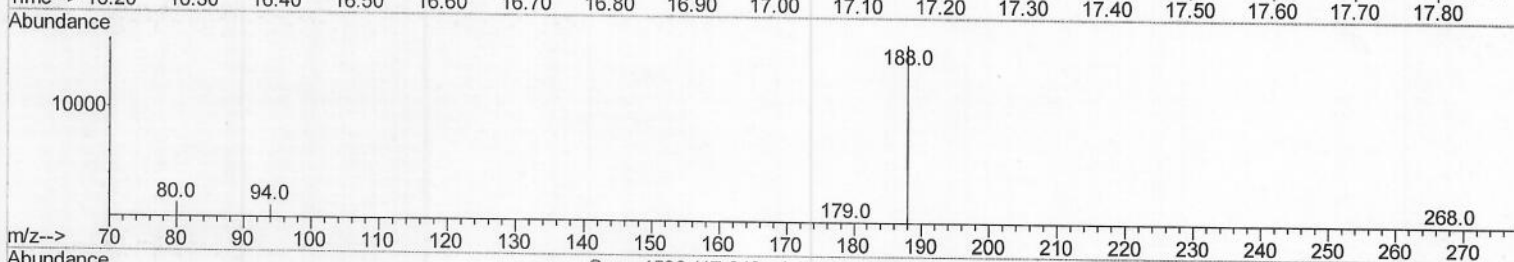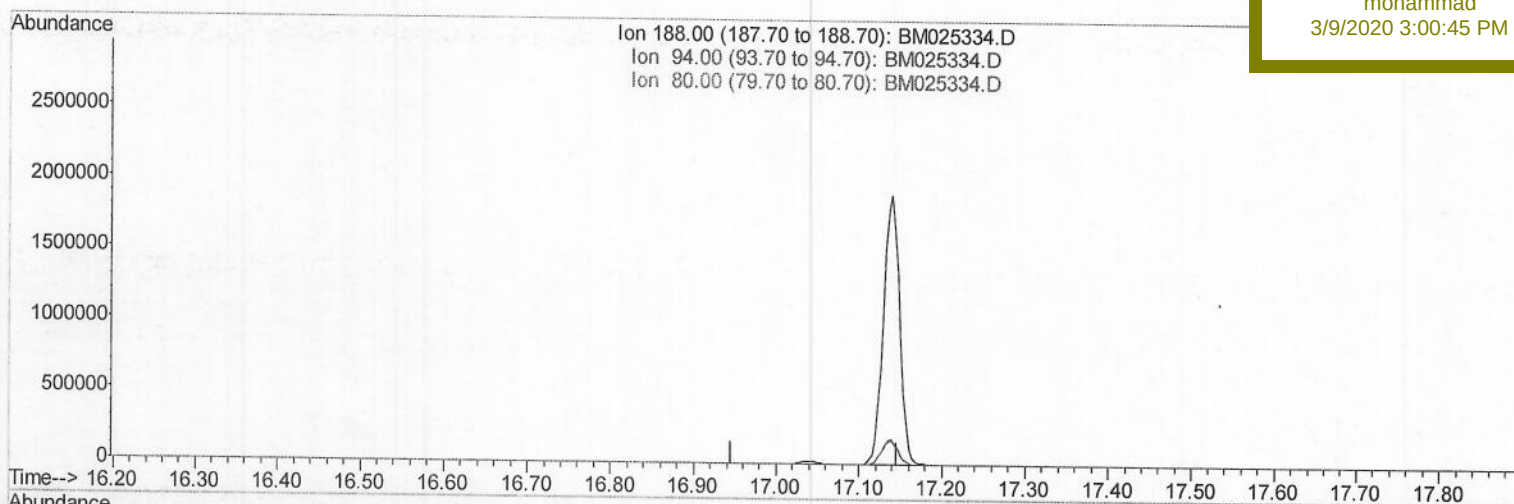

TIC: BM025334.D

(10) Phenanthrene-d10 (I)

17.046min (-17.046) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025334.D
Acq On : 07 Mar 2020 05:06
Operator : CG/JU
Sample : L1612-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 07 05:56:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 00:01:42 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleID :
DBDM2

Manual Integrations
APPROVED

mohammad
3/9/2020 3:00:45 PM

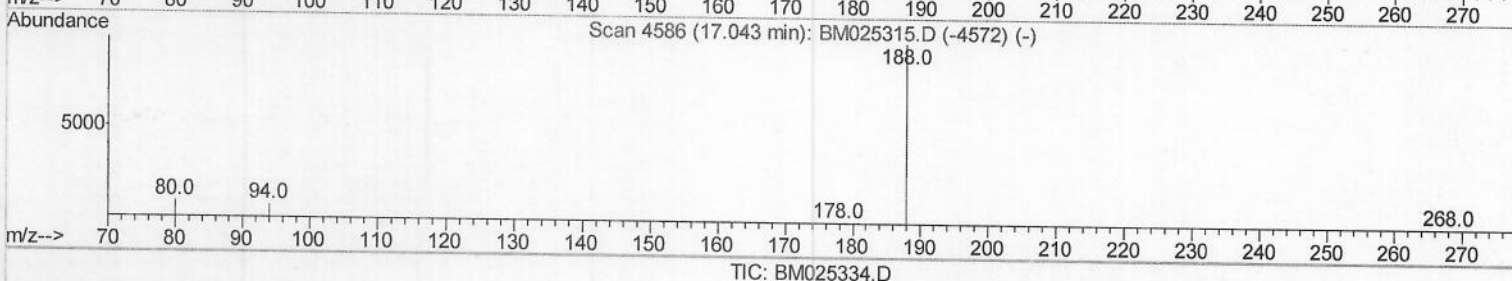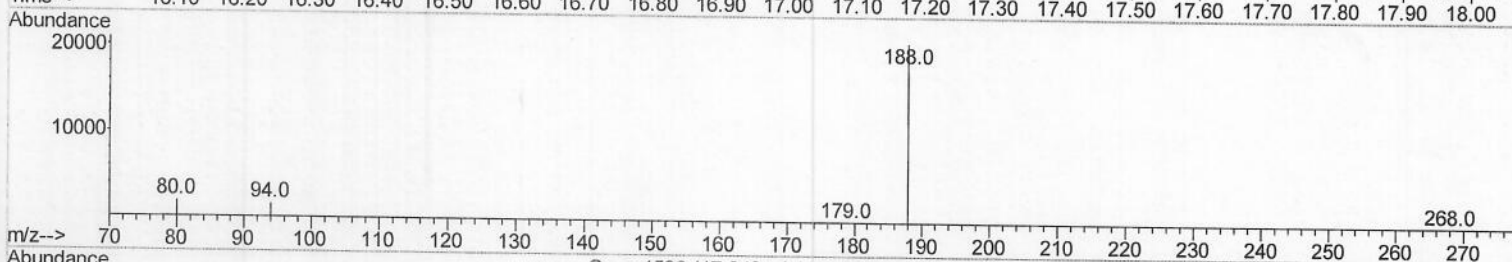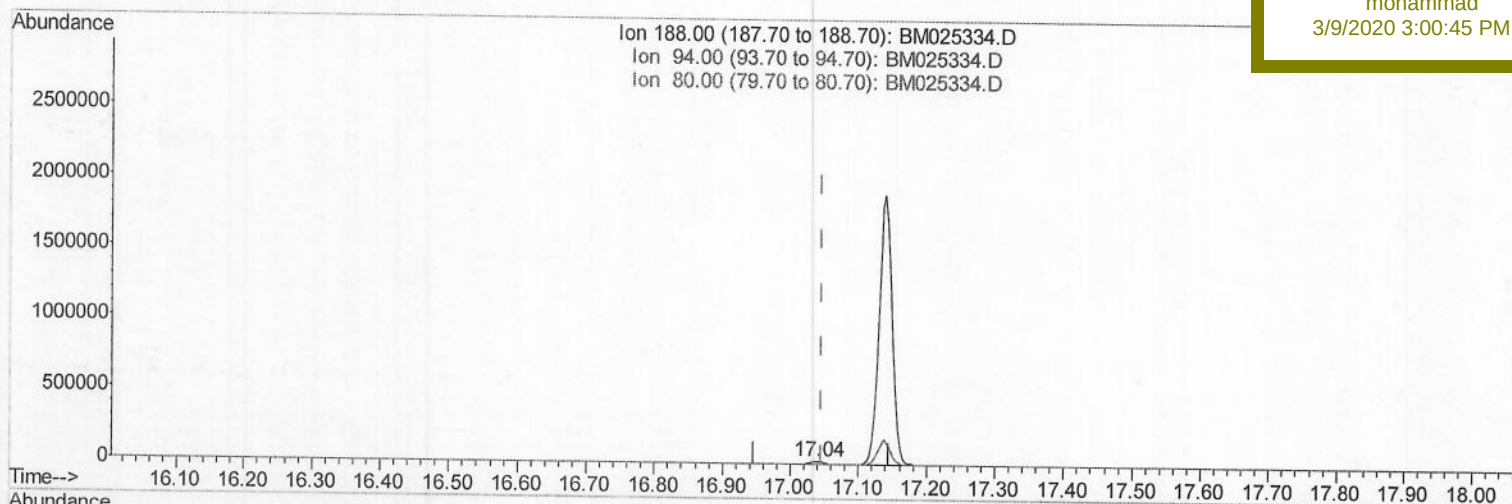

(10) Phenanthrene-d10 (I)

17.039min (-0.007) 0.40ng/ul m> JV 03/11/20

response 28317

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	8.12#
80.00	22.60	9.31#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025334.D
Acq On : 07 Mar 2020 05:06
Operator : CG/JU
Sample : L1612-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 07 05:57:39 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Mar 07 00:01:42 2020

Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :

DBDM2

Manual Integrations

APPROVED

mohammad

3/9/2020 3:00:45 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	3590	0.40	ng/ul	0.00
2) Naphthalene-d8	10.43	136	16024	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.30	164	12242	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.04	188	28317m	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	26619	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	23922	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	12.03	152	11351	0.38	ng/ul	0.00
14) Fluoranthene-d10	19.07	212	32678	0.35	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed