


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025350.D
Acq On : 07 Mar 2020 15:16
Operator : CG/JU
Sample : L1616-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 07 20:40:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
DBDQ7

Manual Integrations
APPROVED

mohammad
3/9/2020 3:01:39 PM

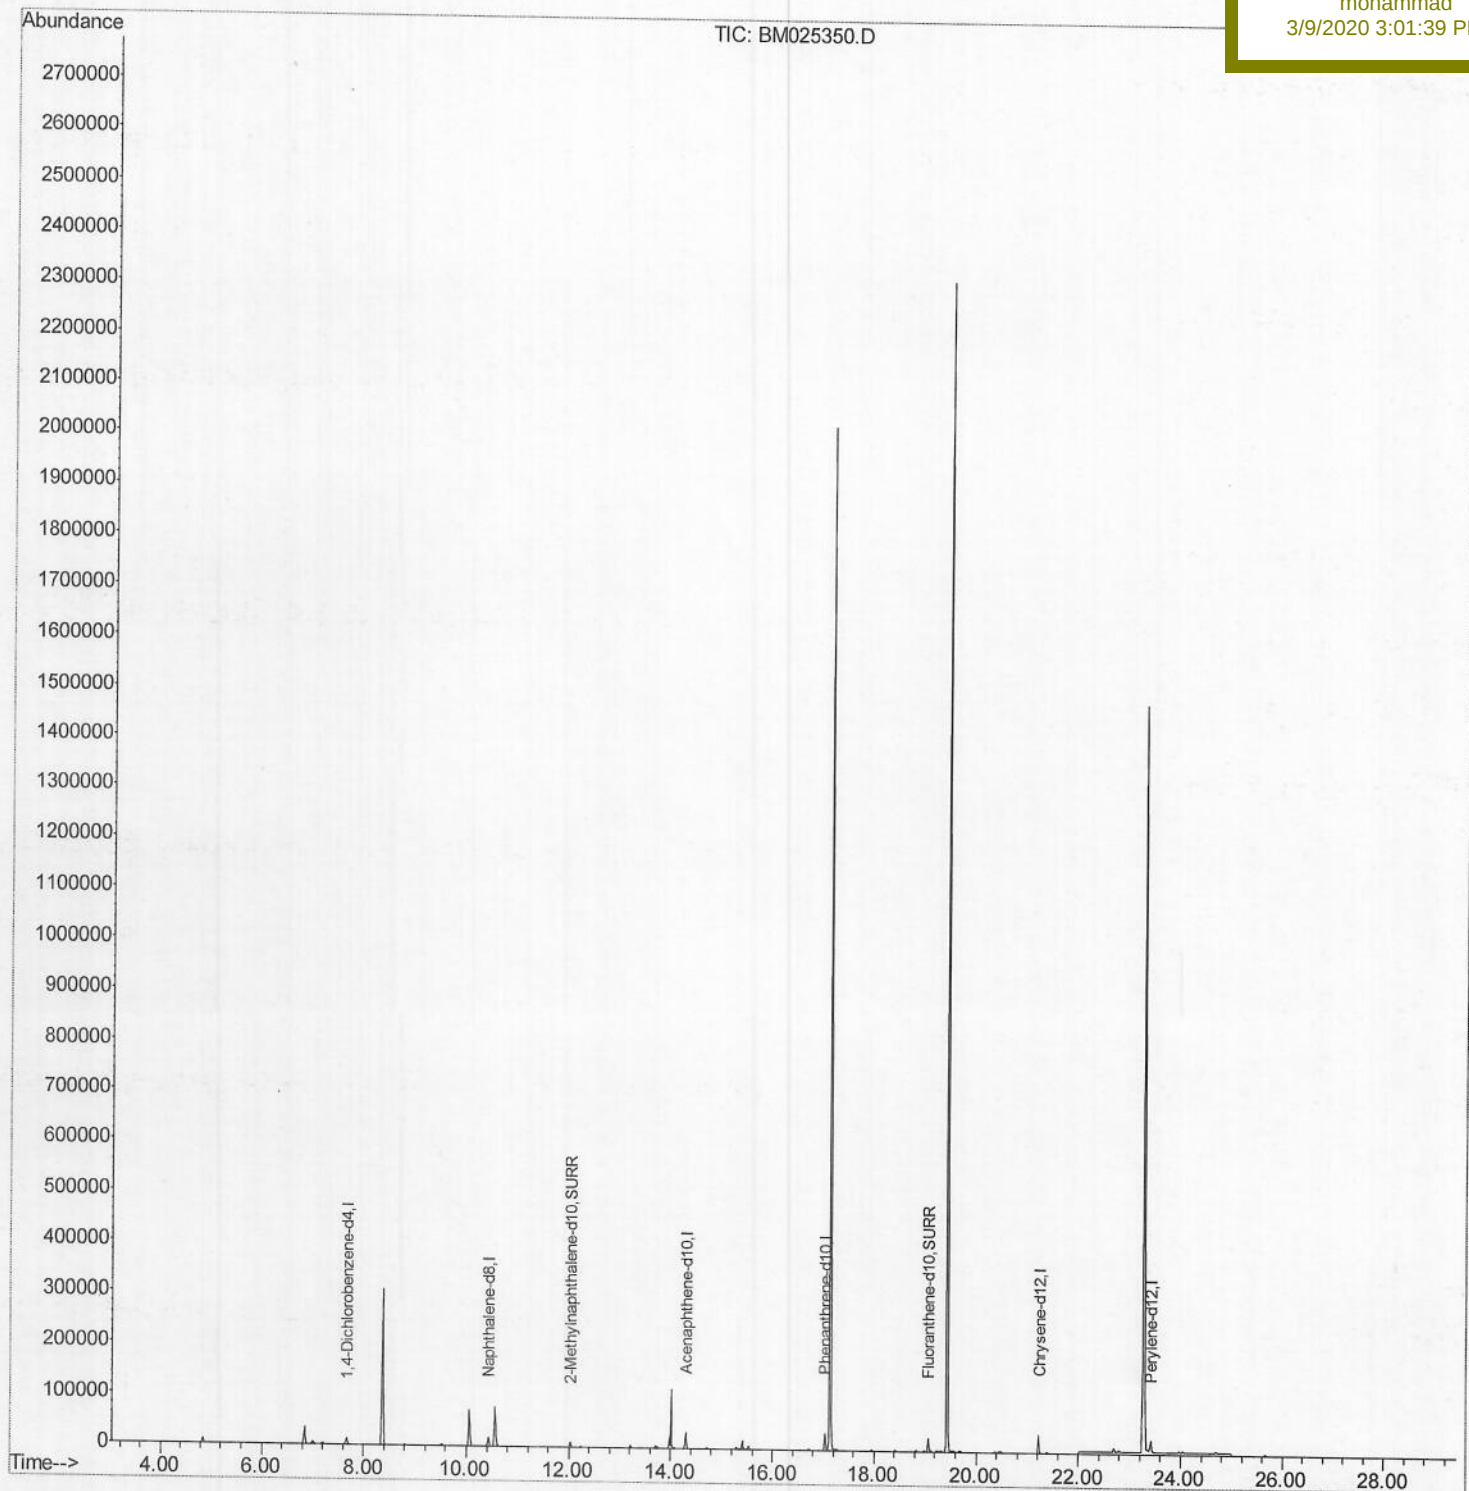

Quantitation Report (Qedit)




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
 Data File : BM025350.D
 Acq On : 07 Mar 2020 15:16
 Operator : CG/JU
 Sample : L1616-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 07 20:39:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 07 20:27:15 2020
 Response via : Initial Calibration

Instrument :
 BNA_M
ClientSampleId :
 DBDQ7

Manual Integrations
APPROVED

mohammad
 3/9/2020 3:01:39 PM

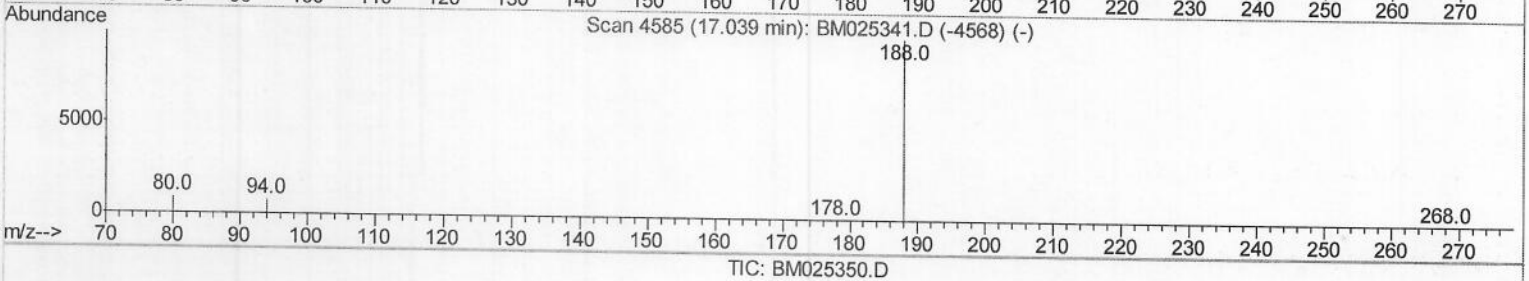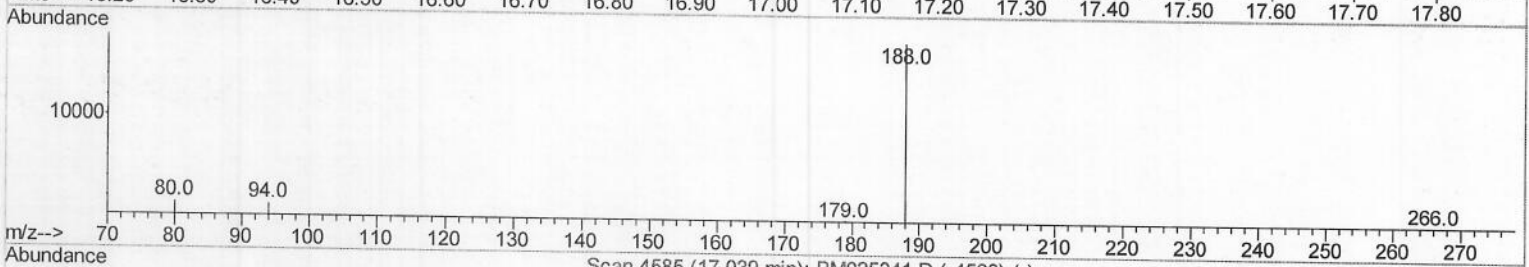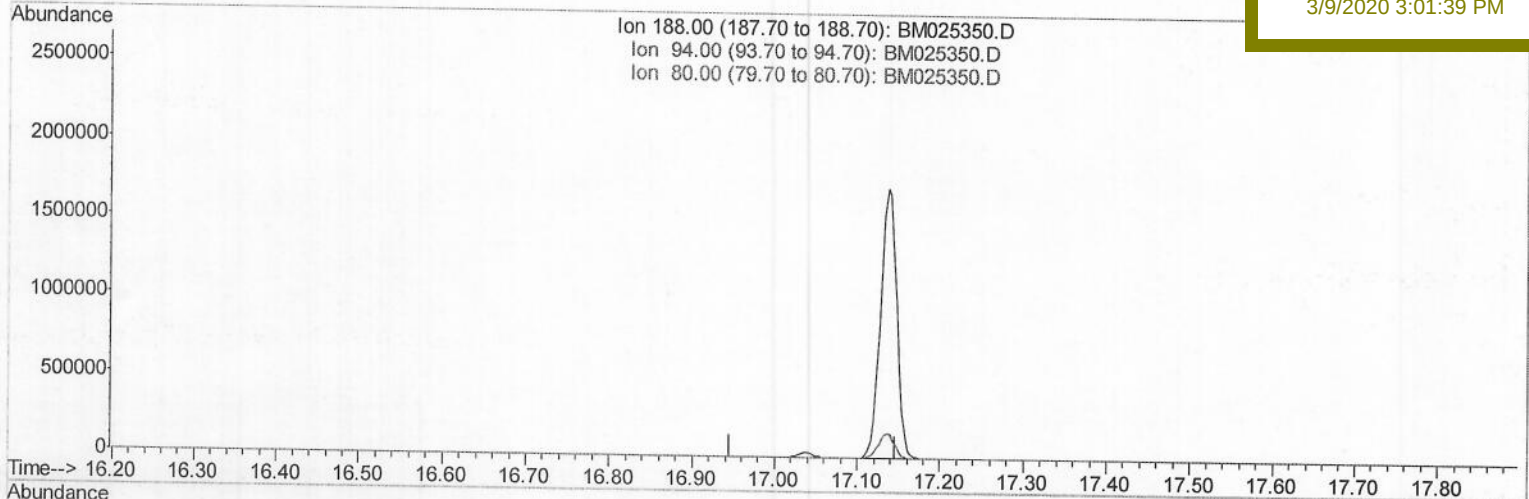

(10) Phenanthrene-d10 (I)
 17.046min (-17.046) 0.00ng/ul
 response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	26.60	0.00#
80.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\

Data File : BM025350.D

Acq On : 07 Mar 2020 15:16

Operator : CG/JU

Sample : L1616-13

Misc :

ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 07 20:39:44 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Sat Mar 07 20:27:15 2020

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




DBDQ7

Manual Integrations

APPROVED

mohammad

3/9/2020 3:01:39 PM

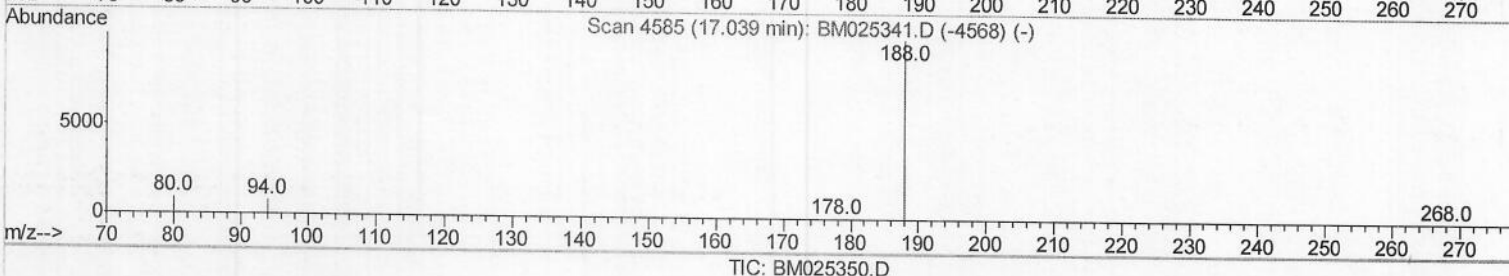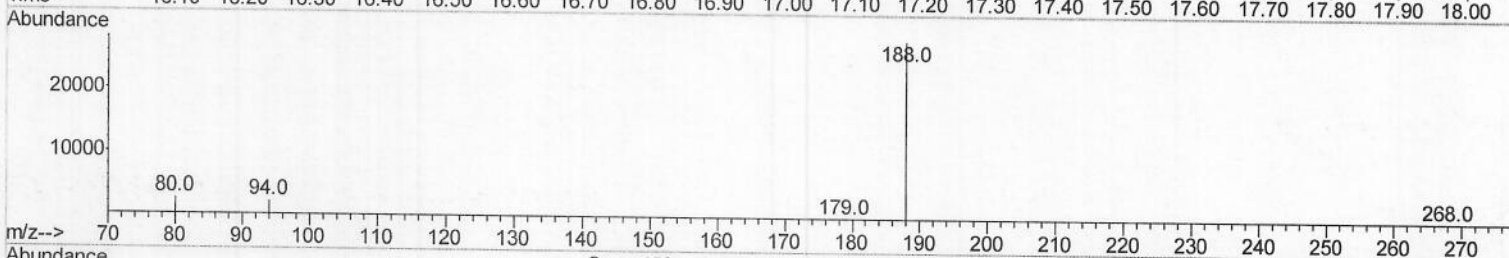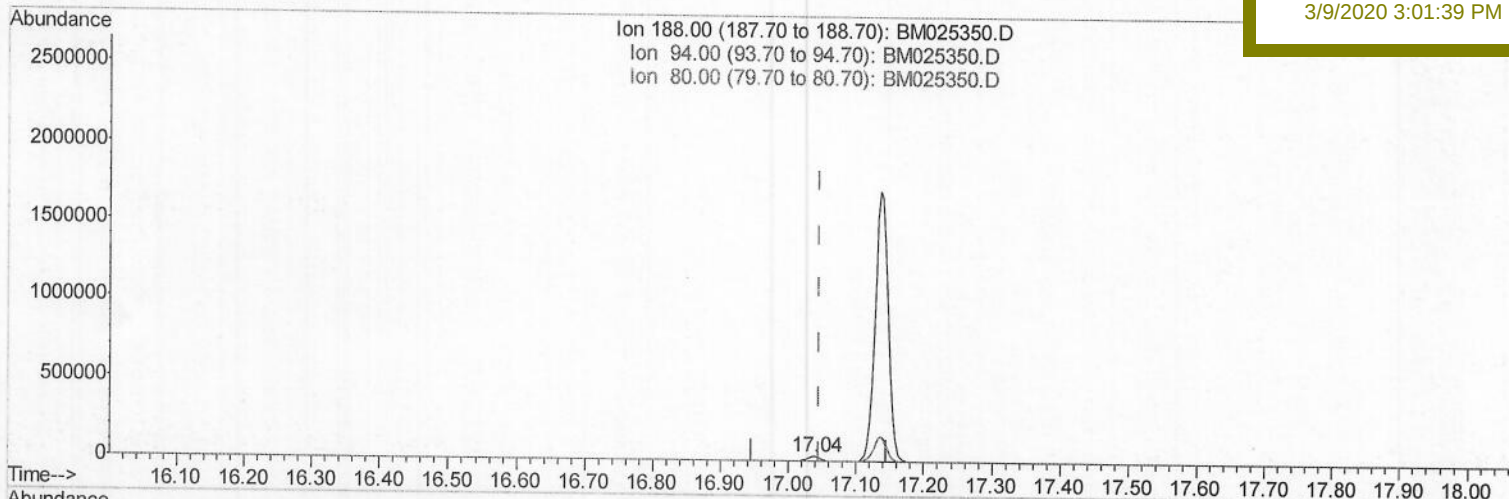

(10) Phenanthrene-d10 (I)

17.039min (-0.007) 0.40ng/ul m > 5v 03/11/20

response 38461

Ion	Exp%	Act%
188.00	100	100
94.00	26.60	7.98#
80.00	22.60	9.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030620\
Data File : BM025350.D
Acq On : 07 Mar 2020 15:16
Operator : CG/JU
Sample : L1616-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Quant Time: Mar 07 20:40:49 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030320.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 07 20:27:15 2020
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
DBDQ7

Manual Integrations
APPROVED

mohammad
3/9/2020 3:01:39 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.67	152	5173	0.40	ng/ul	0.00
2) Naphthalene-d8	10.44	136	23336	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.29	164	16876	0.40	ng/ul	-0.01
10) Phenanthrene-d10	17.04	188	38461m)	0.40	ng/ul	0.00
16) Chrysene-d12	21.22	240	32368	0.40	ng/ul	0.00
20) Perylene-d12	23.41	264	27753	0.40	ng/ul	-0.01
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.03	152	10944	0.25	ng/ul	-0.01
14) Fluoranthene-d10	19.07	212	29883	0.24	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

SV 03/11/20